

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030589.D
 Acq On : 17 Apr 2023 15:23
 Operator : SY/MD
 Sample : 02360-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP5

Quant Time: Apr 18 02:49:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	262595	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	253597	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	123550	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	87843	45.632	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.260%		
7) Chloroethane-d5	1.536	69	72787	45.121	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.240%		
11) 1,1-Dichloroethene-d2	2.066	65	41870	45.864	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.720%		
21) 2-Butanone-d5	3.802	46	95981	90.776	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.780%		
24) Chloroform-d	4.259	84	154754	44.360	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.720%		
26) 1,2-Dichloroethane-d4	4.950	65	106690	47.568	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.140%		
32) Benzene-d6	4.970	84	294234	49.074	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.140%		
36) 1,2-Dichloropropane-d6	5.998	67	89953	48.299	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.600%		
41) Toluene-d8	7.252	98	259393	46.078	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.160%		
43) trans-1,3-Dichloroprop...	7.561	79	43129	45.945	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.900%		
47) 2-Hexanone-d5	8.034	63	63813	86.976	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.980%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	119802	44.330	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.660%		
66) 1,2-Dichlorobenzene-d4	11.571	152	100621	51.238	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.480%		
Target Compounds					Qvalue	
13) Acetone	2.130	43	8639	5.280	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030589.D
Acq On : 17 Apr 2023 15:23
Operator : SY/MD
Sample : 02360-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP5

Quant Time: Apr 18 02:49:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 18 02:45:56 2023
Response via : Initial Calibration

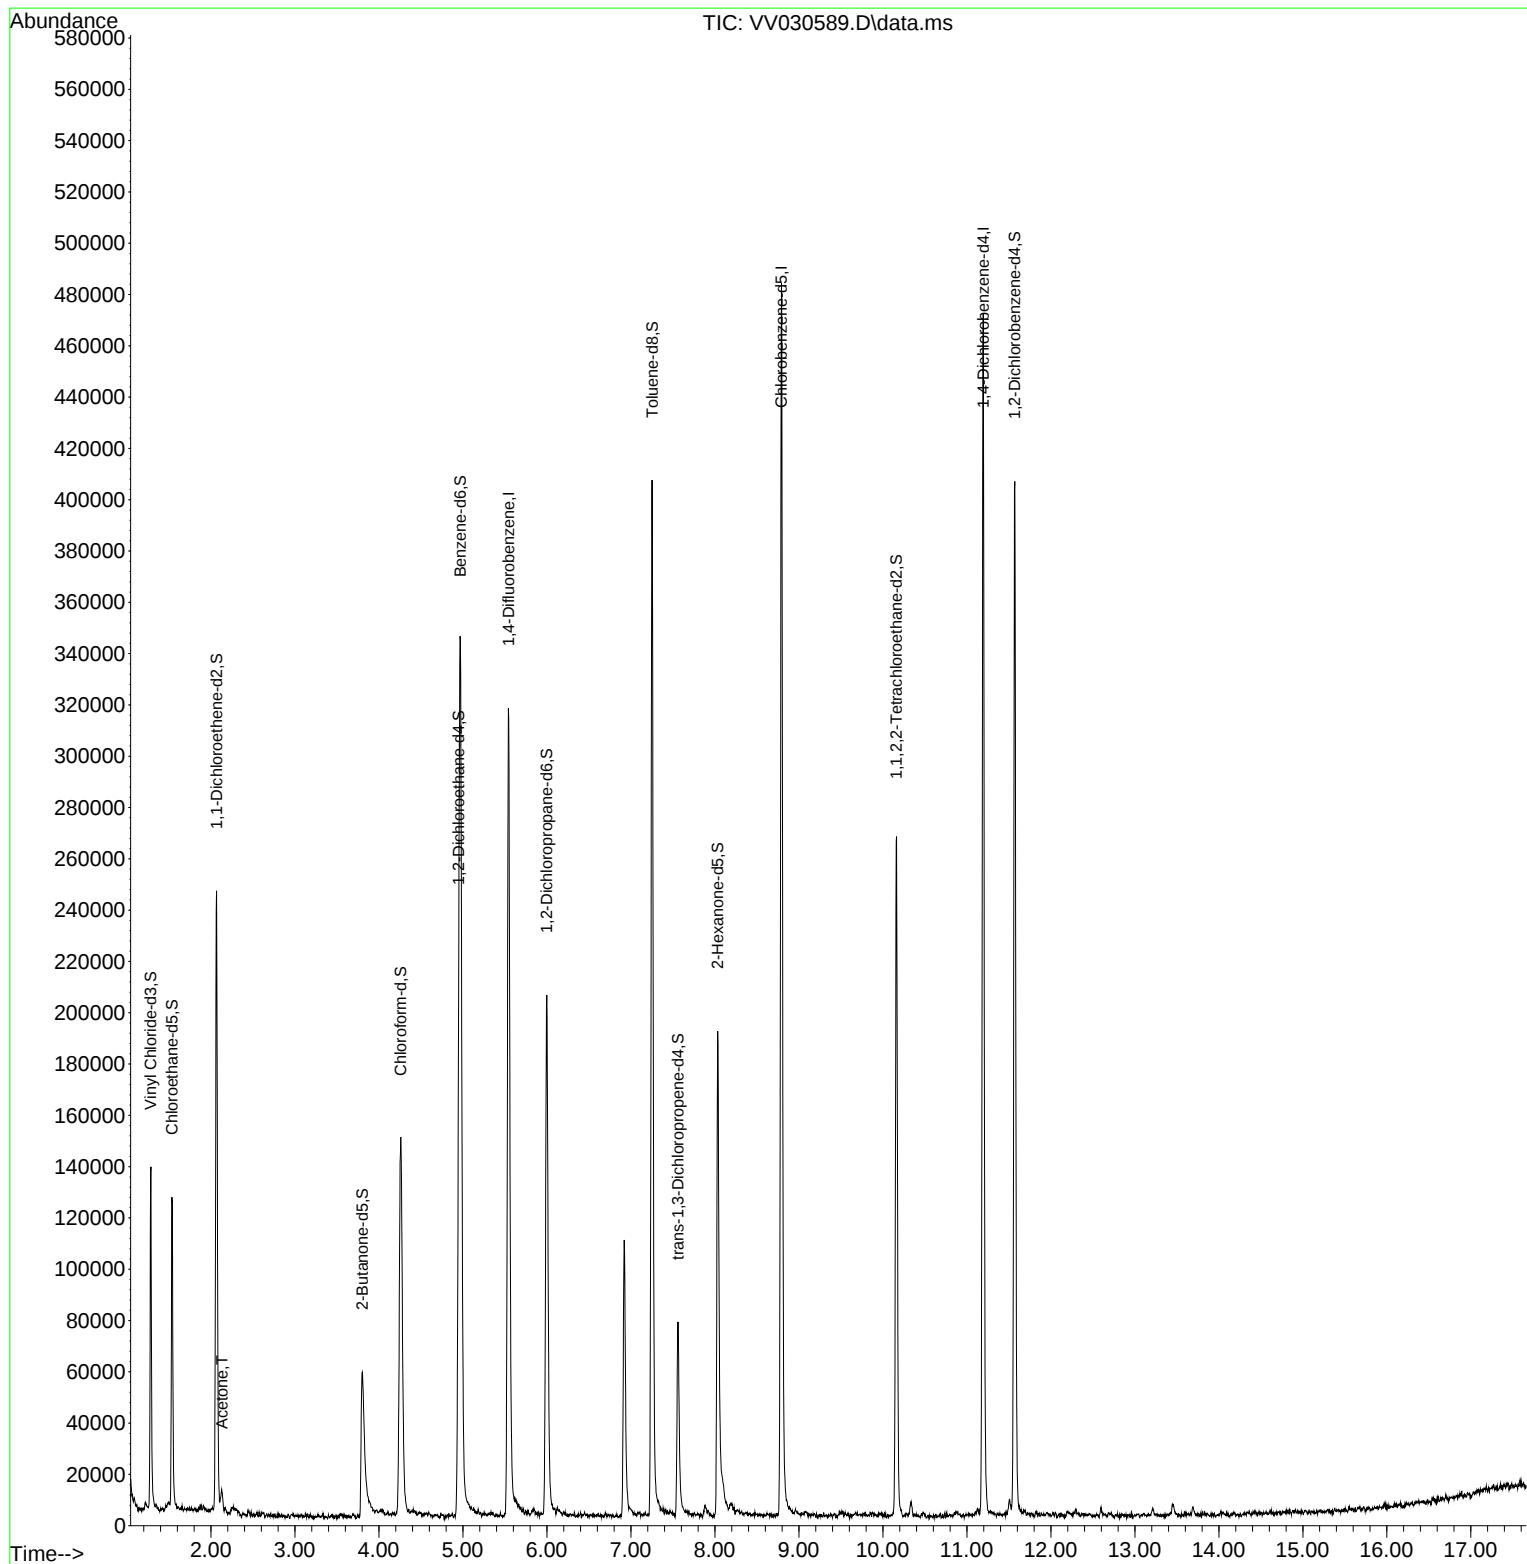

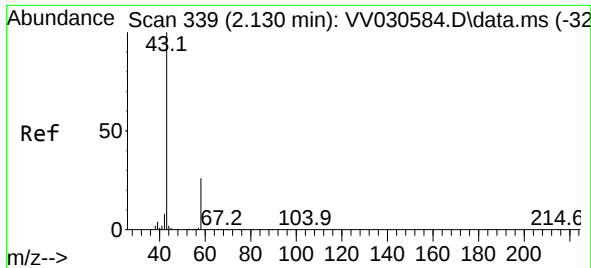

#13

Acetone

Concen: 5.280 ug/L

RT: 2.130 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV030589.D


Acq: 17 Apr 2023 15:23

Instrument :

MSVOA_V

ClientSampleId :

C0AP5

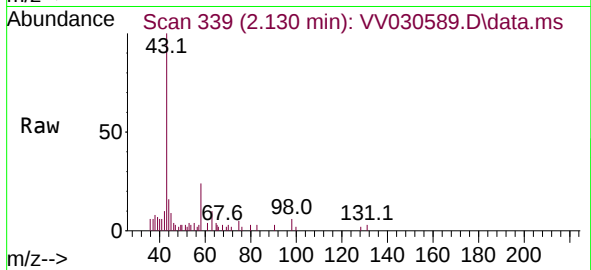

Tgt Ion: 43 Resp: 8639

Ion Ratio Lower Upper

43 100

58 27.8 0.0 52.8

