

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030608.D
 Acq On : 18 Apr 2023 00:42
 Operator : SY/MD
 Sample : VW0417WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK322

Quant Time: Apr 18 04:58:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	228617	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	215492	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	92298	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	80468	48.014	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	96.020%		
7) Chloroethane-d5	1.535	69	67530	48.083	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.160%		
11) 1,1-Dichloroethene-d2	2.063	65	38562	48.519	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.040%		
21) 2-Butanone-d5	3.799	46	89142	96.838	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.840%		
24) Chloroform-d	4.259	84	146519	48.241	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.480%		
26) 1,2-Dichloroethane-d4	4.950	65	99908	51.165	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.320%		
32) Benzene-d6	4.969	84	267212	52.448	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.900%		
36) 1,2-Dichloropropane-d6	5.998	67	86150	54.436	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	108.880%		
41) Toluene-d8	7.252	98	230678	48.223	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.440%		
43) trans-1,3-Dichloroprop...	7.561	79	37508	47.023	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.040%		
47) 2-Hexanone-d5	8.034	63	58775	94.275	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	94.270%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84	110489	48.114	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.220%		
66) 1,2-Dichlorobenzene-d4	11.570	152	83029	56.596	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	113.200%		
Target Compounds						Qvalue
3) Chloromethane	1.220	50	16163	6.269	ug/L	96
6) Bromomethane	1.490	94	2997	3.636	ug/L	93
34) Trichloroethene	5.844	95	10883	6.394	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030608.D
Acq On : 18 Apr 2023 00:42
Operator : SY/MD
Sample : VV0417WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK322

Quant Time: Apr 18 04:58:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 18 02:45:56 2023
Response via : Initial Calibration




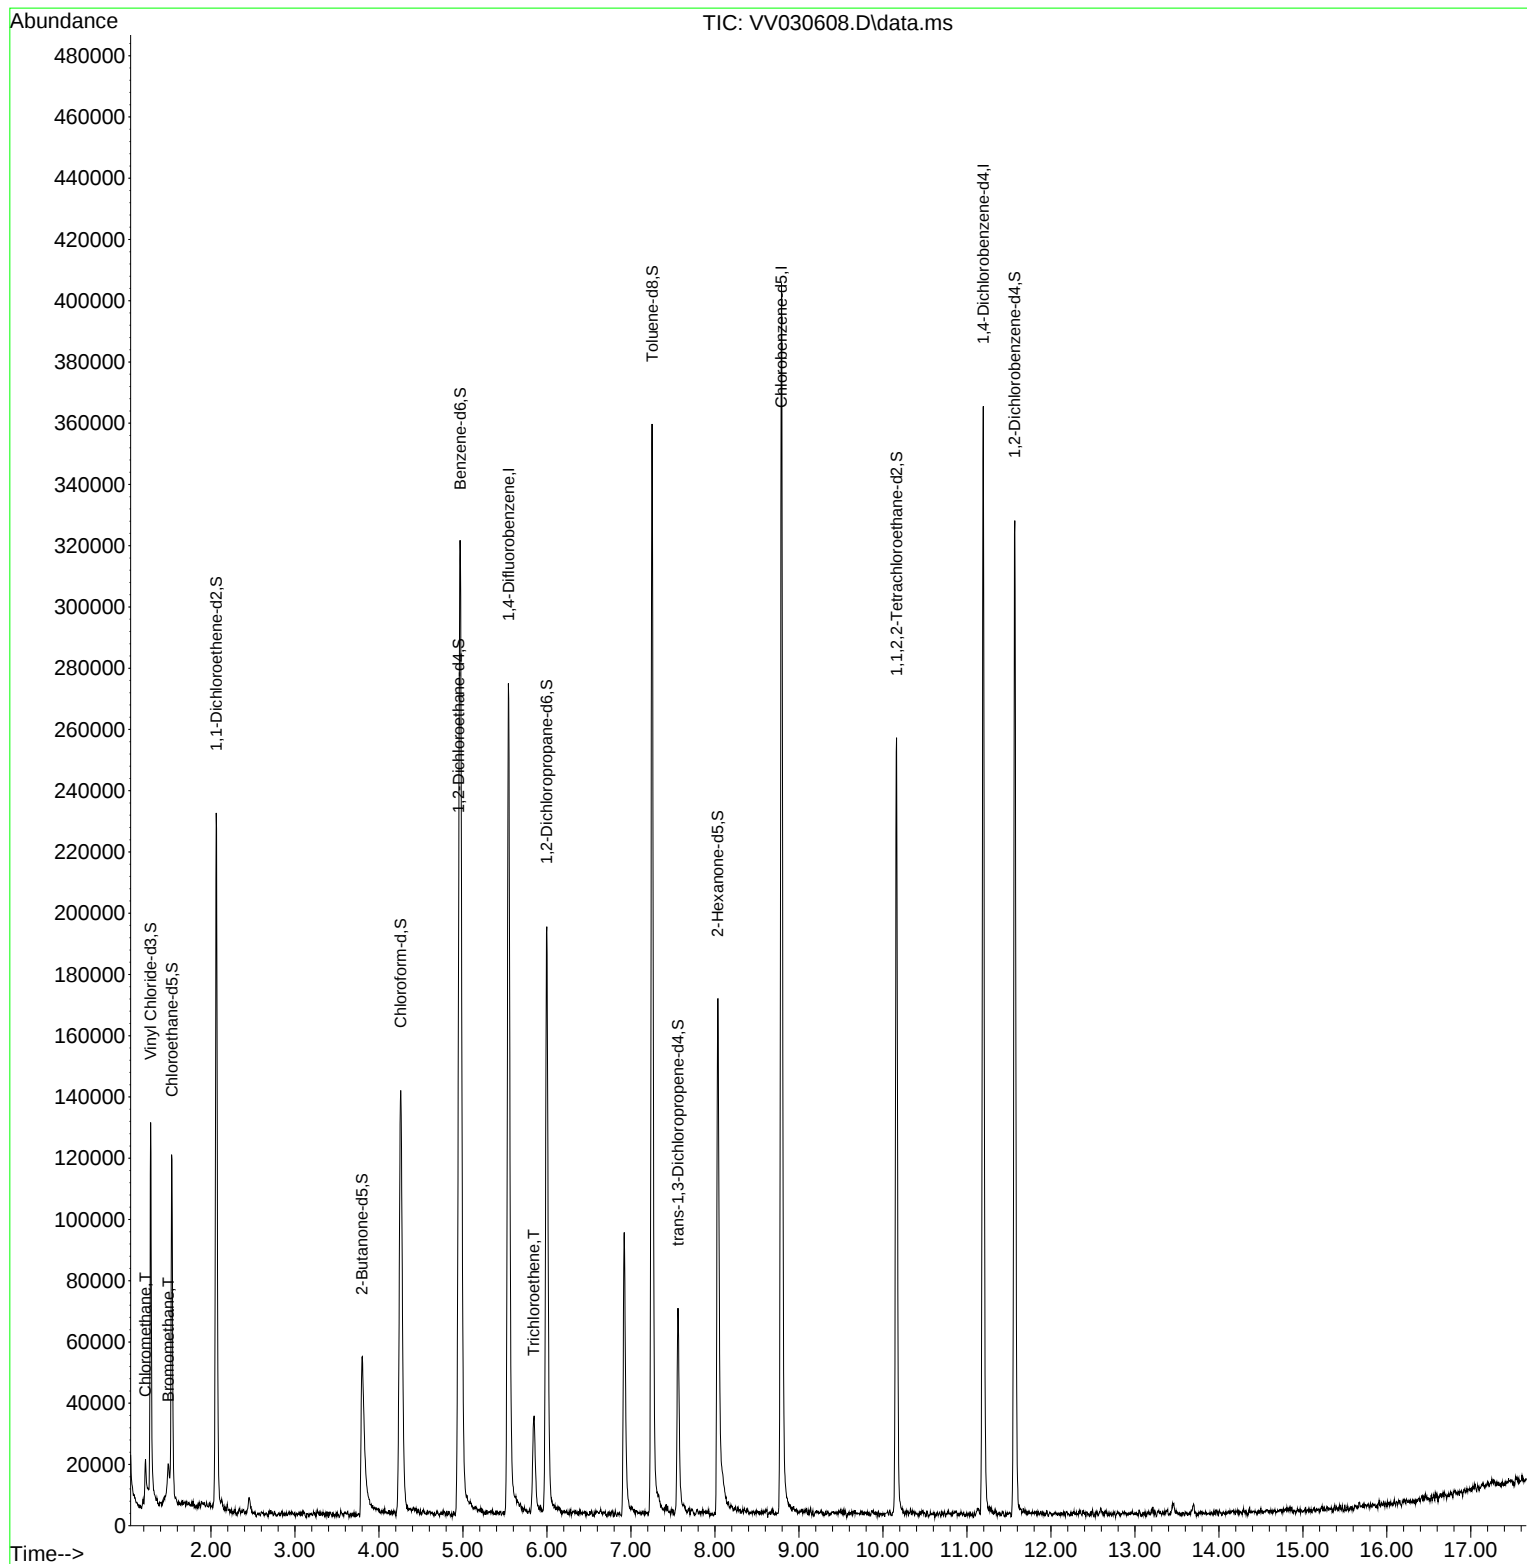


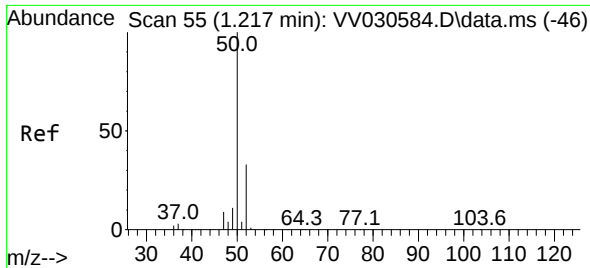

#3
Chloromethane
Concen: 6.269 ug/L
RT: 1.220 min Scan# 50
Delta R.T. 0.003 min
Lab File: VV030608.D
Acq: 18 Apr 2023 00:42




Instrument :
MSVOA_V
ClientSampleId :
VBLK322


Tgt Ion: 50 Resp: 16163
Ion Ratio Lower Upper
50 100
52 29.7 22.5 41.9

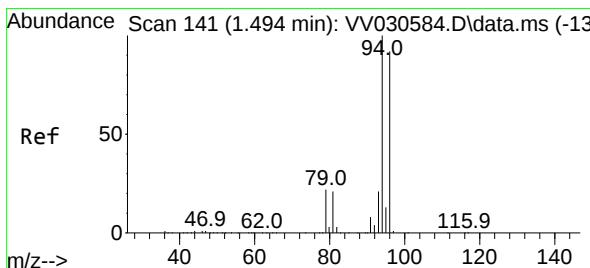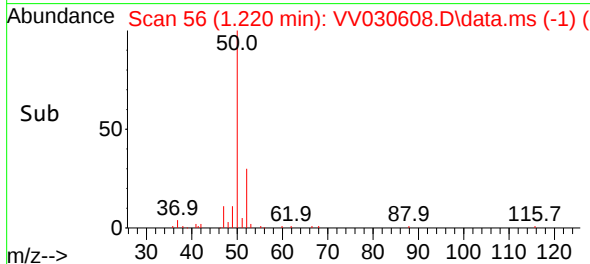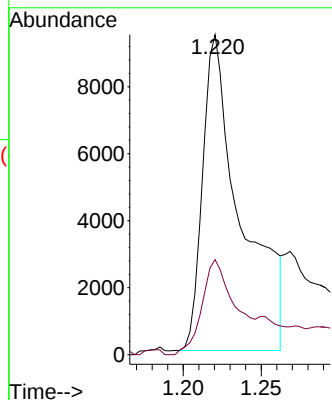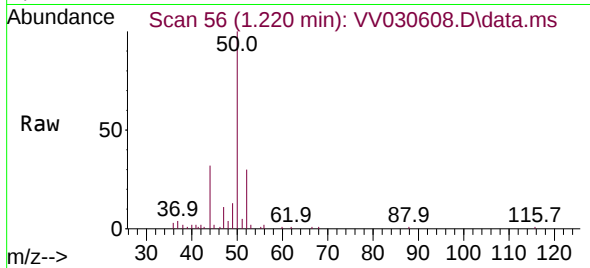

#6
Bromomethane
Concen: 3.636 ug/L
RT: 1.490 min Scan# 140
Delta R.T. -0.003 min
Lab File: VV030608.D
Acq: 18 Apr 2023 00:42


Tgt Ion: 94 Resp: 2997
Ion Ratio Lower Upper
94 100
96 101.4 66.3 123.1

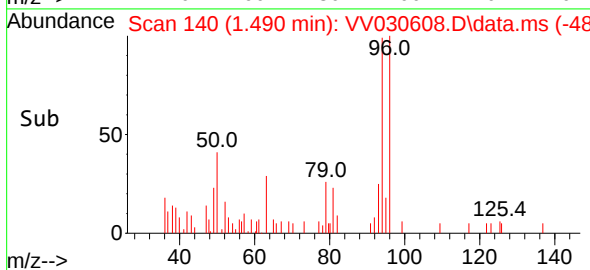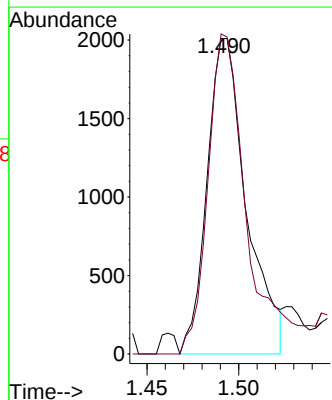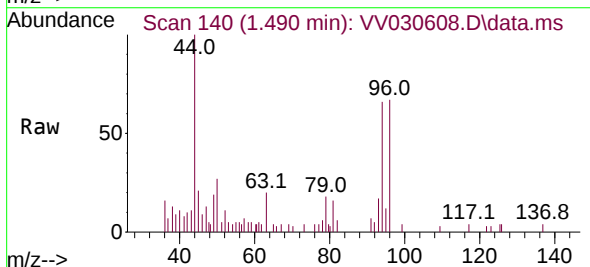

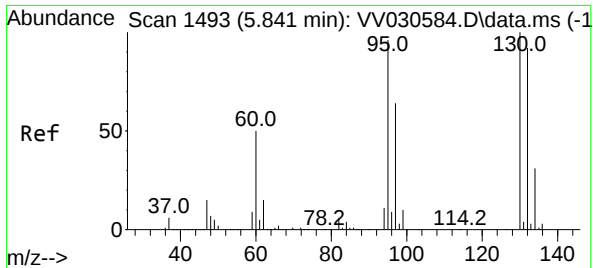

#34
 Trichloroethene
 Concen: 6.394 ug/L
 RT: 5.844 min Scan# 1494
 Delta R.T. 0.003 min
 Lab File: VV030608.D
 Acq: 18 Apr 2023 00:42

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK322

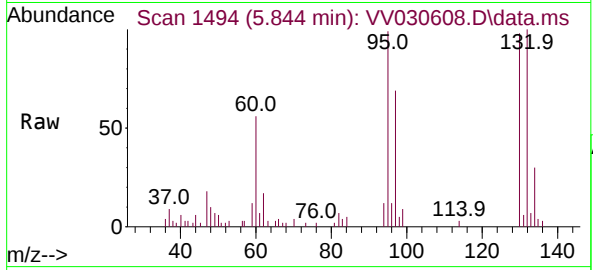

Tgt Ion: 95 Resp: 10883

Ion	Ratio	Lower	Upper
95	100		
97	69.2	45.8	85.2
132	100.8	70.6	131.2
130	98.8	70.9	131.7

