

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030585.D
 Acq On : 17 Apr 2023 13:49
 Operator : SY/MD
 Sample : VV0417MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK320

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030585.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rVB	129285	142852	15.50%	1.927%
2	1.539	148	155	170	rVB	120444	142252	15.44%	1.919%
3	2.066	310	319	332	rBV	245667	354509	38.47%	4.783%
4	2.330	399	401	403	rBV3	1226	628	0.07%	0.008%
5	2.455	431	440	451	rBV4	7883	15235	1.65%	0.206%
6	2.883	572	573	576	rBV3	1182	744	0.08%	0.010%
7	2.950	591	594	597	rBV5	1231	638	0.07%	0.009%
8	2.969	598	600	606	rVB5	2176	1426	0.15%	0.019%
9	3.214	674	676	681	rVB4	2021	1347	0.15%	0.018%
10	3.320	706	709	711	rBV3	1125	620	0.07%	0.008%
11	3.362	718	722	723	rBV4	1256	961	0.10%	0.013%
12	3.426	739	742	745	rBV4	1155	814	0.09%	0.011%
13	3.477	755	758	764	rBV7	1472	1591	0.17%	0.021%
14	3.519	768	771	773	rBV4	1274	944	0.10%	0.013%
15	3.555	778	782	784	rBV5	1247	993	0.11%	0.013%
16	3.635	804	807	812	rBV6	1539	1319	0.14%	0.018%
17	3.719	830	833	835	rVB4	1284	642	0.07%	0.009%
18	3.802	849	859	881	rBV	56986	164284	17.83%	2.216%
19	4.262	989	1002	1026	rVB2	144760	367976	39.93%	4.964%
20	4.477	1066	1069	1075	rVB7	2030	1651	0.18%	0.022%
21	4.567	1095	1097	1101	rVB5	1167	837	0.09%	0.011%
22	4.661	1124	1126	1127	rBV	1197	566	0.06%	0.008%
23	4.818	1172	1175	1176	rBV3	1173	697	0.08%	0.009%
24	4.892	1194	1198	1199	rBV4	912	576	0.06%	0.008%
25	4.969	1204	1222	1242	rBV3	348005	921495	100.00%	12.432%
26	5.378	1346	1349	1352	rBV5	889	810	0.09%	0.011%
27	5.545	1388	1401	1422	rBV	328631	673914	73.13%	9.092%
28	5.998	1531	1542	1563	rBV	202701	403865	43.83%	5.449%
29	6.198	1601	1604	1606	rBV4	1537	865	0.09%	0.012%
30	6.265	1623	1625	1631	rVB6	1801	1130	0.12%	0.015%
31	6.400	1665	1667	1670	rBV4	1263	912	0.10%	0.012%
32	6.529	1705	1707	1713	rBV6	1538	1454	0.16%	0.020%
33	6.731	1768	1770	1773	rBV3	1346	728	0.08%	0.010%
34	6.786	1784	1787	1789	rBV4	1852	1161	0.13%	0.016%
35	6.799	1789	1791	1795	rVB5	1954	1244	0.13%	0.017%
36	6.831	1799	1801	1802	rBV	1305	623	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030585.D
 Acq On : 17 Apr 2023 13:49
 Operator : SY/MD
 Sample : VW0417MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK320

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1819	1829	1848	rVV2	106264	198997	21.60%	2.685%
38	7.252	1920	1932	1950	rBV	404614	708283	76.86%	9.555%
39	7.561	2018	2028	2042	rBV	77123	139889	15.18%	1.887%
40	8.034	2165	2175	2201	rBV	190761	373160	40.50%	5.034%
41	8.284	2250	2253	2257	rVV5	1662	1293	0.14%	0.017%
42	8.622	2355	2358	2361	rVB6	1781	1213	0.13%	0.016%
43	8.641	2361	2364	2366	rBV3	876	632	0.07%	0.009%
44	8.747	2395	2397	2398	rBV	1387	642	0.07%	0.009%
45	8.792	2400	2411	2441	rVV	501302	838956	91.04%	11.318%
46	9.005	2474	2477	2478	rBV3	1568	1020	0.11%	0.014%
47	9.162	2524	2526	2529	rVB4	2175	760	0.08%	0.010%
48	9.333	2576	2579	2581	rBV3	1681	837	0.09%	0.011%
49	9.378	2590	2593	2596	rBV3	1269	907	0.10%	0.012%
50	9.407	2599	2602	2606	rVV5	1920	1348	0.15%	0.018%
51	9.435	2609	2611	2614	rVB4	1717	813	0.09%	0.011%
52	9.596	2656	2661	2664	rBV7	1673	1261	0.14%	0.017%
53	9.612	2664	2666	2668	rBV2	935	616	0.07%	0.008%
54	9.754	2707	2710	2712	rBV4	1126	763	0.08%	0.010%
55	9.770	2712	2715	2719	rVV6	1289	1151	0.12%	0.016%
56	9.808	2726	2727	2731	rVB4	1377	618	0.07%	0.008%
57	9.834	2731	2735	2737	rBV5	1370	951	0.10%	0.013%
58	10.098	2815	2817	2819	rBV3	1755	864	0.09%	0.012%
59	10.162	2823	2837	2851	rBV	262115	422120	45.81%	5.695%
60	10.265	2867	2869	2871	rBV2	1295	564	0.06%	0.008%
61	10.284	2873	2875	2878	rBV4	859	580	0.06%	0.008%
62	10.358	2895	2898	2900	rBV3	2554	1666	0.18%	0.022%
63	10.406	2911	2913	2917	rBV5	820	722	0.08%	0.010%
64	10.439	2921	2923	2926	rBV3	1599	838	0.09%	0.011%
65	10.474	2931	2934	2935	rBV2	2171	1286	0.14%	0.017%
66	10.522	2948	2949	2952	rBV3	1284	814	0.09%	0.011%
67	10.712	3005	3008	3010	rBV3	1056	751	0.08%	0.010%
68	10.841	3045	3048	3049	rBV3	1303	627	0.07%	0.008%
69	11.091	3124	3126	3130	rBV4	1121	886	0.10%	0.012%
70	11.127	3130	3137	3138	rBV7	2786	2660	0.29%	0.036%
71	11.194	3146	3158	3177	rBV	491115	783515	85.03%	10.570%
72	11.339	3200	3203	3209	rVB8	2133	1692	0.18%	0.023%
73	11.471	3238	3244	3248	rVB8	1711	2111	0.23%	0.028%
74	11.570	3262	3275	3290	rBV	405540	652227	70.78%	8.799%
75	11.799	3344	3346	3350	rBV5	1615	1367	0.15%	0.018%
76	11.898	3373	3377	3379	rBV5	1364	1147	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030585.D
 Acq On : 17 Apr 2023 13:49
 Operator : SY/MD
 Sample : VV0417MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK320

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.033	3414	3419	3422	rBV6	1243	1323	0.14%	0.018%
78	12.104	3439	3441	3445	rBV3	1649	863	0.09%	0.012%
79	12.181	3460	3465	3469	rBV6	1911	1805	0.20%	0.024%
80	12.236	3480	3482	3487	rVB6	1123	849	0.09%	0.011%
81	12.284	3493	3497	3499	rVB5	1161	746	0.08%	0.010%
82	12.307	3499	3504	3506	rBV4	1277	1181	0.13%	0.016%
83	12.461	3549	3552	3554	rBV4	1983	1140	0.12%	0.015%
84	12.596	3585	3594	3599	rBV10	5531	8693	0.94%	0.117%
85	12.664	3610	3615	3617	rBV5	1377	1241	0.13%	0.017%
86	12.821	3663	3664	3666	rBV2	1126	576	0.06%	0.008%
87	13.024	3725	3727	3730	rVB4	1455	739	0.08%	0.010%
88	13.146	3762	3765	3767	rBV4	1231	754	0.08%	0.010%
89	13.181	3772	3776	3777	rBV4	1225	930	0.10%	0.013%
90	13.323	3815	3820	3826	rBV8	2018	1970	0.21%	0.027%
91	13.455	3853	3861	3868	rBV2	11422	17475	1.90%	0.236%
92	13.541	3886	3888	3892	rVB5	1700	1046	0.11%	0.014%
93	13.805	3968	3970	3973	rBV3	1208	773	0.08%	0.010%
94	13.856	3982	3986	3988	rVB4	1623	1237	0.13%	0.017%
95	14.094	4057	4060	4062	rBV4	2609	1586	0.17%	0.021%
96	14.361	4142	4143	4145	rBV2	1184	571	0.06%	0.008%
97	14.458	4170	4173	4175	rBV3	1250	841	0.09%	0.011%
98	14.734	4257	4259	4262	rBV4	1610	1093	0.12%	0.015%
99	14.885	4304	4306	4308	rBV3	1804	843	0.09%	0.011%
100	15.024	4347	4349	4351	rBV2	1866	1198	0.13%	0.016%




Sum of corrected areas: 7412323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030585.D
Acq On : 17 Apr 2023 13:49
Operator : SY/MD
Sample : VV0417MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

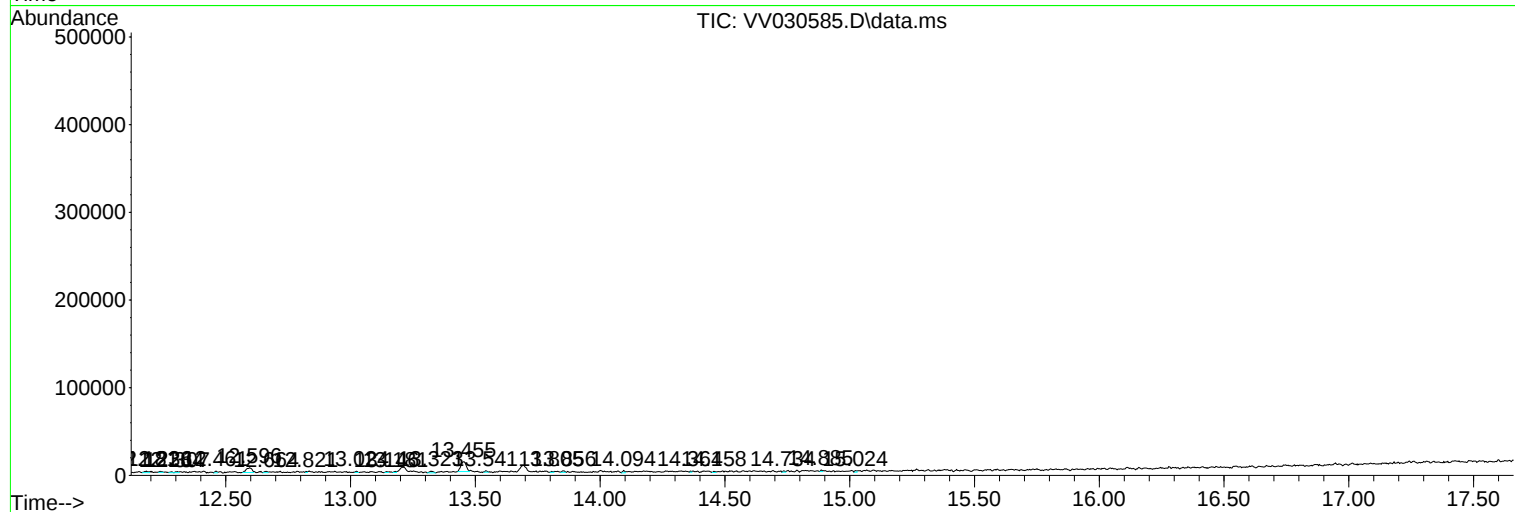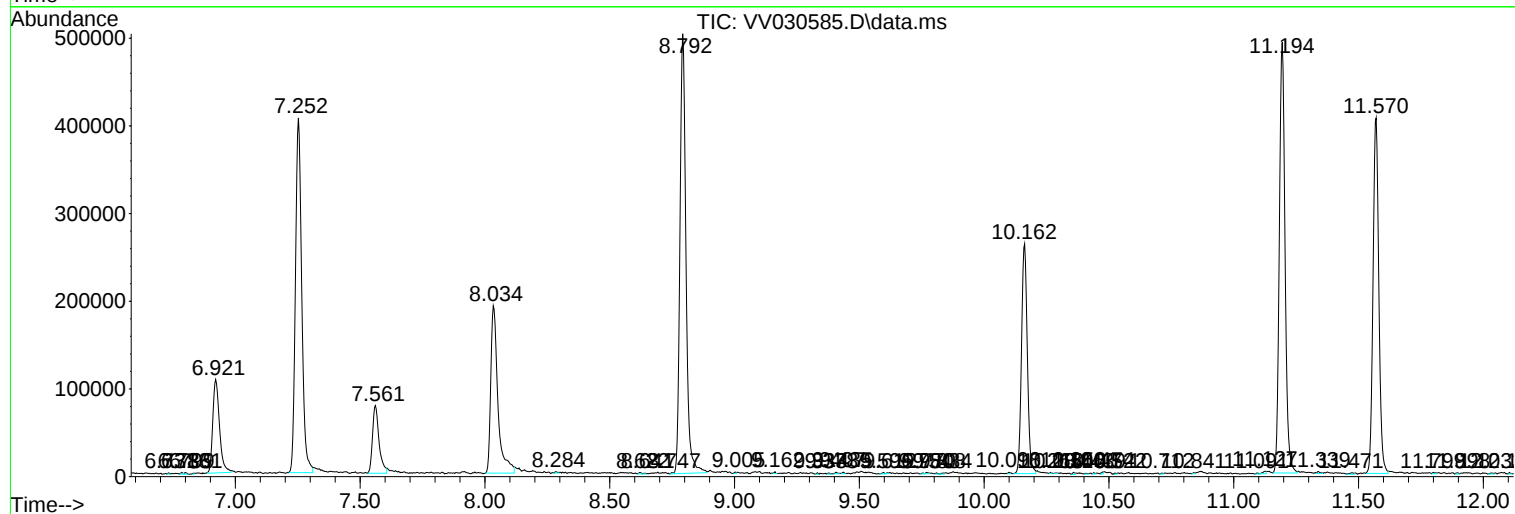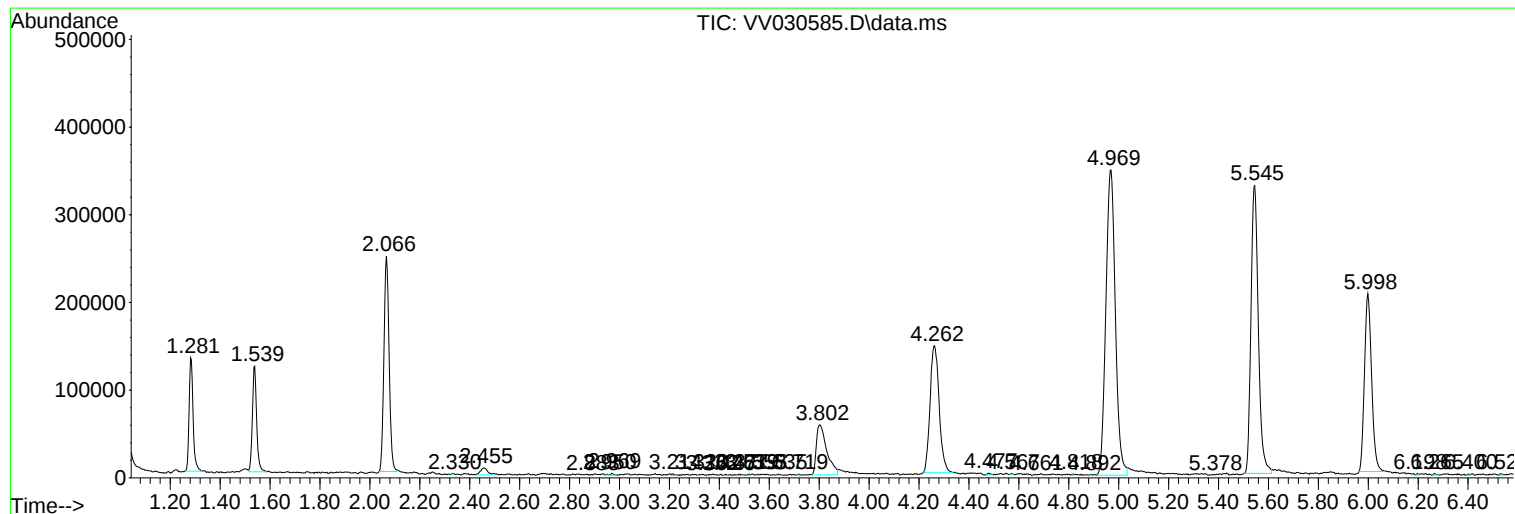

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030585.D
Acq On : 17 Apr 2023 13:49
Operator : SY/MD
Sample : VV0417MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030585.D
Acq On : 17 Apr 2023 13:49
Operator : SY/MD
Sample : VV0417MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc