

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030586.D
 Acq On : 17 Apr 2023 14:12
 Operator : SY/MD
 Sample : VV0417WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK321

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	90	rVB	126990	140409	15.75%	1.956%
2	1.539	148	155	165	rVB	114266	134259	15.06%	1.871%
3	2.066	310	319	332	rBV	240169	343294	38.52%	4.783%
4	2.455	433	440	451	rVB3	8115	13793	1.55%	0.192%
5	2.526	459	462	466	rBV6	1269	923	0.10%	0.013%
6	2.671	505	507	510	rBV4	1357	674	0.08%	0.009%
7	2.690	510	513	515	rBV4	1923	1505	0.17%	0.021%
8	2.783	539	542	546	rVB5	1199	714	0.08%	0.010%
9	2.844	559	561	564	rBV4	909	645	0.07%	0.009%
10	2.944	588	592	594	rBV4	1912	1508	0.17%	0.021%
11	3.034	616	620	621	rBV3	1447	806	0.09%	0.011%
12	3.182	664	666	669	rVV4	1447	877	0.10%	0.012%
13	3.236	680	683	684	rBV3	1661	1030	0.12%	0.014%
14	3.301	701	703	711	rVB9	1914	1294	0.15%	0.018%
15	3.343	714	716	719	rBV4	1271	713	0.08%	0.010%
16	3.433	741	744	747	rVV5	1192	1015	0.11%	0.014%
17	3.535	774	776	782	rBV6	799	889	0.10%	0.012%
18	3.568	782	786	790	rBV5	1542	1311	0.15%	0.018%
19	3.603	794	797	802	rVV7	2091	1603	0.18%	0.022%
20	3.622	802	803	807	rVB4	1339	655	0.07%	0.009%
21	3.661	812	815	818	rVB4	1027	714	0.08%	0.010%
22	3.748	840	842	844	rBV3	1393	546	0.06%	0.008%
23	3.806	850	860	886	rBV	54206	160765	18.04%	2.240%
24	4.146	961	966	967	rBV5	2043	1932	0.22%	0.027%
25	4.185	975	978	981	rBV5	1157	951	0.11%	0.013%
26	4.262	986	1002	1026	rVV2	140706	369159	41.42%	5.143%
27	4.416	1049	1050	1052	rBV2	1400	564	0.06%	0.008%
28	4.648	1119	1122	1125	rBV5	1455	1029	0.12%	0.014%
29	4.796	1166	1168	1172	rVB4	1469	799	0.09%	0.011%
30	4.822	1175	1176	1179	rBV3	1329	700	0.08%	0.010%
31	4.892	1195	1198	1203	rBV4	980	787	0.09%	0.011%
32	4.966	1204	1221	1241	rBV2	333968	891281	100.00%	12.418%
33	5.278	1316	1318	1321	rBV4	1513	981	0.11%	0.014%
34	5.471	1376	1378	1380	rBV3	1219	710	0.08%	0.010%
35	5.542	1388	1400	1421	rBV	316132	653672	73.34%	9.108%
36	5.998	1530	1542	1558	rBV	195047	395478	44.37%	5.510%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030586.D
 Acq On : 17 Apr 2023 14:12
 Operator : SY/MD
 Sample : VV0417WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK321

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.240	1615	1617	1619	rBV3	1467	637	0.07%	0.009%
38	6.436	1676	1678	1681	rVB3	1587	838	0.09%	0.012%
39	6.503	1697	1699	1702	rVB4	1612	801	0.09%	0.011%
40	6.532	1705	1708	1712	rBV6	1511	1582	0.18%	0.022%
41	6.667	1747	1750	1751	rBV3	947	568	0.06%	0.008%
42	6.773	1779	1783	1787	rVB6	1548	1404	0.16%	0.020%
43	6.834	1799	1802	1804	rBV3	1055	695	0.08%	0.010%
44	6.921	1815	1829	1844	rBV	103396	198433	22.26%	2.765%
45	7.252	1920	1932	1953	rBV	388152	683096	76.64%	9.517%
46	7.561	2017	2028	2049	rBV	76737	143039	16.05%	1.993%
47	7.867	2117	2123	2125	rBV7	2241	1881	0.21%	0.026%
48	8.034	2162	2175	2204	rBV	187082	376186	42.21%	5.241%
49	8.506	2319	2322	2323	rBV3	1185	826	0.09%	0.012%
50	8.648	2363	2366	2367	rBV2	1432	668	0.07%	0.009%
51	8.744	2393	2396	2397	rBV2	1246	629	0.07%	0.009%
52	8.793	2400	2411	2431	rVV	485834	797407	89.47%	11.110%
53	9.034	2482	2486	2488	rBV4	1769	1585	0.18%	0.022%
54	9.252	2552	2554	2558	rVB5	1816	882	0.10%	0.012%
55	9.323	2575	2576	2580	rBV4	1098	662	0.07%	0.009%
56	9.368	2588	2590	2591	rBV2	1166	613	0.07%	0.009%
57	9.490	2626	2628	2630	rBV3	1409	849	0.10%	0.012%
58	9.590	2656	2659	2661	rBV4	1344	1033	0.12%	0.014%
59	9.818	2726	2730	2733	rBV6	1740	992	0.11%	0.014%
60	9.837	2734	2736	2741	rVB7	1304	801	0.09%	0.011%
61	9.899	2753	2755	2760	rBV6	797	542	0.06%	0.008%
62	10.063	2802	2806	2809	rVV5	1895	1514	0.17%	0.021%
63	10.091	2813	2815	2818	rVB3	1166	558	0.06%	0.008%
64	10.162	2825	2837	2853	rBV	257008	418989	47.01%	5.838%
65	10.532	2949	2952	2955	rBV5	939	795	0.09%	0.011%
66	10.596	2970	2972	2975	rBV4	1133	752	0.08%	0.010%
67	10.683	2996	2999	3000	rBV4	1445	774	0.09%	0.011%
68	10.757	3020	3022	3026	rVB5	1289	885	0.10%	0.012%
69	10.789	3029	3032	3034	rBV3	860	563	0.06%	0.008%
70	10.825	3041	3043	3045	rBV3	1304	660	0.07%	0.009%
71	10.911	3066	3070	3072	rBV4	1734	1460	0.16%	0.020%
72	10.960	3080	3085	3086	rBV4	1766	1148	0.13%	0.016%
73	11.124	3133	3136	3138	rBV3	3100	2287	0.26%	0.032%
74	11.194	3147	3158	3176	rBV	476338	753389	84.53%	10.497%
75	11.571	3263	3275	3289	rBV	384937	623178	69.92%	8.683%
76	11.712	3317	3319	3324	rBV4	1064	636	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030586.D
 Acq On : 17 Apr 2023 14:12
 Operator : SY/MD
 Sample : VV0417WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK321

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.757	3330	3333	3334	rBV3	1707	824	0.09%	0.011%
78	11.821	3348	3353	3354	rBV4	1250	1240	0.14%	0.017%
79	11.908	3376	3380	3387	rVB9	1933	2175	0.24%	0.030%
80	12.062	3426	3428	3429	rBV2	1379	544	0.06%	0.008%
81	12.259	3486	3489	3490	rBV2	941	605	0.07%	0.008%
82	12.300	3499	3502	3504	rBV4	1273	729	0.08%	0.010%
83	12.426	3539	3541	3545	rVB5	1589	935	0.10%	0.013%
84	12.487	3556	3560	3561	rBV4	1103	571	0.06%	0.008%
85	12.513	3567	3568	3572	rBV4	1573	1127	0.13%	0.016%
86	12.561	3580	3583	3585	rBV3	1446	892	0.10%	0.012%
87	12.741	3635	3639	3641	rBV4	1213	984	0.11%	0.014%
88	12.754	3641	3643	3645	rVB3	1501	732	0.08%	0.010%
89	12.767	3645	3647	3651	rBV5	1145	850	0.10%	0.012%
90	13.005	3719	3721	3723	rVB2	1544	762	0.09%	0.011%
91	13.104	3750	3752	3755	rBV4	1060	590	0.07%	0.008%
92	13.162	3768	3770	3773	rBV4	1279	952	0.11%	0.013%
93	13.275	3802	3805	3807	rBV4	1256	753	0.08%	0.010%
94	13.381	3833	3838	3839	rBV4	1678	1491	0.17%	0.021%
95	13.519	3879	3881	3884	rBV4	927	579	0.06%	0.008%
96	13.551	3890	3891	3894	rBV3	1211	751	0.08%	0.010%
97	13.950	4011	4015	4022	rBV10	2029	2332	0.26%	0.032%
98	14.011	4029	4034	4038	rBV7	2222	2710	0.30%	0.038%
99	14.435	4163	4166	4168	rBV4	1107	689	0.08%	0.010%
100	14.789	4273	4276	4278	rBV3	2343	1233	0.14%	0.017%




Sum of corrected areas: 7177272

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030586.D
Acq On : 17 Apr 2023 14:12
Operator : SY/MD
Sample : VV0417WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

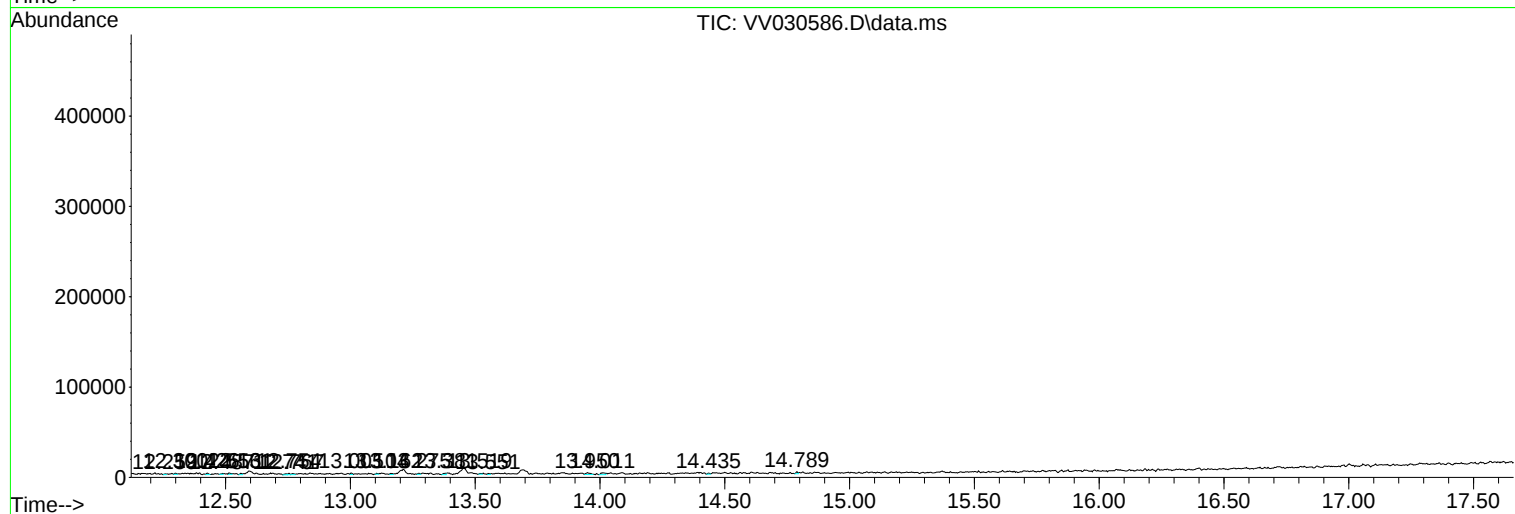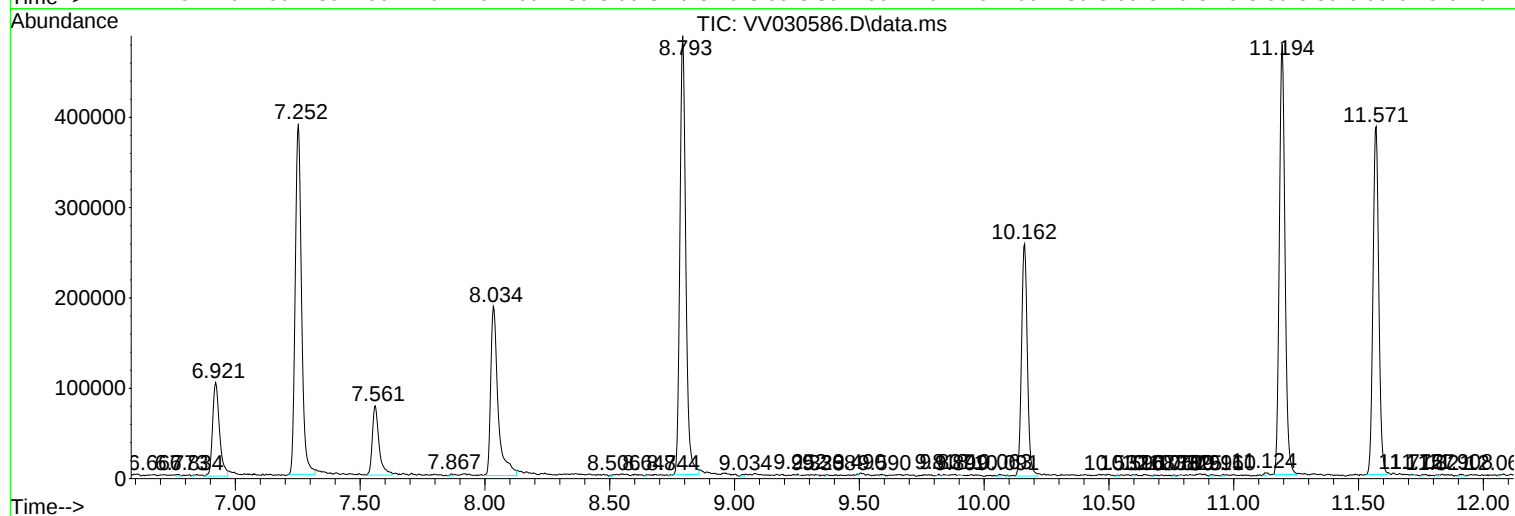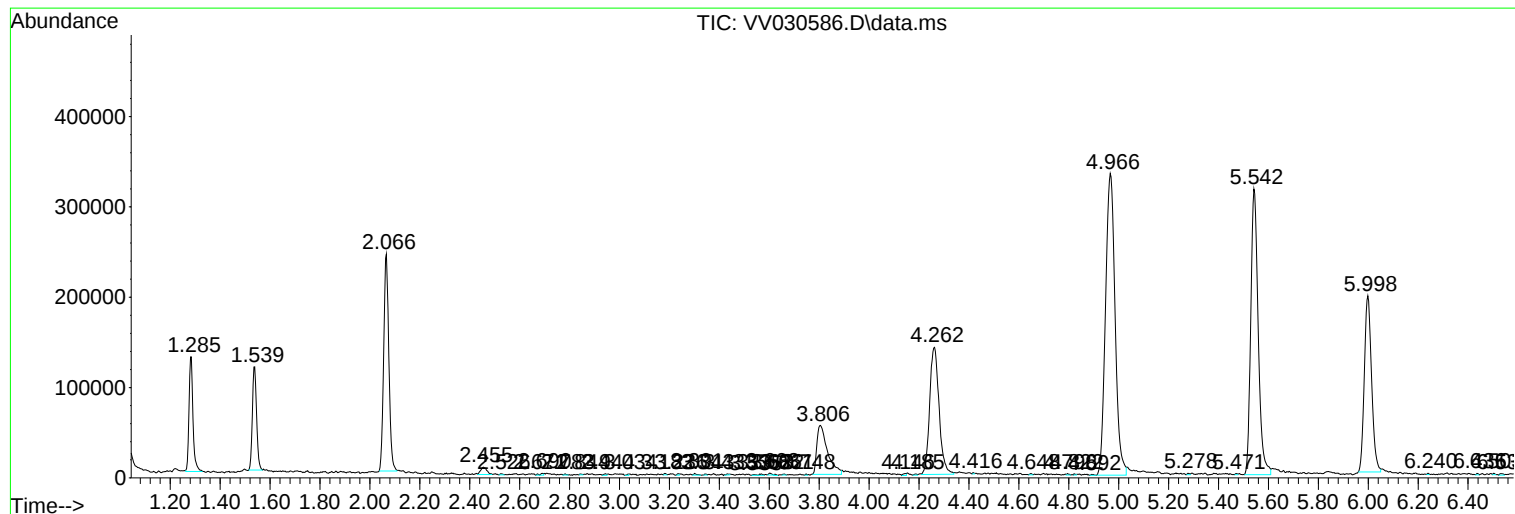

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030586.D
Acq On : 17 Apr 2023 14:12
Operator : SY/MD
Sample : VV0417WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030586.D
Acq On : 17 Apr 2023 14:12
Operator : SY/MD
Sample : VV0417WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK321

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------