

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030589.D
 Acq On : 17 Apr 2023 15:23
 Operator : SY/MD
 Sample : 02360-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	90	rVB	132209	144930	15.72%	2.003%
2	1.536	148	154	168	rVB	119972	141306	15.32%	1.953%
3	2.066	310	319	331	rBV	239924	351714	38.14%	4.861%
4	2.439	433	435	438	rBV4	1662	1169	0.13%	0.016%
5	2.500	453	454	455	rBV	920	340	0.04%	0.005%
6	2.574	474	477	481	rVB6	1868	1036	0.11%	0.014%
7	2.597	482	484	485	rBV2	1111	377	0.04%	0.005%
8	2.712	517	520	525	rBV7	1500	1092	0.12%	0.015%
9	2.802	545	548	549	rBV2	1599	648	0.07%	0.009%
10	2.889	573	575	577	rBV3	850	482	0.05%	0.007%
11	2.918	581	584	591	rVB9	1812	1795	0.19%	0.025%
12	2.960	591	597	600	rBV8	1684	2349	0.25%	0.032%
13	3.101	637	641	644	rBV5	901	744	0.08%	0.010%
14	3.124	646	648	651	rVB4	1347	597	0.06%	0.008%
15	3.179	662	665	666	rBV3	1316	750	0.08%	0.010%
16	3.220	677	678	679	rBV	767	217	0.02%	0.003%
17	3.240	682	684	685	rBV2	784	305	0.03%	0.004%
18	3.352	716	719	720	rVB3	759	326	0.04%	0.005%
19	3.362	720	722	723	rBV2	646	289	0.03%	0.004%
20	3.397	730	733	738	rBV7	1586	1277	0.14%	0.018%
21	3.465	752	754	756	rVB3	1129	502	0.05%	0.007%
22	3.491	756	762	765	rVB7	1662	1615	0.18%	0.022%
23	3.516	765	770	773	rBV7	1535	1464	0.16%	0.020%
24	3.529	773	774	775	rBV	1047	357	0.04%	0.005%
25	3.613	799	800	802	rBV2	1009	495	0.05%	0.007%
26	3.661	813	815	818	rBV4	856	494	0.05%	0.007%
27	3.745	838	841	844	rBV5	1319	864	0.09%	0.012%
28	3.767	844	848	849	rBV4	656	355	0.04%	0.005%
29	3.802	849	859	883	rBV	56351	166187	18.02%	2.297%
30	4.262	989	1002	1027	rVB	146107	373184	40.47%	5.157%
31	4.738	1148	1150	1152	rBV2	1525	898	0.10%	0.012%
32	4.789	1162	1166	1169	rBV4	1719	1463	0.16%	0.020%
33	4.831	1177	1179	1183	rBV6	1458	1181	0.13%	0.016%
34	4.966	1203	1221	1248	rBV2	343320	922235	100.00%	12.745%
35	5.445	1368	1370	1374	rBV3	1365	664	0.07%	0.009%
36	5.542	1388	1400	1425	rBV	313887	648535	70.32%	8.963%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030589.D
 Acq On : 17 Apr 2023 15:23
 Operator : SY/MD
 Sample : 02360-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	5.998	1530	1542	1561	rBV	201278	410582	44.52%	5.674%
38	6.375	1657	1659	1661	rBV3	1395	692	0.08%	0.010%
39	6.416	1670	1672	1675	rBV4	1397	958	0.10%	0.013%
40	6.558	1712	1716	1718	rBV5	1268	771	0.08%	0.011%
41	6.825	1797	1799	1800	rBV2	749	162	0.02%	0.002%
42	6.921	1819	1829	1845	rBV	106717	194340	21.07%	2.686%
43	7.252	1920	1932	1953	rBV	403666	713137	77.33%	9.856%
44	7.561	2019	2028	2045	rBV	74297	135244	14.66%	1.869%
45	7.728	2078	2080	2082	rBV3	971	510	0.06%	0.007%
46	7.825	2108	2110	2112	rBV2	1330	704	0.08%	0.010%
47	7.867	2120	2123	2124	rBV3	1968	1139	0.12%	0.016%
48	7.985	2157	2160	2162	rBV4	1397	747	0.08%	0.010%
49	8.034	2162	2175	2205	rBV	189443	376522	40.83%	5.204%
50	8.249	2239	2242	2245	rBV4	1494	1274	0.14%	0.018%
51	8.477	2311	2313	2315	rBV3	1944	933	0.10%	0.013%
52	8.587	2343	2347	2351	rBV7	1152	1162	0.13%	0.016%
53	8.728	2388	2391	2394	rBV4	1525	1121	0.12%	0.015%
54	8.793	2400	2411	2429	rBV	479100	785499	85.17%	10.856%
55	9.034	2483	2486	2490	rBV5	1372	1280	0.14%	0.018%
56	9.233	2544	2548	2549	rBV4	1239	807	0.09%	0.011%
57	9.294	2564	2567	2572	rBV6	1631	1243	0.13%	0.017%
58	9.407	2600	2602	2605	rBV4	1164	916	0.10%	0.013%
59	9.452	2614	2616	2618	rVB3	975	372	0.04%	0.005%
60	9.616	2663	2667	2671	rBV5	1914	1812	0.20%	0.025%
61	9.632	2671	2672	2674	rBV2	1107	531	0.06%	0.007%
62	9.847	2737	2739	2742	rBV4	1678	1260	0.14%	0.017%
63	9.950	2770	2771	2773	rBV2	1459	746	0.08%	0.010%
64	10.001	2786	2787	2789	rBV2	1171	433	0.05%	0.006%
65	10.056	2800	2804	2805	rBV4	1191	839	0.09%	0.012%
66	10.162	2826	2837	2854	rVB	262883	415125	45.01%	5.737%
67	10.329	2885	2889	2890	rBV4	4282	3026	0.33%	0.042%
68	10.555	2957	2959	2960	rBV2	1141	337	0.04%	0.005%
69	10.567	2960	2963	2964	rBV3	782	489	0.05%	0.007%
70	10.596	2970	2972	2973	rBV2	610	217	0.02%	0.003%
71	10.712	3007	3008	3012	rVB3	1372	747	0.08%	0.010%
72	10.735	3012	3015	3019	rBV6	1798	1261	0.14%	0.017%
73	10.754	3019	3021	3024	rBV3	1720	1033	0.11%	0.014%
74	10.960	3081	3085	3088	rVB6	1571	1285	0.14%	0.018%
75	10.979	3088	3091	3092	rBV2	962	633	0.07%	0.009%
76	11.194	3145	3158	3178	rBV	468352	745532	80.84%	10.303%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030589.D
 Acq On : 17 Apr 2023 15:23
 Operator : SY/MD
 Sample : 02360-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.362	3207	3210	3212	rBV5	1511	1051	0.11%	0.015%
78	11.571	3264	3275	3290	rVB	399819	630902	68.41%	8.719%
79	12.053	3421	3425	3430	rVB7	1900	1890	0.20%	0.026%
80	12.124	3443	3447	3450	rBV6	1327	1121	0.12%	0.015%
81	12.165	3458	3460	3461	rBV2	949	311	0.03%	0.004%
82	12.175	3461	3463	3465	rBV4	1086	601	0.07%	0.008%
83	12.188	3465	3467	3470	rBV5	1606	1278	0.14%	0.018%
84	12.596	3587	3594	3600	rBV8	4108	5762	0.62%	0.080%
85	12.686	3619	3622	3628	rBV7	1455	1724	0.19%	0.024%
86	12.770	3644	3648	3650	rBV4	1443	1340	0.15%	0.019%
87	12.792	3653	3655	3658	rVV4	1614	823	0.09%	0.011%
88	12.808	3658	3660	3662	rVV3	861	352	0.04%	0.005%
89	12.818	3662	3663	3665	rVB2	1263	424	0.05%	0.006%
90	12.905	3689	3690	3691	rBV	742	241	0.03%	0.003%
91	12.915	3691	3693	3695	rVV2	1142	684	0.07%	0.009%
92	12.960	3704	3707	3712	rVB5	2552	1933	0.21%	0.027%
93	12.995	3712	3718	3720	rBV7	1323	1372	0.15%	0.019%
94	13.069	3738	3741	3743	rBV3	1074	859	0.09%	0.012%
95	13.371	3833	3835	3837	rBV3	1349	659	0.07%	0.009%
96	13.567	3893	3896	3900	rVB4	907	700	0.08%	0.010%
97	13.590	3900	3903	3906	rBV4	1914	1287	0.14%	0.018%
98	13.805	3966	3970	3973	rBV5	1827	1665	0.18%	0.023%
99	13.927	4004	4008	4011	rBV4	1544	1220	0.13%	0.017%




Sum of corrected areas: 7235856

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030589.D
Acq On : 17 Apr 2023 15:23
Operator : SY/MD
Sample : 02360-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

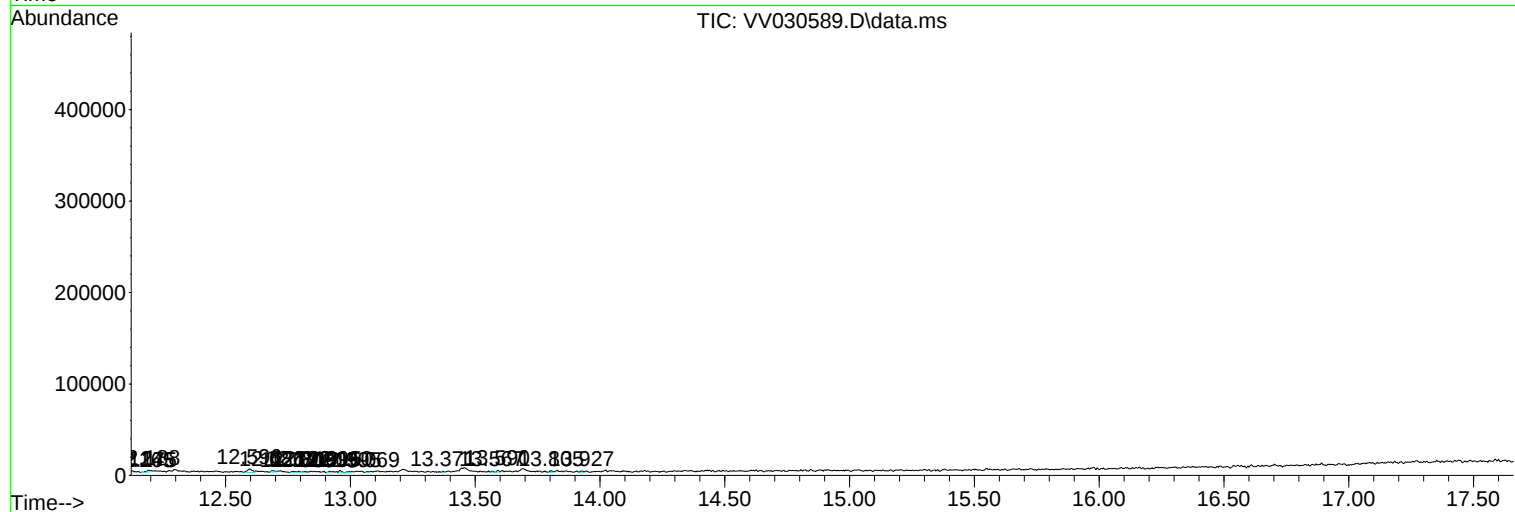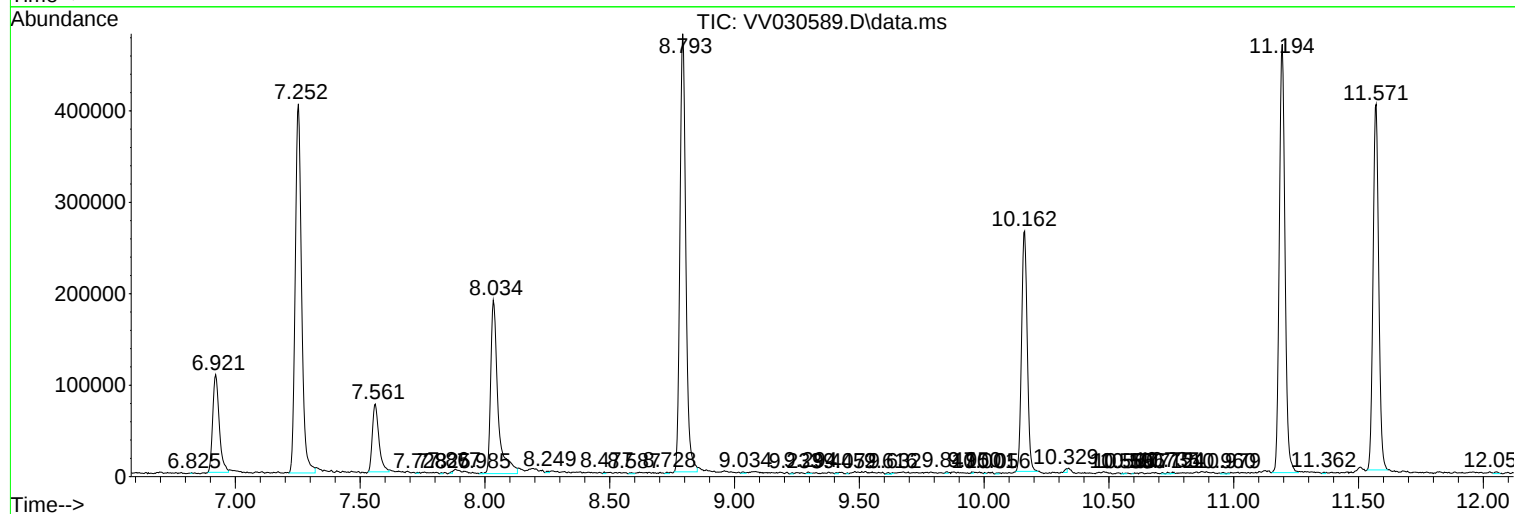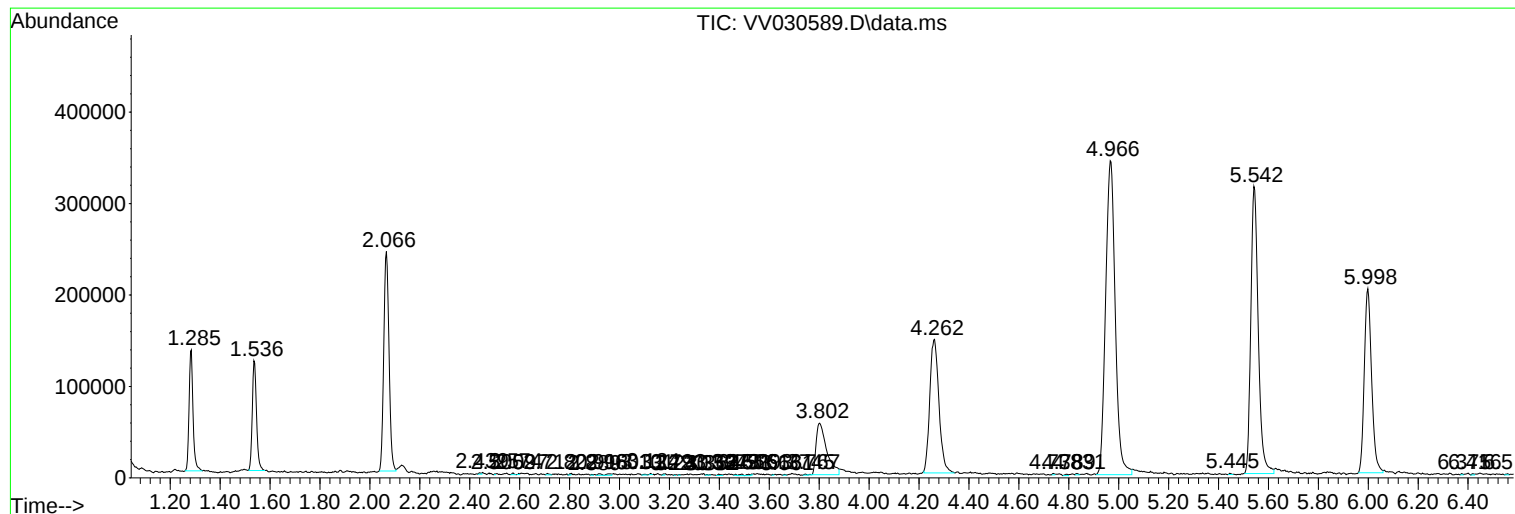

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030589.D
Acq On : 17 Apr 2023 15:23
Operator : SY/MD
Sample : 02360-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030589.D
Acq On : 17 Apr 2023 15:23
Operator : SY/MD
Sample : 02360-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------