

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030590.D
 Acq On : 17 Apr 2023 15:47
 Operator : SY/MD
 Sample : 02360-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	91	rVB	121876	134369	15.10%	1.921%
2	1.536	148	154	168	rVB	117827	140416	15.78%	2.007%
3	2.066	310	319	331	rBV	222838	319807	35.93%	4.571%
4	2.516	457	459	462	rBV3	1294	758	0.09%	0.011%
5	2.851	557	563	565	rBV6	992	748	0.08%	0.011%
6	2.909	577	581	582	rBV3	1383	1013	0.11%	0.014%
7	3.050	623	625	628	rBV3	891	377	0.04%	0.005%
8	3.089	633	637	639	rBV5	1138	1051	0.12%	0.015%
9	3.169	658	662	664	rBV4	1178	735	0.08%	0.011%
10	3.198	667	671	673	rBV4	1481	1029	0.12%	0.015%
11	3.429	741	743	744	rBV2	760	312	0.04%	0.004%
12	3.458	749	752	755	rBV4	1892	1195	0.13%	0.017%
13	3.523	770	772	774	rBB3	1014	405	0.05%	0.006%
14	3.568	784	786	790	rVB4	1597	892	0.10%	0.013%
15	3.593	790	794	796	rBV4	1642	1547	0.17%	0.022%
16	3.645	808	810	814	rVB4	1245	689	0.08%	0.010%
17	3.661	814	815	819	rBV4	1013	641	0.07%	0.009%
18	3.725	832	835	836	rBV3	1609	747	0.08%	0.011%
19	3.802	850	859	888	rBV	56934	169544	19.05%	2.424%
20	4.063	937	940	942	rVB4	1384	762	0.09%	0.011%
21	4.159	967	970	972	rBV5	1561	884	0.10%	0.013%
22	4.259	983	1001	1026	rBV2	141383	369458	41.51%	5.281%
23	4.471	1065	1067	1069	rVB3	1313	521	0.06%	0.007%
24	4.507	1076	1078	1081	rBV3	1128	807	0.09%	0.012%
25	4.719	1142	1144	1146	rBV2	864	390	0.04%	0.006%
26	4.809	1167	1172	1173	rBV4	1118	1059	0.12%	0.015%
27	4.966	1203	1221	1245	rBV2	334300	890022	100.00%	12.722%
28	5.542	1387	1400	1420	rBV	299806	624464	70.16%	8.926%
29	5.998	1530	1542	1563	rBV	194292	400858	45.04%	5.730%
30	6.439	1677	1679	1680	rVB2	1063	372	0.04%	0.005%
31	6.548	1711	1713	1714	rVB2	1629	501	0.06%	0.007%
32	6.564	1716	1718	1720	rBV3	1269	636	0.07%	0.009%
33	6.590	1725	1726	1729	rBV3	1108	568	0.06%	0.008%
34	6.619	1733	1735	1739	rVV5	998	602	0.07%	0.009%
35	6.642	1739	1742	1744	rBV4	1661	1075	0.12%	0.015%
36	6.680	1752	1754	1756	rBV3	1097	622	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030590.D
 Acq On : 17 Apr 2023 15:47
 Operator : SY/MD
 Sample : 02360-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.719	1765	1766	1771	rBV5	1159	855	0.10%	0.012%
38	6.744	1772	1774	1776	rVB3	2155	932	0.10%	0.013%
39	6.754	1776	1777	1779	rBV2	1035	510	0.06%	0.007%
40	6.773	1779	1783	1784	rBV4	817	420	0.05%	0.006%
41	6.818	1793	1797	1799	rVB5	1154	782	0.09%	0.011%
42	6.831	1799	1801	1803	rBV3	1235	471	0.05%	0.007%
43	6.844	1803	1805	1806	rBV2	925	392	0.04%	0.006%
44	6.921	1819	1829	1849	rBV	102172	190527	21.41%	2.723%
45	7.137	1892	1896	1900	rBV6	1640	1723	0.19%	0.025%
46	7.252	1921	1932	1952	rBV	376253	667939	75.05%	9.548%
47	7.561	2019	2028	2043	rBV	75836	132694	14.91%	1.897%
48	7.879	2121	2127	2135	rBV10	3756	6108	0.69%	0.087%
49	7.973	2154	2156	2164	rVB9	1299	1280	0.14%	0.018%
50	8.034	2166	2175	2200	rBV	181564	356422	40.05%	5.095%
51	8.359	2274	2276	2278	rBV3	1400	567	0.06%	0.008%
52	8.516	2321	2325	2328	rBV6	1226	926	0.10%	0.013%
53	8.587	2343	2347	2348	rBV4	962	608	0.07%	0.009%
54	8.699	2378	2382	2385	rBV5	1351	1411	0.16%	0.020%
55	8.793	2399	2411	2434	rBV	466677	777171	87.32%	11.109%
56	9.268	2555	2559	2560	rBV4	1428	1109	0.12%	0.016%
57	9.330	2576	2578	2582	rVB5	873	520	0.06%	0.007%
58	9.378	2591	2593	2596	rVB4	1440	664	0.07%	0.009%
59	9.500	2628	2631	2632	rBV3	2119	1031	0.12%	0.015%
60	9.574	2651	2654	2657	rBV5	1016	729	0.08%	0.010%
61	9.703	2691	2694	2698	rBV5	1514	1251	0.14%	0.018%
62	9.748	2705	2708	2712	rBV6	1330	1052	0.12%	0.015%
63	9.786	2717	2720	2721	rBV2	1223	592	0.07%	0.008%
64	9.905	2753	2757	2758	rBV3	1244	835	0.09%	0.012%
65	10.030	2794	2796	2800	rVB4	1846	1111	0.12%	0.016%
66	10.050	2800	2802	2806	rBV4	1310	637	0.07%	0.009%
67	10.075	2806	2810	2813	rBV5	1167	1206	0.14%	0.017%
68	10.162	2822	2837	2852	rBV	261893	419432	47.13%	5.996%
69	10.329	2883	2889	2890	rBV4	5026	4096	0.46%	0.059%
70	10.693	2999	3002	3006	rVB4	1824	1288	0.14%	0.018%
71	10.712	3006	3008	3012	rVB5	1383	749	0.08%	0.011%
72	10.735	3012	3015	3016	rBV3	1176	724	0.08%	0.010%
73	10.796	3031	3034	3035	rBV3	1345	693	0.08%	0.010%
74	10.838	3045	3047	3049	rBV3	1081	490	0.06%	0.007%
75	10.892	3062	3064	3066	rBV2	1081	449	0.05%	0.006%
76	10.940	3075	3079	3082	rBV5	1336	1400	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030590.D
 Acq On : 17 Apr 2023 15:47
 Operator : SY/MD
 Sample : 02360-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.053	3112	3114	3116	rBV2	1344	657	0.07%	0.009%
78	11.194	3147	3158	3175	rBV	455587	717992	80.67%	10.263%
79	11.374	3212	3214	3217	rBV3	1449	1043	0.12%	0.015%
80	11.493	3248	3251	3252	rBV3	1391	589	0.07%	0.008%
81	11.571	3264	3275	3290	rVB	388301	609366	68.47%	8.711%
82	11.799	3344	3346	3348	rVB3	1531	683	0.08%	0.010%
83	12.050	3422	3424	3427	rBV3	1357	815	0.09%	0.012%
84	12.108	3438	3442	3443	rBV3	717	371	0.04%	0.005%
85	12.220	3474	3477	3481	rBV5	1421	996	0.11%	0.014%
86	12.297	3500	3501	3503	rBV2	1092	423	0.05%	0.006%
87	12.432	3541	3543	3545	rBV4	1345	564	0.06%	0.008%
88	12.455	3548	3550	3552	rBV3	1080	500	0.06%	0.007%
89	12.474	3554	3556	3557	rBV2	1297	506	0.06%	0.007%
90	12.519	3568	3570	3571	rBV2	1780	780	0.09%	0.011%
91	12.580	3584	3589	3590	rBV4	1925	1461	0.16%	0.021%
92	12.645	3607	3609	3610	rBV2	925	342	0.04%	0.005%
93	12.725	3630	3634	3638	rVB7	1316	887	0.10%	0.013%
94	12.979	3710	3713	3717	rBV4	1474	960	0.11%	0.014%
95	13.162	3767	3770	3773	rBV5	1378	1214	0.14%	0.017%
96	13.262	3797	3801	3803	rBV4	1881	1391	0.16%	0.020%
97	13.368	3833	3834	3836	rBV2	989	528	0.06%	0.008%
98	13.545	3887	3889	3893	rBV4	1564	714	0.08%	0.010%
99	14.143	4073	4075	4078	rVB3	1372	582	0.07%	0.008%
100	14.345	4135	4138	4139	rBV3	1410	670	0.08%	0.010%




Sum of corrected areas: 6995706

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030590.D
Acq On : 17 Apr 2023 15:47
Operator : SY/MD
Sample : 02360-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

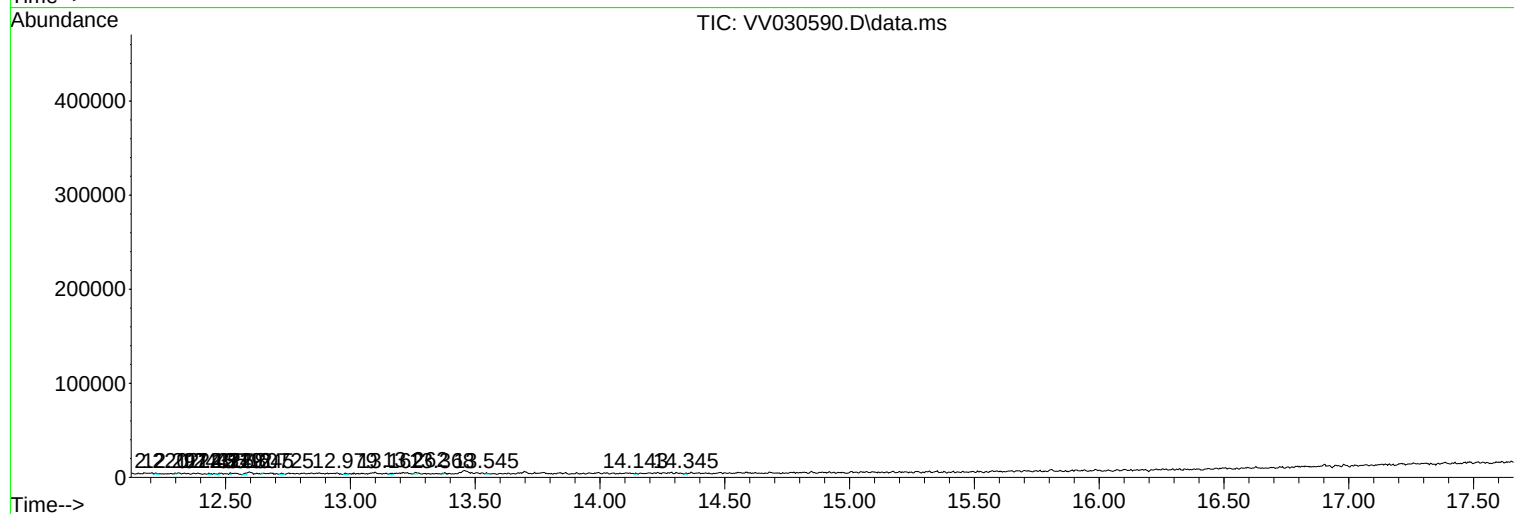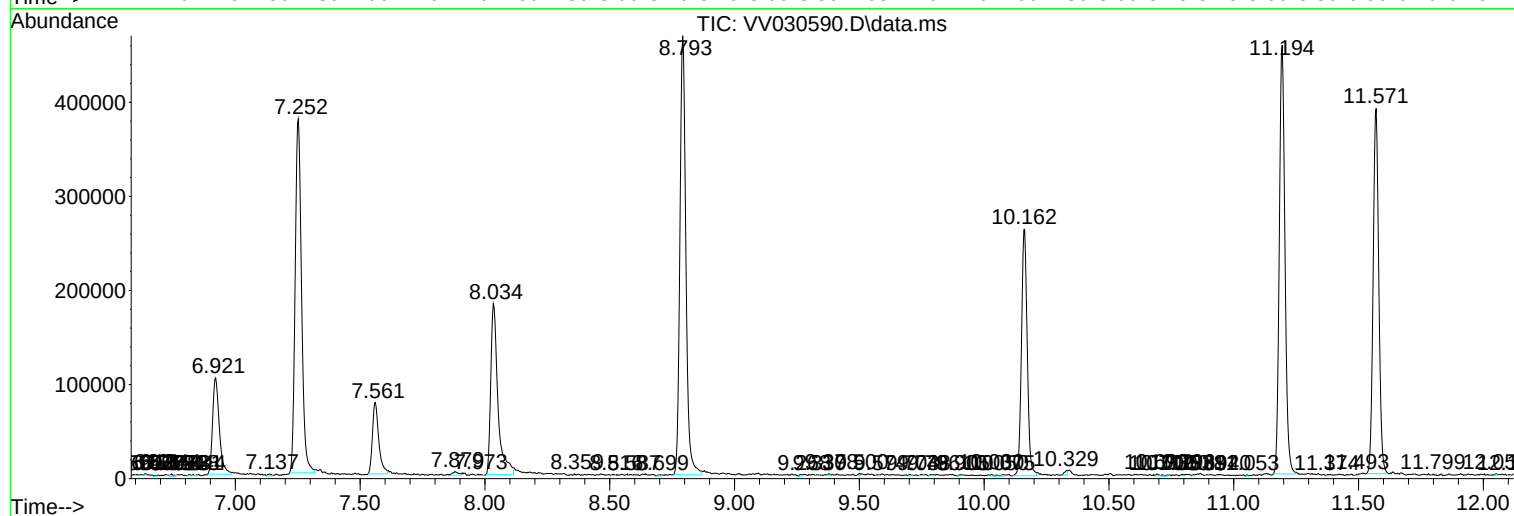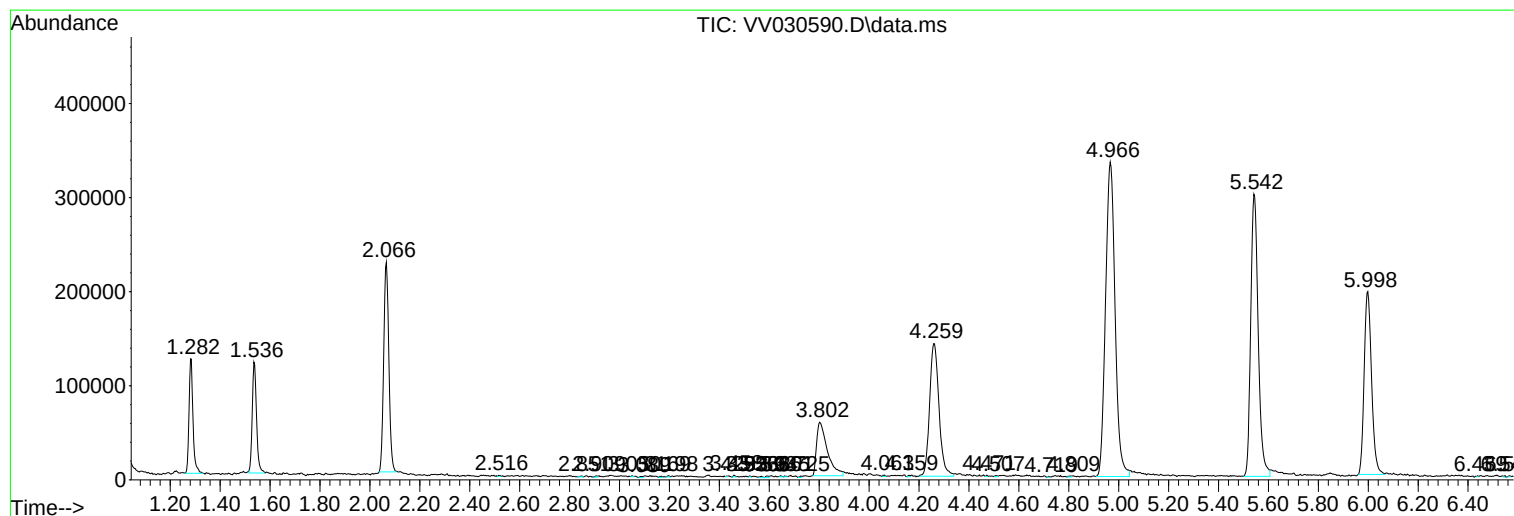

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030590.D
Acq On : 17 Apr 2023 15:47
Operator : SY/MD
Sample : 02360-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030590.D
Acq On : 17 Apr 2023 15:47
Operator : SY/MD
Sample : 02360-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc