

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030593.D
 Acq On : 17 Apr 2023 16:59
 Operator : SY/MD
 Sample : 02360-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	92	rVB	119746	130174	0.06%	0.059%
2	1.535	148	154	169	rVB	107844	129332	0.06%	0.059%
3	2.069	309	320	335	rBV2	403145	713082	0.34%	0.326%
4	2.384	416	418	420	rBV3	985	450	0.00%	0.000%
5	2.433	430	433	434	rBV3	1006	549	0.00%	0.000%
6	2.500	452	454	457	rBV4	1187	870	0.00%	0.000%
7	2.542	465	467	468	rBV2	1107	408	0.00%	0.000%
8	2.584	476	480	482	rVB4	1122	597	0.00%	0.000%
9	2.632	493	495	497	rBV3	1406	755	0.00%	0.000%
10	2.757	533	534	538	rBV4	906	478	0.00%	0.000%
11	2.879	571	572	575	rVB3	1537	501	0.00%	0.000%
12	2.899	575	578	582	rBV5	1492	1343	0.00%	0.001%
13	2.918	582	584	587	rVB4	1757	687	0.00%	0.000%
14	2.944	590	592	594	rVV3	1048	396	0.00%	0.000%
15	3.005	607	611	616	rVB6	1488	1388	0.00%	0.001%
16	3.027	616	618	620	rBV3	1460	639	0.00%	0.000%
17	3.053	623	626	627	rBV3	797	465	0.00%	0.000%
18	3.076	630	633	634	rBV4	1797	979	0.00%	0.000%
19	3.117	638	646	647	rBV6	4974	5063	0.00%	0.002%
20	3.198	668	671	673	rVB4	1424	810	0.00%	0.000%
21	3.211	673	675	677	rBV3	808	526	0.00%	0.000%
22	3.259	685	690	694	rBV7	2170	1816	0.00%	0.001%
23	3.297	698	702	705	rVB4	1421	1160	0.00%	0.001%
24	3.320	705	709	712	rBV6	780	706	0.00%	0.000%
25	3.368	721	724	726	rBV3	1154	801	0.00%	0.000%
26	3.442	743	747	748	rBV3	1058	660	0.00%	0.000%
27	3.481	755	759	761	rBV5	1728	911	0.00%	0.000%
28	3.516	766	770	773	rBV5	1586	1515	0.00%	0.001%
29	3.574	785	788	789	rBV3	1330	615	0.00%	0.000%
30	3.680	819	821	826	rBV6	1904	2014	0.00%	0.001%
31	3.822	850	865	890	rBV2	248564	693140	0.33%	0.317%
32	4.259	988	1001	1027	rVB2	134730	360000	0.17%	0.164%
33	4.394	1041	1043	1047	rVB5	1636	1081	0.00%	0.000%
34	4.522	1069	1083	1105	rVB	188324	483500	0.23%	0.221%
35	4.651	1121	1123	1124	rBV2	1433	605	0.00%	0.000%
36	4.838	1178	1181	1183	rBV4	1188	701	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030593.D
 Acq On : 17 Apr 2023 16:59
 Operator : SY/MD
 Sample : 02360-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	4.866	1188	1190	1193	rVB4	1469	706	0.00%	0.000%
38	4.883	1193	1195	1196	rBV2	1230	572	0.00%	0.000%
39	4.969	1205	1222	1249	rBV2	311428	849025	0.40%	0.388%
40	5.297	1323	1324	1328	rVB3	1920	860	0.00%	0.000%
41	5.320	1328	1331	1332	rBV2	1021	588	0.00%	0.000%
42	5.410	1355	1359	1363	rBV6	1521	1692	0.00%	0.001%
43	5.468	1375	1377	1378	rBV2	1579	658	0.00%	0.000%
44	5.545	1388	1401	1422	rBV	253981	535306	0.25%	0.244%
45	5.873	1477	1503	1506	rBV5	80884721	211477503	100.00%	96.587%
46	6.921	1819	1829	1846	rBV2	100742	185961	0.09%	0.085%
47	7.252	1922	1932	1951	rBV	350182	607744	0.29%	0.278%
48	7.561	2020	2028	2044	rVB	69634	114203	0.05%	0.052%
49	7.780	2088	2096	2108	rVB	42356	69488	0.03%	0.032%
50	8.034	2166	2175	2200	rBV	169226	321816	0.15%	0.147%
51	8.622	2356	2358	2359	rBV2	1439	665	0.00%	0.000%
52	8.792	2401	2411	2432	rBV	385313	636246	0.30%	0.291%
53	9.361	2586	2588	2590	rBV3	2026	1096	0.00%	0.001%
54	9.979	2778	2780	2785	rBV5	1353	942	0.00%	0.000%
55	10.017	2790	2792	2794	rBV3	1286	752	0.00%	0.000%
56	10.104	2817	2819	2824	rBV6	793	684	0.00%	0.000%
57	10.162	2825	2837	2861	rVB	236529	383131	0.18%	0.175%
58	10.381	2902	2905	2908	rBV4	2145	1322	0.00%	0.001%
59	10.416	2914	2916	2921	rVB5	2088	1417	0.00%	0.001%
60	10.442	2921	2924	2926	rBV4	1848	1128	0.00%	0.001%
61	10.471	2930	2933	2935	rBV4	2013	1469	0.00%	0.001%
62	10.542	2951	2955	2957	rBV5	2069	1580	0.00%	0.001%
63	10.660	2990	2992	2994	rBV2	1108	583	0.00%	0.000%
64	10.763	3020	3024	3027	rBV6	1196	960	0.00%	0.000%
65	11.056	3113	3115	3118	rBV4	1149	727	0.00%	0.000%
66	11.194	3147	3158	3177	rBV	390102	616304	0.29%	0.281%
67	11.410	3222	3225	3226	rBV2	1380	750	0.00%	0.000%
68	11.570	3264	3275	3294	rBV	345225	557338	0.26%	0.255%
69	11.847	3357	3361	3364	rBV6	1623	1733	0.00%	0.001%
70	12.008	3409	3411	3413	rBV3	1296	858	0.00%	0.000%
71	12.030	3415	3418	3421	rVB5	1789	1287	0.00%	0.001%
72	12.049	3421	3424	3428	rBV7	1567	1162	0.00%	0.001%
73	12.123	3443	3447	3449	rBV5	2330	1854	0.00%	0.001%
74	12.152	3453	3456	3459	rVB5	1984	1356	0.00%	0.001%
75	12.339	3513	3514	3518	rBV4	1035	460	0.00%	0.000%
76	12.371	3522	3524	3528	rBV5	1954	1432	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030593.D
 Acq On : 17 Apr 2023 16:59
 Operator : SY/MD
 Sample : 02360-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.448	3545	3548	3549	rBV3	1116	590	0.00%	0.000%
78	12.490	3559	3561	3565	rVB4	1127	770	0.00%	0.000%
79	12.529	3571	3573	3575	rBV3	1077	623	0.00%	0.000%
80	12.580	3587	3589	3590	rBV2	2192	1015	0.00%	0.000%
81	12.783	3650	3652	3654	rVB3	1801	773	0.00%	0.000%
82	12.808	3654	3660	3663	rBV6	1795	1899	0.00%	0.001%
83	12.892	3680	3686	3689	rBV7	2097	2237	0.00%	0.001%
84	12.914	3691	3693	3695	rBV3	997	363	0.00%	0.000%
85	12.982	3712	3714	3717	rBV5	849	468	0.00%	0.000%
86	13.368	3830	3834	3839	rBV7	1375	1493	0.00%	0.001%
87	13.458	3852	3862	3869	rBV7	3616	6775	0.00%	0.003%
88	13.561	3890	3894	3896	rVB5	2174	1474	0.00%	0.001%
89	13.577	3898	3899	3901	rBV2	1213	434	0.00%	0.000%
90	13.609	3907	3909	3911	rBV2	978	400	0.00%	0.000%
91	13.657	3921	3924	3925	rBV3	1342	552	0.00%	0.000%
92	13.757	3953	3955	3958	rVB4	1576	651	0.00%	0.000%
93	13.921	4005	4006	4010	rVB4	1056	700	0.00%	0.000%
94	13.985	4022	4026	4027	rBV3	1793	1199	0.00%	0.001%
95	14.053	4043	4047	4050	rVB5	1862	1421	0.00%	0.001%
96	14.114	4064	4066	4069	rBV3	1575	982	0.00%	0.000%
97	14.345	4136	4138	4141	rBV4	1206	642	0.00%	0.000%
98	14.622	4223	4224	4227	rBV3	1146	519	0.00%	0.000%
99	14.750	4262	4264	4268	rBV4	1504	1211	0.00%	0.001%
100	15.133	4381	4383	4385	rBV2	1648	855	0.00%	0.000%




Sum of corrected areas: 218950121

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030593.D
Acq On : 17 Apr 2023 16:59
Operator : SY/MD
Sample : 02360-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

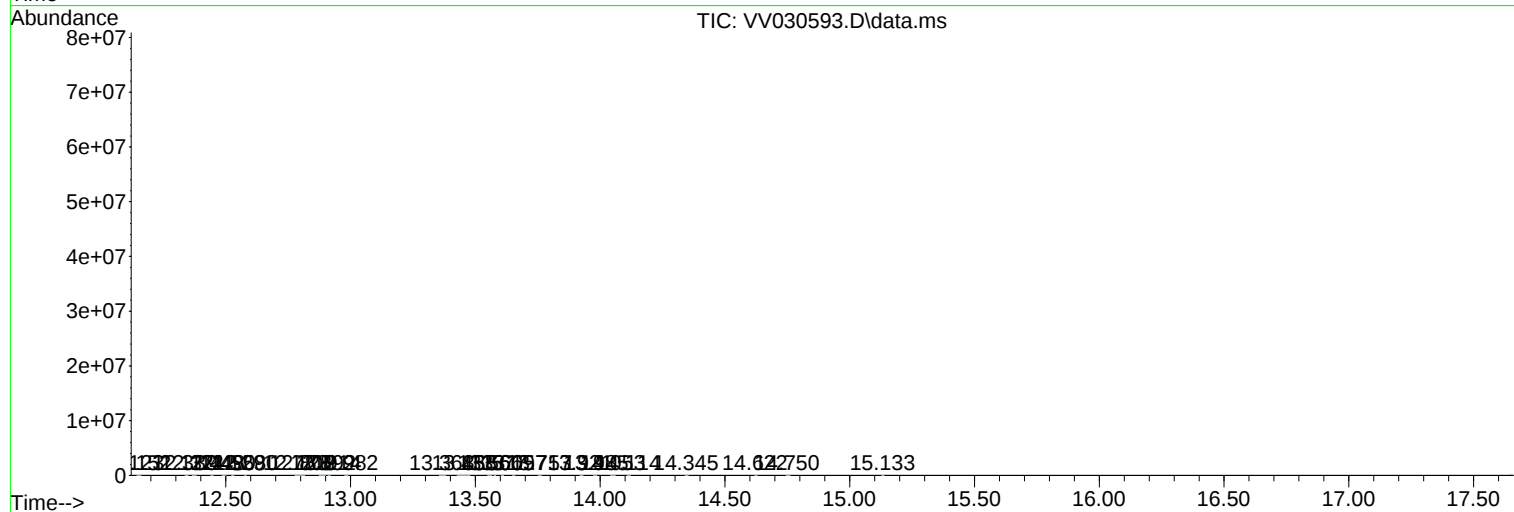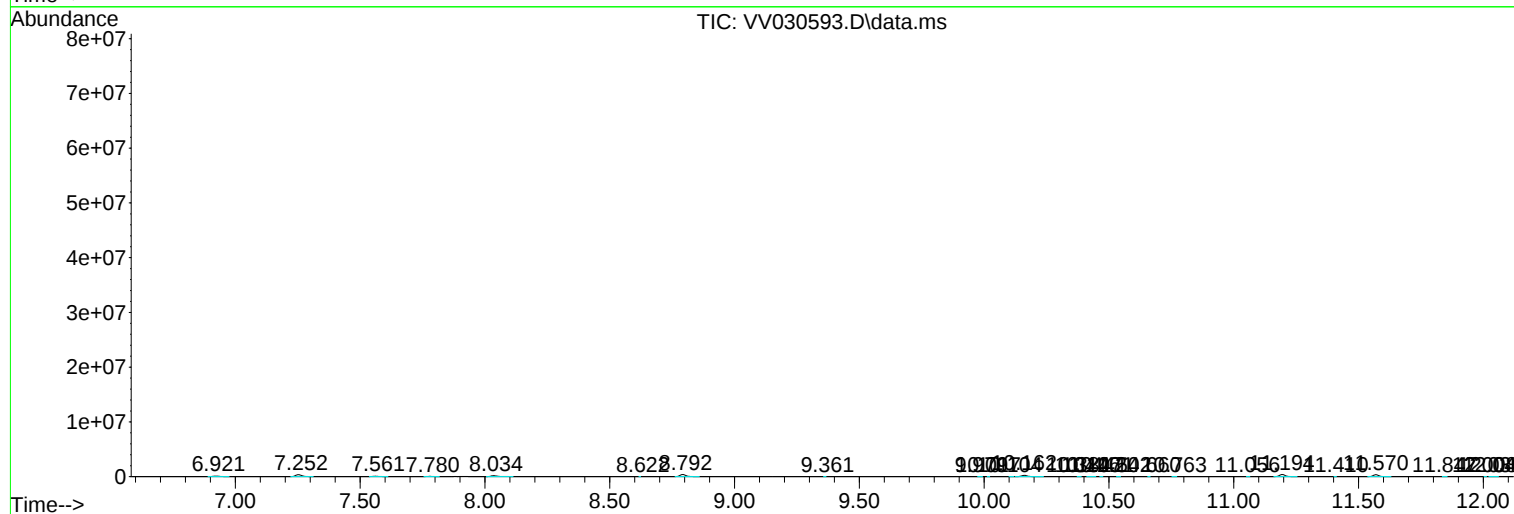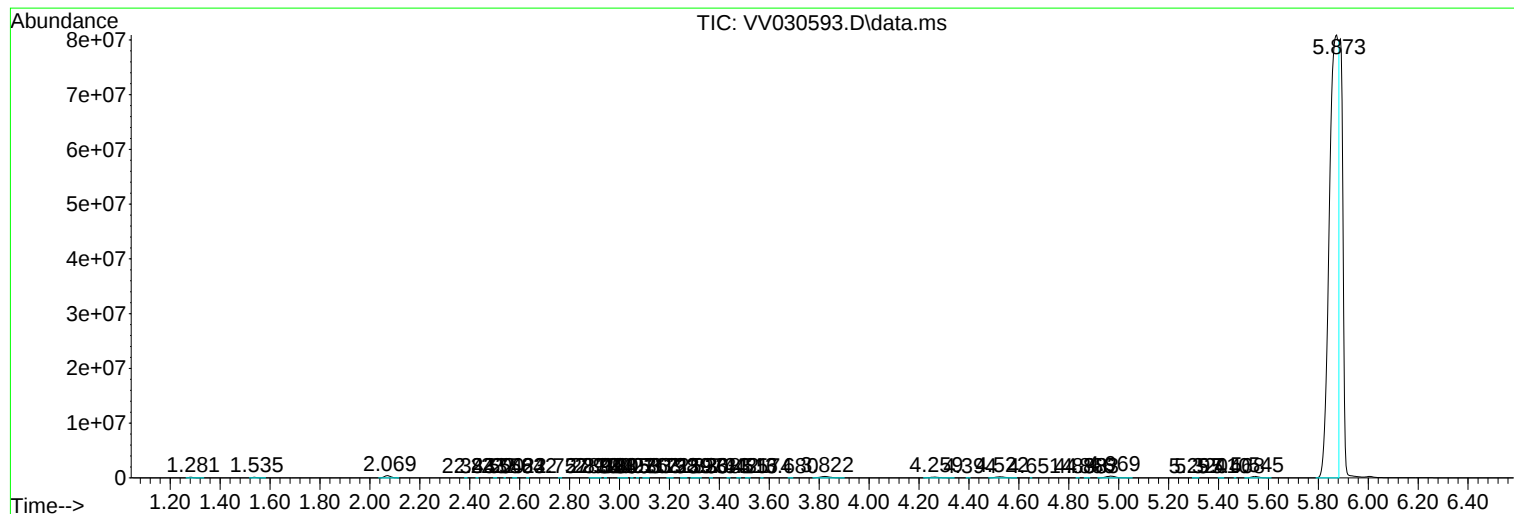

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030593.D
Acq On : 17 Apr 2023 16:59
Operator : SY/MD
Sample : 02360-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030593.D
Acq On : 17 Apr 2023 16:59
Operator : SY/MD
Sample : 02360-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc