

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030594.D
 Acq On : 17 Apr 2023 17:22
 Operator : SY/MD
 Sample : 02360-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rBV	127772	143449	1.18%	0.757%
2	1.536	148	154	170	rVB	118702	142201	1.17%	0.750%
3	2.066	310	319	332	rVB	246227	357877	2.94%	1.889%
4	2.420	426	429	432	rBV5	1279	909	0.01%	0.005%
5	2.822	552	554	557	rVB4	1614	784	0.01%	0.004%
6	2.844	557	561	563	rBV5	1961	1167	0.01%	0.006%
7	2.876	567	571	573	rBV4	1723	1087	0.01%	0.006%
8	2.889	573	575	579	rVB5	1307	654	0.01%	0.003%
9	2.947	588	593	595	rBV4	1952	1507	0.01%	0.008%
10	3.002	606	610	612	rBV5	802	572	0.00%	0.003%
11	3.031	616	619	621	rVB4	928	433	0.00%	0.002%
12	3.050	621	625	626	rBV4	1002	692	0.01%	0.004%
13	3.118	643	646	648	rVV4	1262	610	0.01%	0.003%
14	3.134	648	651	653	rVB4	2218	1094	0.01%	0.006%
15	3.195	667	670	671	rBV3	971	591	0.00%	0.003%
16	3.227	676	680	682	rBV5	1501	1330	0.01%	0.007%
17	3.256	687	689	694	rVB5	1309	862	0.01%	0.005%
18	3.304	702	704	708	rBV5	901	738	0.01%	0.004%
19	3.352	717	719	722	rBV4	1156	660	0.01%	0.003%
20	3.375	724	726	731	rVB6	1742	1292	0.01%	0.007%
21	3.413	736	738	741	rVB4	1041	575	0.00%	0.003%
22	3.436	741	745	746	rBV4	1138	728	0.01%	0.004%
23	3.468	752	755	756	rBV3	1486	622	0.01%	0.003%
24	3.513	764	769	773	rVB8	1412	1162	0.01%	0.006%
25	3.532	773	775	779	rBV5	1076	785	0.01%	0.004%
26	3.568	781	786	790	rVB6	1434	1841	0.02%	0.010%
27	3.632	803	806	807	rBV2	995	549	0.00%	0.003%
28	3.642	807	809	810	rBV	1080	507	0.00%	0.003%
29	3.680	819	821	823	rVB2	1286	587	0.00%	0.003%
30	3.690	823	824	825	rBV	1406	430	0.00%	0.002%
31	3.735	836	838	839	rBV3	1123	484	0.00%	0.003%
32	3.815	849	863	888	rBV3	69133	250193	2.05%	1.320%
33	4.262	988	1002	1026	rVB	144692	367325	3.01%	1.939%
34	4.741	1148	1151	1153	rVB4	1424	780	0.01%	0.004%
35	4.754	1153	1155	1157	rBV3	1510	824	0.01%	0.004%
36	4.870	1186	1191	1192	rBV5	1188	862	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030594.D
 Acq On : 17 Apr 2023 17:22
 Operator : SY/MD
 Sample : 02360-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	4.966	1205	1221	1243	rBV2	347582	902967	7.41%	4.765%
38	5.265	1312	1314	1317	rBV4	1485	968	0.01%	0.005%
39	5.384	1348	1351	1354	rVB5	2028	1298	0.01%	0.007%
40	5.404	1354	1357	1360	rBV5	1843	1174	0.01%	0.006%
41	5.478	1376	1380	1381	rBV4	1927	1110	0.01%	0.006%
42	5.542	1388	1400	1420	rBV	299879	620661	5.09%	3.275%
43	5.841	1475	1493	1530	rBV	6357136	12183883	100.00%	64.300%
44	6.921	1819	1829	1848	rBV	105083	195501	1.60%	1.032%
45	7.252	1919	1932	1953	rBV	399184	705679	5.79%	3.724%
46	7.561	2019	2028	2044	rBV2	78139	136493	1.12%	0.720%
47	7.860	2117	2121	2123	rBV4	1688	1486	0.01%	0.008%
48	8.034	2166	2175	2206	rBV	179720	356577	2.93%	1.882%
49	8.420	2291	2295	2296	rBV3	1248	832	0.01%	0.004%
50	8.577	2342	2344	2346	rBV3	1276	584	0.00%	0.003%
51	8.793	2398	2411	2432	rBV	459912	765754	6.28%	4.041%
52	8.985	2469	2471	2473	rBV2	1234	602	0.00%	0.003%
53	9.034	2482	2486	2487	rBV4	1409	998	0.01%	0.005%
54	9.198	2535	2537	2539	rBV3	1315	532	0.00%	0.003%
55	9.307	2569	2571	2575	rVB3	2008	929	0.01%	0.005%
56	9.326	2575	2577	2581	rBV5	1784	1404	0.01%	0.007%
57	9.641	2672	2675	2678	rBV4	1385	865	0.01%	0.005%
58	9.706	2687	2695	2697	rBV8	1559	2161	0.02%	0.011%
59	9.722	2697	2700	2703	rVV5	1255	888	0.01%	0.005%
60	10.056	2799	2804	2806	rBV6	1739	1267	0.01%	0.007%
61	10.162	2826	2837	2861	rVB	262760	423713	3.48%	2.236%
62	10.419	2914	2917	2918	rBV2	1242	718	0.01%	0.004%
63	10.522	2946	2949	2953	rBV6	1503	1530	0.01%	0.008%
64	10.558	2958	2960	2962	rBV2	1396	835	0.01%	0.004%
65	10.677	2994	2997	2998	rBV4	1362	718	0.01%	0.004%
66	10.728	3009	3013	3014	rBV4	1350	876	0.01%	0.005%
67	10.789	3030	3032	3034	rBV3	1636	795	0.01%	0.004%
68	10.841	3047	3048	3051	rVB3	1473	557	0.00%	0.003%
69	10.985	3090	3093	3096	rVV5	1143	615	0.01%	0.003%
70	11.001	3096	3098	3101	rVB4	1110	508	0.00%	0.003%
71	11.043	3110	3111	3114	rBV3	1102	439	0.00%	0.002%
72	11.194	3146	3158	3176	rBV	444644	704316	5.78%	3.717%
73	11.419	3223	3228	3232	rVB7	1433	1415	0.01%	0.007%
74	11.442	3232	3235	3237	rBV3	1816	1055	0.01%	0.006%
75	11.500	3251	3253	3255	rBV3	1899	982	0.01%	0.005%
76	11.571	3264	3275	3293	rVB	390600	616731	5.06%	3.255%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030594.D
 Acq On : 17 Apr 2023 17:22
 Operator : SY/MD
 Sample : 02360-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.709	3316	3318	3319	rBV2	1288	452	0.00%	0.002%
78	11.857	3362	3364	3366	rBV2	1184	648	0.01%	0.003%
79	12.075	3429	3432	3434	rBV4	1333	825	0.01%	0.004%
80	12.127	3445	3448	3452	rBV7	1250	1016	0.01%	0.005%
81	12.268	3489	3492	3493	rBV3	1113	557	0.00%	0.003%
82	12.349	3513	3517	3519	rBV4	1448	1180	0.01%	0.006%
83	12.384	3526	3528	3534	rBV7	1239	1229	0.01%	0.006%
84	12.522	3568	3571	3578	rBV7	2572	3233	0.03%	0.017%
85	12.796	3654	3656	3659	rVB4	1103	601	0.00%	0.003%
86	12.841	3668	3670	3672	rBV3	1069	515	0.00%	0.003%
87	12.995	3716	3718	3720	rBV3	1200	429	0.00%	0.002%
88	13.117	3755	3756	3760	rVB4	1051	583	0.00%	0.003%
89	13.143	3761	3764	3766	rBV3	1447	796	0.01%	0.004%
90	13.188	3776	3778	3782	rBV4	1327	1118	0.01%	0.006%
91	13.407	3844	3846	3847	rBV2	1079	447	0.00%	0.002%
92	13.567	3893	3896	3897	rBV4	805	444	0.00%	0.002%
93	13.738	3946	3949	3952	rBV4	1822	1470	0.01%	0.008%
94	13.886	3993	3995	3998	rBV4	1548	766	0.01%	0.004%
95	13.963	4017	4019	4022	rVB5	1137	569	0.00%	0.003%
96	13.988	4025	4027	4028	rBV2	1312	500	0.00%	0.003%
97	14.024	4036	4038	4041	rBV4	1056	463	0.00%	0.002%
98	14.313	4127	4128	4133	rBV4	1071	1021	0.01%	0.005%
99	14.786	4272	4275	4277	rBV3	1657	1166	0.01%	0.006%
100	15.548	4509	4512	4513	rBV3	2492	1395	0.01%	0.007%




Sum of corrected areas: 18948602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030594.D
Acq On : 17 Apr 2023 17:22
Operator : SY/MD
Sample : 02360-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

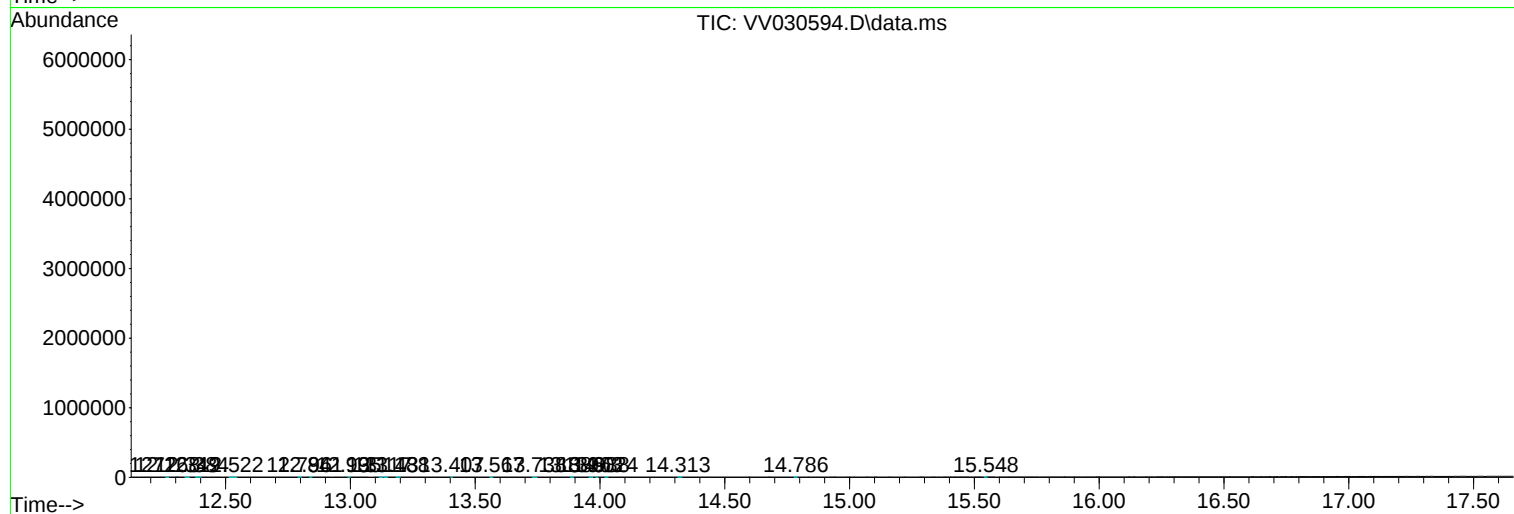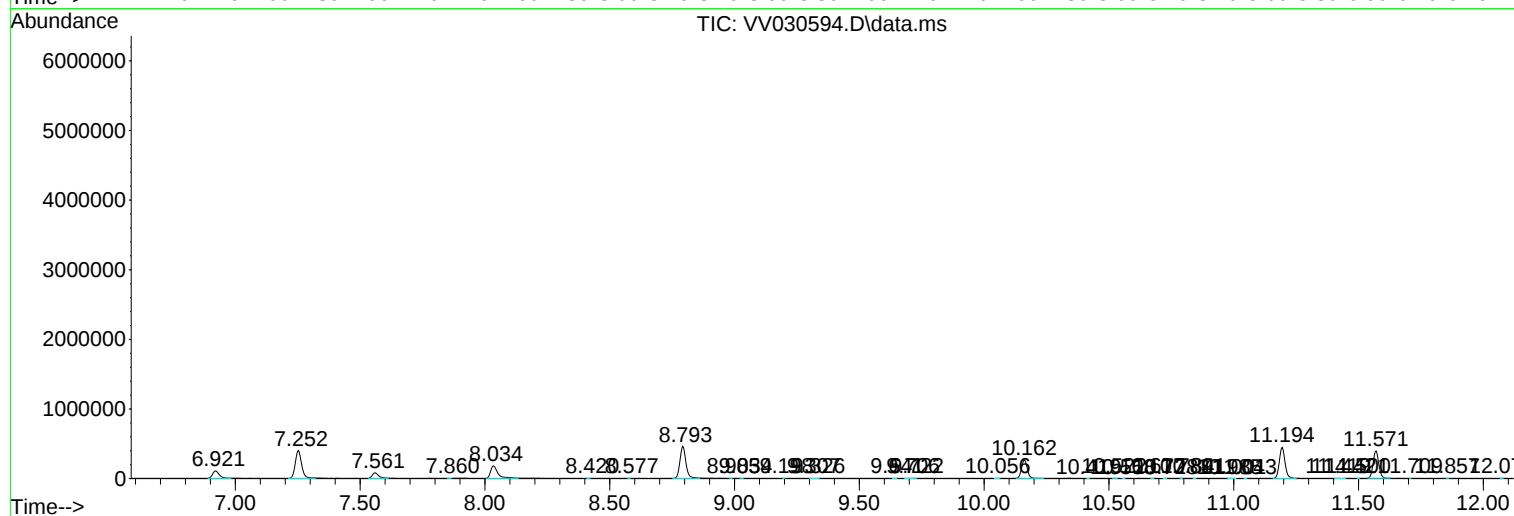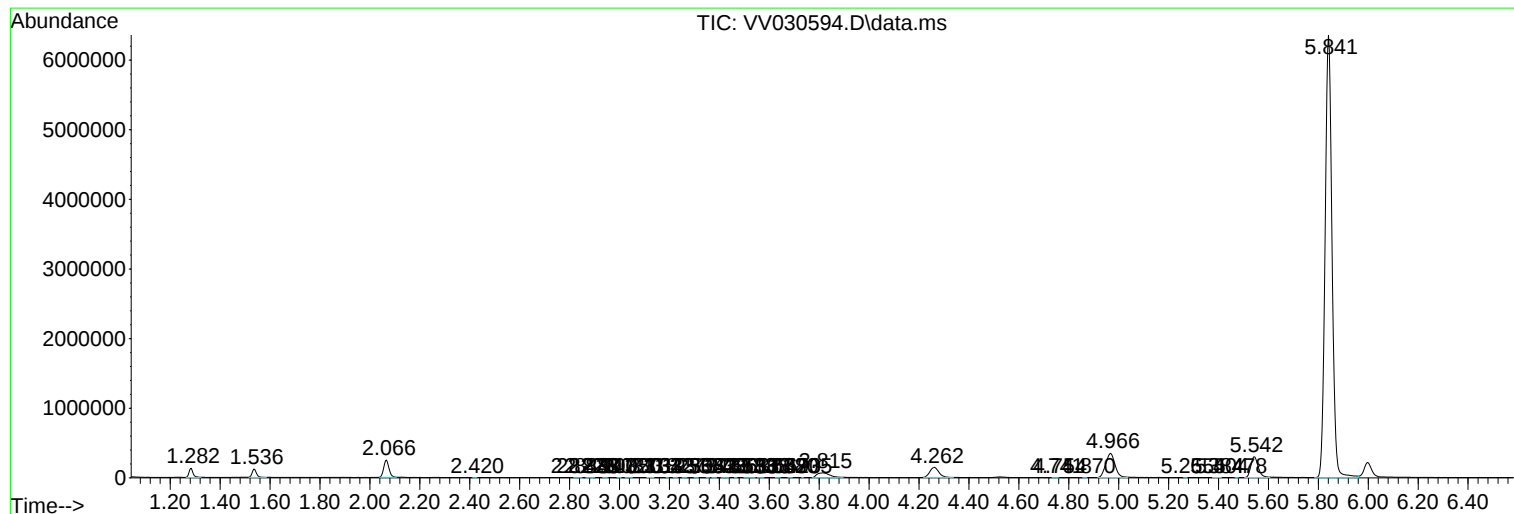

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030594.D
Acq On : 17 Apr 2023 17:22
Operator : SY/MD
Sample : 02360-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030594.D
Acq On : 17 Apr 2023 17:22
Operator : SY/MD
Sample : 02360-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------