

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030595.D
 Acq On : 17 Apr 2023 17:46
 Operator : SY/MD
 Sample : 02360-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030595.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	95	rVB	127437	143091	0.86%	0.615%
2	1.535	148	154	169	rVB	115615	136776	0.83%	0.588%
3	2.066	309	319	335	rBV	247171	370639	2.24%	1.594%
4	2.577	473	478	483	rBV7	1352	1894	0.01%	0.008%
5	2.670	506	507	510	rVB3	773	336	0.00%	0.001%
6	2.690	510	513	514	rBV3	1954	1210	0.01%	0.005%
7	2.725	521	524	527	rVB5	2224	1419	0.01%	0.006%
8	2.764	534	536	538	rBV3	1347	620	0.00%	0.003%
9	2.918	580	584	587	rBV5	2126	1765	0.01%	0.008%
10	2.976	598	602	606	rBV5	1696	1733	0.01%	0.007%
11	3.021	614	616	618	rBV2	893	510	0.00%	0.002%
12	3.056	622	627	630	rVB5	1999	2018	0.01%	0.009%
13	3.079	630	634	635	rBV3	2014	1207	0.01%	0.005%
14	3.198	669	671	673	rBV3	1252	471	0.00%	0.002%
15	3.387	728	730	735	rBV6	1510	879	0.01%	0.004%
16	3.420	737	740	743	rBV5	1682	1129	0.01%	0.005%
17	3.519	769	771	773	rBV4	1099	469	0.00%	0.002%
18	3.568	784	786	787	rBV2	882	323	0.00%	0.001%
19	3.613	795	800	801	rBV4	1199	898	0.01%	0.004%
20	3.696	823	826	828	rBV4	1178	908	0.01%	0.004%
21	3.805	850	860	898	rBV3	55974	194438	1.17%	0.836%
22	4.156	967	969	971	rBV3	1379	715	0.00%	0.003%
23	4.259	987	1001	1020	rBV	142189	366278	2.21%	1.575%
24	4.680	1131	1132	1133	rBV	768	168	0.00%	0.001%
25	4.786	1163	1165	1169	rBV5	1285	956	0.01%	0.004%
26	4.828	1176	1178	1181	rBV3	1449	1012	0.01%	0.004%
27	4.892	1196	1198	1202	rVB4	2038	977	0.01%	0.004%
28	4.966	1204	1221	1243	rBV2	333478	888477	5.36%	3.822%
29	5.458	1372	1374	1375	rBV2	2126	912	0.01%	0.004%
30	5.542	1388	1400	1423	rBV	308493	632884	3.82%	2.722%
31	5.841	1478	1493	1528	rBV	8742941	16577784	100.00%	71.305%
32	6.526	1704	1706	1708	rBV3	1330	656	0.00%	0.003%
33	6.921	1818	1829	1857	rBV	103221	201629	1.22%	0.867%
34	7.252	1920	1932	1959	rBV	385135	688309	4.15%	2.961%
35	7.561	2018	2028	2047	rBV	76572	141394	0.85%	0.608%
36	8.034	2165	2175	2205	rBV	173128	349324	2.11%	1.503%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030595.D
 Acq On : 17 Apr 2023 17:46
 Operator : SY/MD
 Sample : 02360-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.387	2281	2285	2286	rBV4	1391	777	0.00%	0.003%
38	8.686	2376	2378	2380	rBV3	1732	981	0.01%	0.004%
39	8.792	2400	2411	2430	rBV	469617	771612	4.65%	3.319%
40	9.130	2514	2516	2517	rBV2	1464	464	0.00%	0.002%
41	9.484	2624	2626	2629	rBV3	1056	875	0.01%	0.004%
42	9.654	2677	2679	2680	rVB2	1215	441	0.00%	0.002%
43	9.664	2680	2682	2684	rBV2	874	306	0.00%	0.001%
44	9.853	2739	2741	2742	rBV2	1063	312	0.00%	0.001%
45	10.162	2826	2837	2851	rBV	249227	401504	2.42%	1.727%
46	10.291	2873	2877	2879	rBV4	1123	919	0.01%	0.004%
47	10.336	2882	2891	2892	rBV8	3195	4035	0.02%	0.017%
48	10.371	2900	2902	2903	rBV3	1017	356	0.00%	0.002%
49	10.413	2912	2915	2916	rBV3	1334	824	0.00%	0.004%
50	10.873	3056	3058	3059	rBV3	1718	693	0.00%	0.003%
51	10.963	3084	3086	3088	rBV3	1248	609	0.00%	0.003%
52	11.030	3105	3107	3110	rBV4	1431	854	0.01%	0.004%
53	11.078	3116	3122	3124	rBV6	1674	1593	0.01%	0.007%
54	11.194	3147	3158	3179	rBV	454763	717741	4.33%	3.087%
55	11.336	3198	3202	3204	rBV5	1623	1130	0.01%	0.005%
56	11.570	3264	3275	3294	rVB	383751	604390	3.65%	2.600%
57	11.873	3366	3369	3371	rBV4	1596	863	0.01%	0.004%
58	11.972	3399	3400	3401	rBV	1026	269	0.00%	0.001%
59	12.017	3410	3414	3416	rBV4	1007	967	0.01%	0.004%
60	12.059	3423	3427	3428	rBV3	1486	801	0.00%	0.003%
61	12.091	3435	3437	3439	rVB3	1024	401	0.00%	0.002%
62	12.133	3446	3450	3452	rBV5	1869	1470	0.01%	0.006%
63	12.275	3492	3494	3495	rBV2	1024	291	0.00%	0.001%
64	12.345	3510	3516	3517	rBV5	2449	1853	0.01%	0.008%
65	12.416	3535	3538	3540	rBV3	1786	1304	0.01%	0.006%
66	12.522	3569	3571	3575	rVB4	2199	1278	0.01%	0.005%
67	12.541	3575	3577	3579	rBV2	1218	654	0.00%	0.003%
68	12.734	3635	3637	3638	rBV2	1014	349	0.00%	0.002%
69	12.766	3644	3647	3650	rBV3	1702	1080	0.01%	0.005%
70	12.792	3653	3655	3656	rBV2	1177	447	0.00%	0.002%
71	12.898	3687	3688	3693	rBV5	1583	970	0.01%	0.004%
72	12.937	3699	3700	3704	rVB4	1624	651	0.00%	0.003%
73	12.959	3704	3707	3709	rBV3	1226	715	0.00%	0.003%
74	12.992	3713	3717	3718	rBV3	1252	876	0.01%	0.004%
75	13.213	3784	3786	3787	rBV2	1638	570	0.00%	0.002%
76	13.371	3830	3835	3836	rBV4	1638	1494	0.01%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030595.D
 Acq On : 17 Apr 2023 17:46
 Operator : SY/MD
 Sample : 02360-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

77	13.426	3849	3852	3854	rBV3	1255	947	0.01%	0.004%
78	13.644	3918	3920	3921	rBV2	740	165	0.00%	0.001%
79	13.657	3922	3924	3925	rBV2	1181	438	0.00%	0.002%
80	13.689	3931	3934	3937	rBV5	1620	1333	0.01%	0.006%
81	13.779	3959	3962	3963	rBV3	1320	607	0.00%	0.003%
82	14.069	4049	4052	4056	rBV5	1593	1454	0.01%	0.006%
83	14.139	4072	4074	4076	rBV2	1594	697	0.00%	0.003%
84	14.313	4126	4128	4131	rBV4	1506	999	0.01%	0.004%
85	14.345	4136	4138	4139	rBV2	1317	482	0.00%	0.002%




Sum of corrected areas: 23249049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030595.D
Acq On : 17 Apr 2023 17:46
Operator : SY/MD
Sample : 02360-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

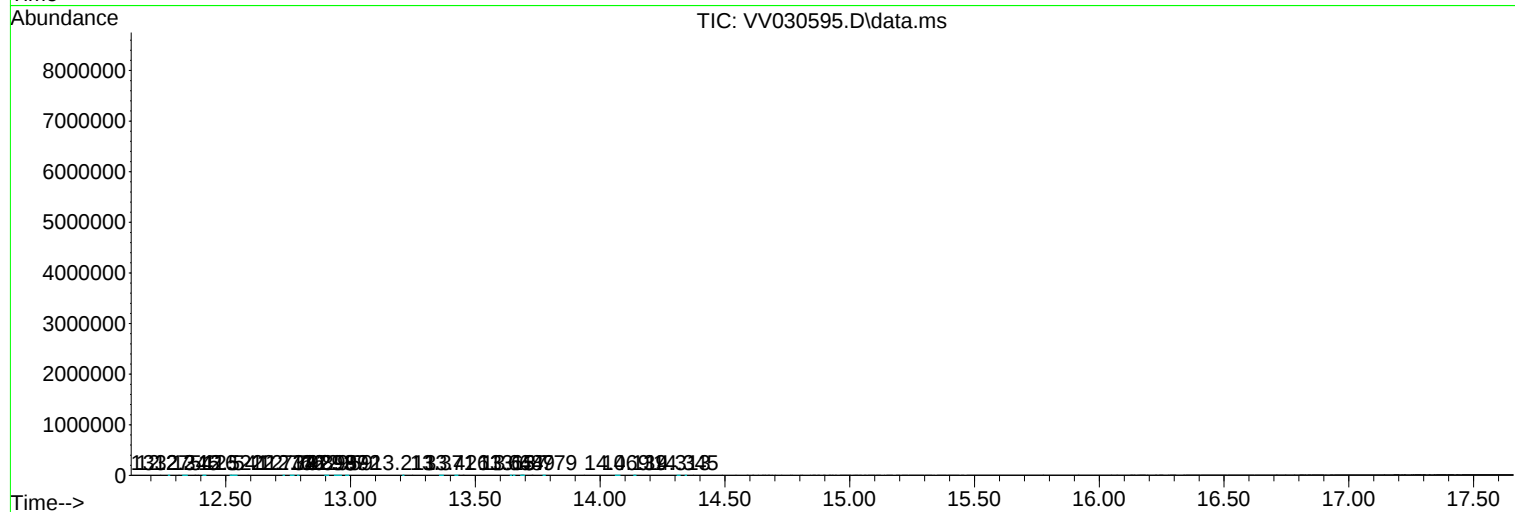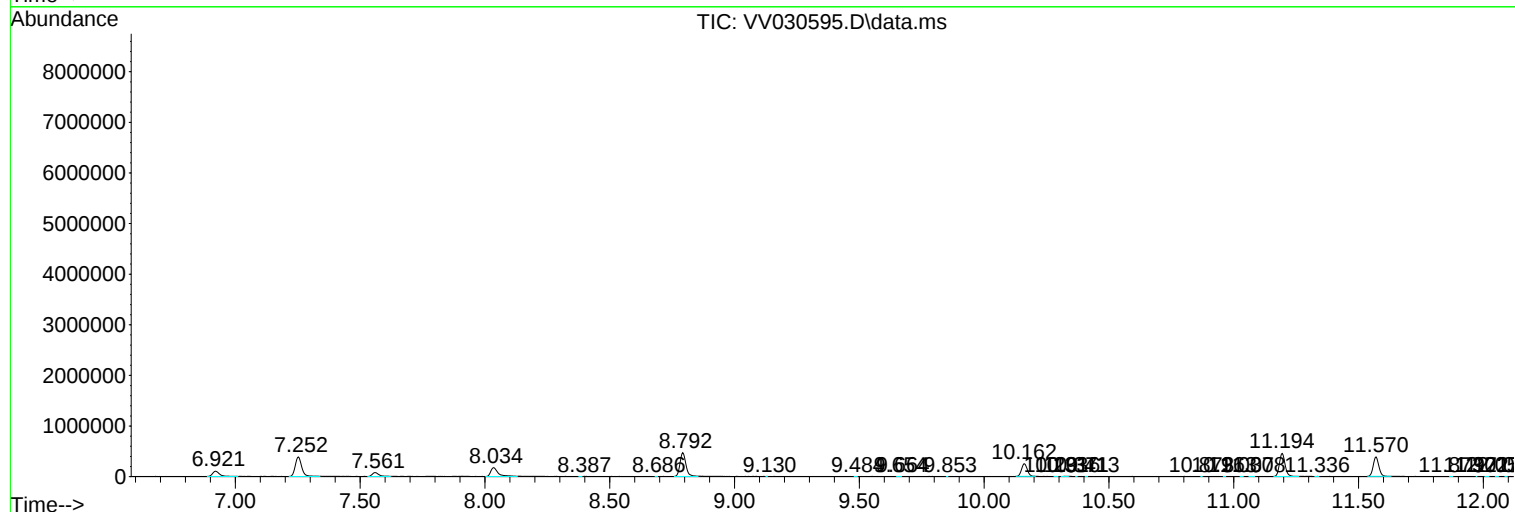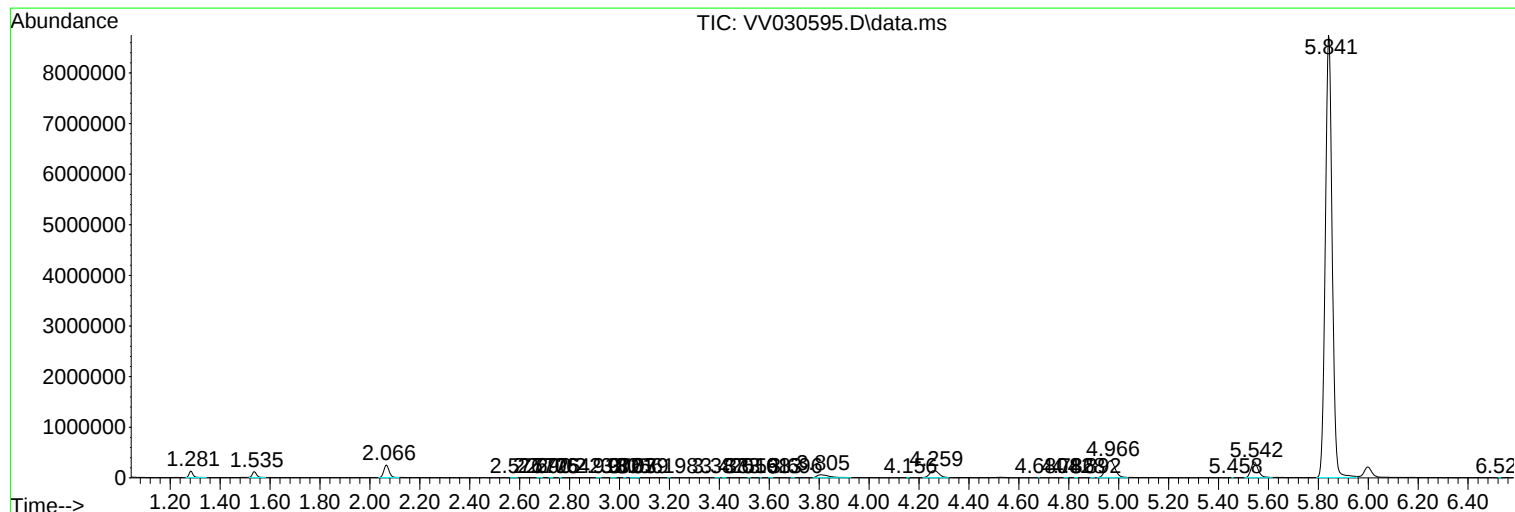

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030595.D
Acq On : 17 Apr 2023 17:46
Operator : SY/MD
Sample : 02360-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030595.D
Acq On : 17 Apr 2023 17:46
Operator : SY/MD
Sample : 02360-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------