

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030599.D
 Acq On : 17 Apr 2023 19:25
 Operator : SY/MD
 Sample : 02360-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	70	75	92	rVB	119460	134674	3.20%	1.240%
2	1.535	148	154	172	rVB	121063	149857	3.56%	1.380%
3	2.066	310	319	335	rVB2	228483	344716	8.20%	3.174%
4	2.687	509	512	515	rBV5	2598	2414	0.06%	0.022%
5	2.780	539	541	542	rBV2	1588	696	0.02%	0.006%
6	2.937	586	590	595	rVB8	1770	1955	0.05%	0.018%
7	2.960	595	597	600	rBV3	1470	903	0.02%	0.008%
8	3.069	628	631	633	rBV4	1371	931	0.02%	0.009%
9	3.246	685	686	690	rVV4	1269	706	0.02%	0.006%
10	3.352	715	719	720	rBV4	1804	996	0.02%	0.009%
11	3.432	741	744	748	rVB6	1318	976	0.02%	0.009%
12	3.455	748	751	752	rBV3	1153	809	0.02%	0.007%
13	3.500	761	765	766	rBV5	1245	798	0.02%	0.007%
14	3.571	783	787	789	rBV5	1283	1037	0.02%	0.010%
15	3.587	789	792	797	rVB7	1616	1479	0.04%	0.014%
16	3.822	850	865	888	rBV4	121563	380554	9.05%	3.504%
17	4.172	971	974	976	rVB4	1755	885	0.02%	0.008%
18	4.259	984	1001	1026	rBV	131828	349103	8.30%	3.214%
19	4.471	1063	1067	1068	rBV3	1705	1255	0.03%	0.012%
20	4.674	1128	1130	1131	rBV2	1493	732	0.02%	0.007%
21	4.796	1165	1168	1172	rBV5	1745	1304	0.03%	0.012%
22	4.966	1205	1221	1248	rBV2	307943	814267	19.36%	7.496%
23	5.455	1370	1373	1377	rBV5	2008	1455	0.03%	0.013%
24	5.542	1386	1400	1425	rBV	288832	611232	14.54%	5.627%
25	5.841	1479	1493	1526	rBV	2161945	4205134	100.00%	38.714%
26	5.998	1534	1542	1557	rVB2	178177	348214	8.28%	3.206%
27	6.326	1640	1644	1648	rVB7	1503	1178	0.03%	0.011%
28	6.368	1655	1657	1660	rVB5	1635	737	0.02%	0.007%
29	6.416	1669	1672	1674	rBV3	1519	888	0.02%	0.008%
30	6.516	1701	1703	1707	rVB5	1741	1333	0.03%	0.012%
31	6.844	1801	1805	1806	rBV3	1195	839	0.02%	0.008%
32	6.921	1817	1829	1848	rBV2	92566	179564	4.27%	1.653%
33	7.252	1921	1932	1952	rBV	345617	607251	14.44%	5.591%
34	7.561	2019	2028	2047	rBV	65978	117256	2.79%	1.080%
35	8.037	2166	2176	2202	rBV	148378	303641	7.22%	2.795%
36	8.320	2262	2264	2270	rVB8	2520	1803	0.04%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030599.D
 Acq On : 17 Apr 2023 19:25
 Operator : SY/MD
 Sample : 02360-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.371	2277	2280	2282	rBV4	1266	708	0.02%	0.007%
38	8.384	2282	2284	2287	rVB3	2112	1248	0.03%	0.011%
39	8.519	2322	2326	2330	rBV6	1851	1840	0.04%	0.017%
40	8.599	2348	2351	2356	rVB6	1735	1251	0.03%	0.012%
41	8.628	2356	2360	2361	rBV3	1355	1039	0.02%	0.010%
42	8.735	2389	2393	2394	rBV4	1237	919	0.02%	0.008%
43	8.792	2400	2411	2434	rBV	426430	709944	16.88%	6.536%
44	9.172	2527	2529	2532	rBV4	1326	983	0.02%	0.009%
45	9.307	2566	2571	2575	rBV8	1561	1709	0.04%	0.016%
46	9.371	2587	2591	2594	rBV5	1868	1872	0.04%	0.017%
47	9.532	2638	2641	2644	rBV5	2002	1602	0.04%	0.015%
48	9.577	2652	2655	2658	rBV5	1780	1129	0.03%	0.010%
49	9.773	2714	2716	2719	rBV3	1142	833	0.02%	0.008%
50	9.824	2729	2732	2733	rBV4	1381	991	0.02%	0.009%
51	9.921	2758	2762	2764	rBV4	1239	878	0.02%	0.008%
52	9.943	2767	2769	2772	rBV4	1471	931	0.02%	0.009%
53	10.082	2810	2812	2816	rVB4	1604	903	0.02%	0.008%
54	10.107	2816	2820	2822	rBV5	1220	702	0.02%	0.006%
55	10.120	2822	2824	2826	rVV4	1881	1210	0.03%	0.011%
56	10.162	2826	2837	2863	rVB	229715	376217	8.95%	3.464%
57	10.287	2874	2876	2879	rVB4	1496	875	0.02%	0.008%
58	10.403	2910	2912	2917	rBV6	1280	1160	0.03%	0.011%
59	10.448	2924	2926	2928	rBV3	1615	866	0.02%	0.008%
60	10.545	2954	2956	2958	rBV3	1306	732	0.02%	0.007%
61	10.648	2985	2988	2990	rBV3	2202	1250	0.03%	0.012%
62	10.767	3023	3025	3029	rVB5	1362	846	0.02%	0.008%
63	10.792	3029	3033	3038	rBV7	2180	1945	0.05%	0.018%
64	10.815	3038	3040	3043	rBV4	1793	919	0.02%	0.008%
65	10.902	3064	3067	3069	rBV3	1514	770	0.02%	0.007%
66	11.046	3108	3112	3113	rBV4	1156	816	0.02%	0.008%
67	11.062	3115	3117	3120	rBV3	1128	756	0.02%	0.007%
68	11.194	3147	3158	3176	rBV	387522	608245	14.46%	5.600%
69	11.432	3230	3232	3234	rBV3	1367	795	0.02%	0.007%
70	11.570	3262	3275	3298	rVV	329566	528797	12.58%	4.868%
71	11.677	3306	3308	3312	rBV5	1548	870	0.02%	0.008%
72	11.792	3342	3344	3347	rBV2	1406	1049	0.02%	0.010%
73	11.824	3352	3354	3357	rVV5	1338	728	0.02%	0.007%
74	11.934	3384	3388	3389	rBV4	1638	982	0.02%	0.009%
75	12.059	3423	3427	3430	rBV5	1163	905	0.02%	0.008%
76	12.130	3445	3449	3451	rBV4	1374	853	0.02%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030599.D
 Acq On : 17 Apr 2023 19:25
 Operator : SY/MD
 Sample : 02360-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.159	3455	3458	3461	rBV5	2004	1188	0.03%	0.011%
78	12.303	3499	3503	3506	rBV6	1332	1218	0.03%	0.011%
79	12.419	3534	3539	3540	rBV5	2970	2201	0.05%	0.020%
80	12.577	3585	3588	3590	rVB2	1292	779	0.02%	0.007%
81	12.625	3601	3603	3609	rVB6	1827	1695	0.04%	0.016%
82	12.667	3609	3616	3618	rBV7	1305	1204	0.03%	0.011%
83	12.728	3633	3635	3639	rVB4	1162	760	0.02%	0.007%
84	12.750	3639	3642	3643	rBV4	1933	1010	0.02%	0.009%
85	12.857	3672	3675	3677	rBV3	1616	1045	0.02%	0.010%
86	13.008	3720	3722	3725	rBV3	1263	834	0.02%	0.008%
87	13.027	3725	3728	3734	rVB6	1778	1660	0.04%	0.015%
88	13.056	3734	3737	3739	rVB3	1695	999	0.02%	0.009%
89	13.072	3739	3742	3744	rBV3	1613	1247	0.03%	0.011%
90	13.127	3755	3759	3762	rBV6	1362	1059	0.03%	0.010%
91	13.204	3780	3783	3785	rBV4	1663	696	0.02%	0.006%
92	13.217	3785	3787	3790	rVV4	1584	857	0.02%	0.008%
93	13.287	3807	3809	3812	rVB4	1944	978	0.02%	0.009%
94	13.342	3823	3826	3829	rVB3	1597	1080	0.03%	0.010%
95	13.358	3829	3831	3834	rBV4	1425	787	0.02%	0.007%
96	13.390	3838	3841	3843	rVV4	1966	1243	0.03%	0.011%
97	13.670	3924	3928	3929	rVV3	1770	878	0.02%	0.008%
98	14.220	4095	4099	4101	rBV4	1599	1309	0.03%	0.012%
99	14.602	4215	4218	4219	rBV3	1261	779	0.02%	0.007%
100	15.210	4399	4407	4410	rBV10	2416	3834	0.09%	0.035%




Sum of corrected areas: 10861980

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030599.D
Acq On : 17 Apr 2023 19:25
Operator : SY/MD
Sample : 02360-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

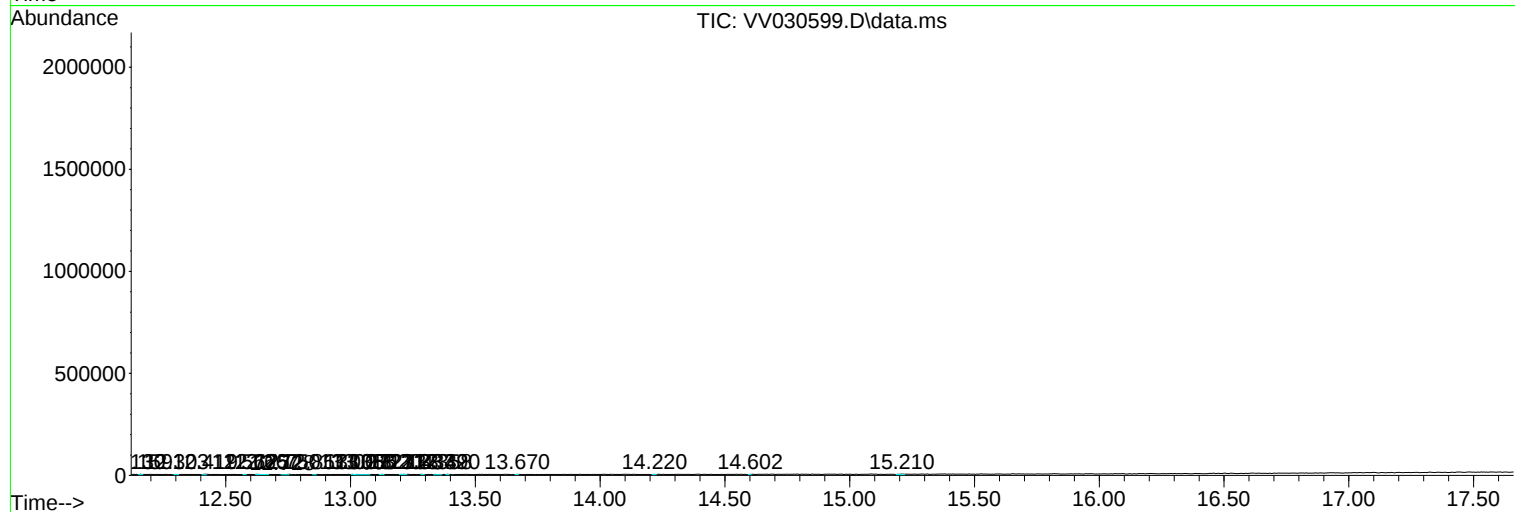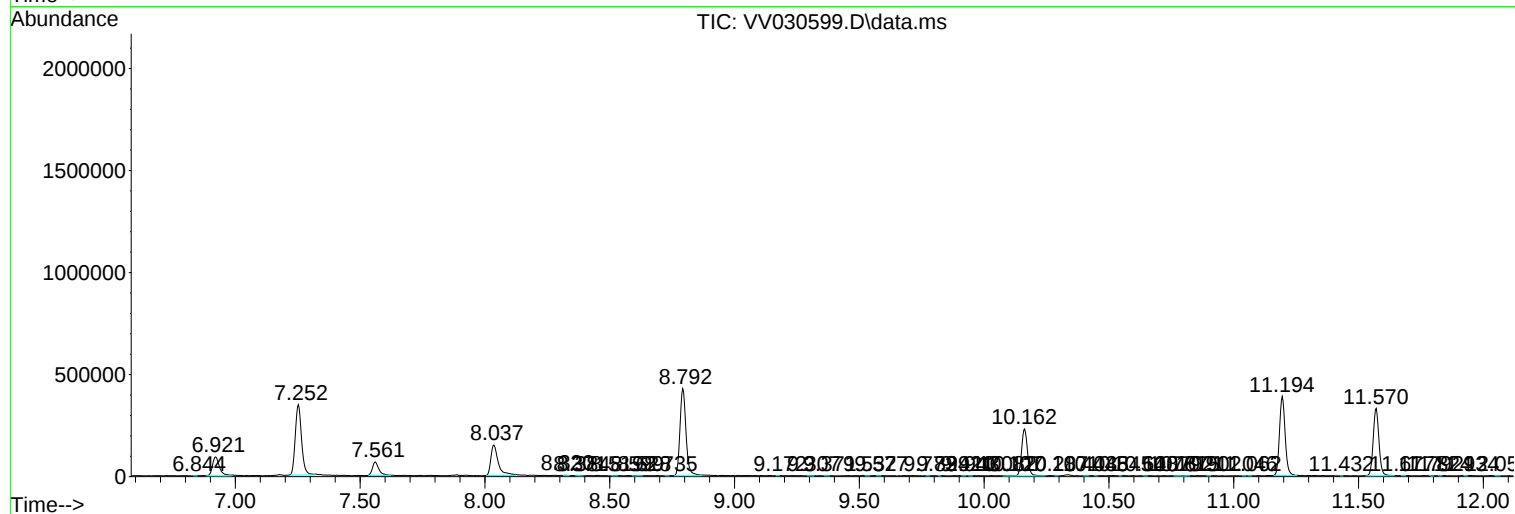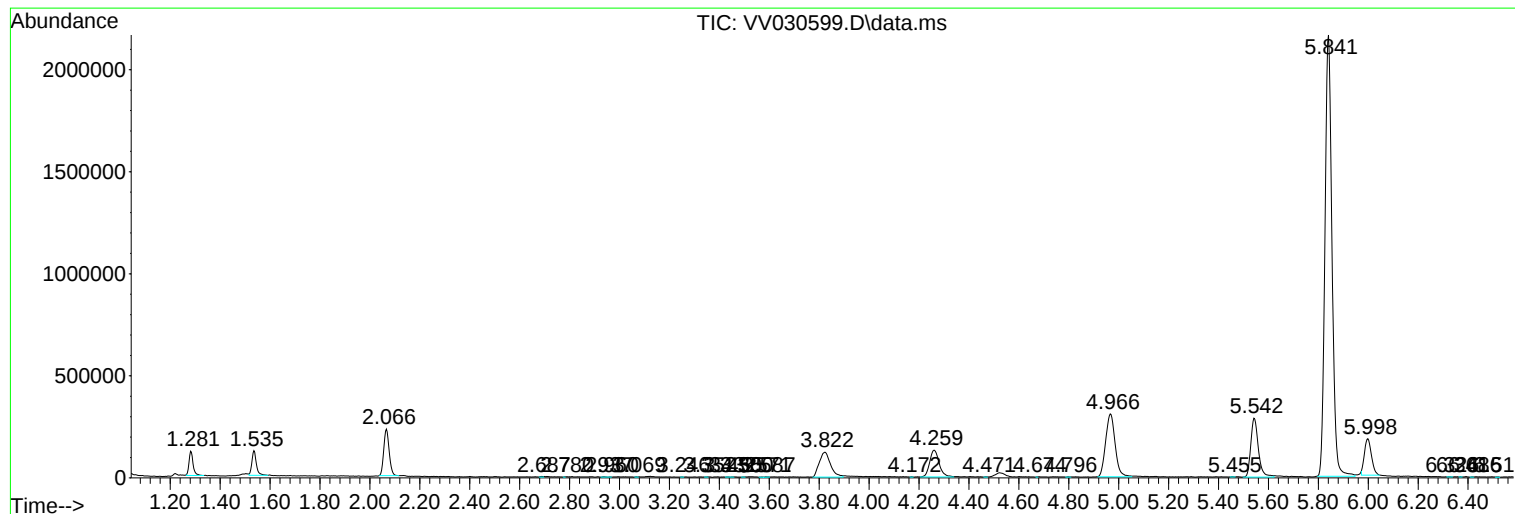

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030599.D
Acq On : 17 Apr 2023 19:25
Operator : SY/MD
Sample : 02360-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030599.D
Acq On : 17 Apr 2023 19:25
Operator : SY/MD
Sample : 02360-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc