

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030600.D
 Acq On : 17 Apr 2023 19:48
 Operator : SY/MD
 Sample : 02360-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	52	56	64	rBV	11885	13629	1.63%	0.188%
2	1.281	70	75	93	rVB	118408	138828	16.61%	1.915%
3	1.536	148	154	169	rVB	118355	143247	17.14%	1.976%
4	2.066	310	319	333	rBV	218243	314092	37.59%	4.332%
5	2.233	369	371	372	rBV2	1734	711	0.09%	0.010%
6	2.683	509	511	513	rBV4	1166	479	0.06%	0.007%
7	2.735	524	527	533	rBV7	1838	1604	0.19%	0.022%
8	2.831	555	557	558	rBV2	2110	791	0.09%	0.011%
9	2.957	593	596	598	rVB3	1475	934	0.11%	0.013%
10	2.982	600	604	606	rVV4	1499	789	0.09%	0.011%
11	3.252	685	688	689	rBV4	986	508	0.06%	0.007%
12	3.317	705	708	710	rBV4	1769	1230	0.15%	0.017%
13	3.423	739	741	744	rBV3	1251	607	0.07%	0.008%
14	3.494	761	763	765	rBV3	1018	356	0.04%	0.005%
15	3.574	784	788	790	rBV5	1295	737	0.09%	0.010%
16	3.593	791	794	797	rVB6	1513	936	0.11%	0.013%
17	3.616	797	801	803	rBV4	1207	1015	0.12%	0.014%
18	3.629	803	805	810	rVV5	998	861	0.10%	0.012%
19	3.654	810	813	819	rVV8	1772	1408	0.17%	0.019%
20	3.802	850	859	879	rBV	48084	138058	16.52%	1.904%
21	4.047	932	935	937	rBV4	1782	1111	0.13%	0.015%
22	4.085	944	947	951	rBV6	2292	1546	0.19%	0.021%
23	4.262	990	1002	1025	rVB	134632	334039	39.98%	4.607%
24	4.542	1087	1089	1092	rBV4	1104	611	0.07%	0.008%
25	4.635	1115	1118	1119	rBV3	1182	586	0.07%	0.008%
26	4.760	1156	1157	1159	rBV2	842	414	0.05%	0.006%
27	4.854	1182	1186	1188	rBV5	1482	1310	0.16%	0.018%
28	4.966	1205	1221	1242	rBV2	315732	835575	100.00%	11.524%
29	5.339	1335	1337	1340	rBV4	1899	797	0.10%	0.011%
30	5.474	1375	1379	1383	rVB7	2046	1875	0.22%	0.026%
31	5.494	1383	1385	1386	rBV2	1303	599	0.07%	0.008%
32	5.542	1388	1400	1423	rBV	289194	610004	73.00%	8.413%
33	5.776	1470	1473	1475	rBV3	1636	1123	0.13%	0.015%
34	5.841	1481	1493	1517	rBV	352295	702319	84.05%	9.686%
35	5.998	1532	1542	1560	rVB	189703	375374	44.92%	5.177%
36	6.288	1630	1632	1638	rVB6	2085	1639	0.20%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030600.D
 Acq On : 17 Apr 2023 19:48
 Operator : SY/MD
 Sample : 02360-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.339	1646	1648	1649	rBV2	994	409	0.05%	0.006%
38	6.584	1722	1724	1728	rBV5	1375	633	0.08%	0.009%
39	6.696	1756	1759	1763	rBV6	2220	1204	0.14%	0.017%
40	6.921	1818	1829	1844	rBV	92810	174739	20.91%	2.410%
41	7.104	1882	1886	1888	rBV5	1503	1167	0.14%	0.016%
42	7.117	1888	1890	1893	rVV3	1419	940	0.11%	0.013%
43	7.178	1907	1909	1910	rBV2	2160	901	0.11%	0.012%
44	7.252	1920	1932	1952	rBV	356997	638400	76.40%	8.804%
45	7.561	2019	2028	2049	rBV	67210	122048	14.61%	1.683%
46	7.670	2061	2062	2064	rBV2	1350	531	0.06%	0.007%
47	7.837	2112	2114	2116	rBV3	1312	806	0.10%	0.011%
48	8.034	2166	2175	2205	rBV	157881	324785	38.87%	4.479%
49	8.792	2400	2411	2433	rBV	433219	727299	87.04%	10.030%
50	9.497	2628	2630	2633	rVB4	1762	811	0.10%	0.011%
51	9.522	2633	2638	2639	rBV5	2001	1593	0.19%	0.022%
52	9.628	2668	2671	2673	rBV4	1408	1159	0.14%	0.016%
53	9.654	2677	2679	2680	rBV2	1171	501	0.06%	0.007%
54	9.731	2700	2703	2705	rBV3	1966	1035	0.12%	0.014%
55	9.911	2757	2759	2760	rBV3	810	224	0.03%	0.003%
56	9.940	2767	2768	2770	rBV2	399	185	0.02%	0.003%
57	9.960	2770	2774	2777	rBV4	1899	1715	0.21%	0.024%
58	10.005	2787	2788	2790	rBV2	1081	339	0.04%	0.005%
59	10.046	2798	2801	2802	rBV3	1330	750	0.09%	0.010%
60	10.069	2806	2808	2811	rVB4	1453	767	0.09%	0.011%
61	10.095	2814	2816	2818	rBV2	1573	671	0.08%	0.009%
62	10.162	2824	2837	2854	rBV	245474	391880	46.90%	5.405%
63	10.278	2871	2873	2875	rBV3	1724	685	0.08%	0.009%
64	10.548	2952	2957	2958	rBV5	1899	1647	0.20%	0.023%
65	10.612	2974	2977	2979	rBV3	1976	1093	0.13%	0.015%
66	10.644	2984	2987	2992	rVV6	1266	1438	0.17%	0.020%
67	10.699	3001	3004	3007	rVB5	1460	1089	0.13%	0.015%
68	10.715	3007	3009	3010	rBV2	1222	585	0.07%	0.008%
69	10.857	3051	3053	3054	rBV2	1141	405	0.05%	0.006%
70	11.043	3109	3111	3112	rBV2	1174	480	0.06%	0.007%
71	11.194	3146	3158	3174	rBV	408978	641603	76.79%	8.849%
72	11.458	3238	3240	3242	rBV3	978	575	0.07%	0.008%
73	11.570	3264	3275	3292	rBV	338756	541357	64.79%	7.466%
74	12.030	3416	3418	3419	rBV2	1219	563	0.07%	0.008%
75	12.059	3425	3427	3430	rVB4	1864	968	0.12%	0.013%
76	12.207	3471	3473	3475	rVB3	1822	597	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030600.D
 Acq On : 17 Apr 2023 19:48
 Operator : SY/MD
 Sample : 02360-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.300	3495	3502	3509	rBV7	11376	16761	2.01%	0.231%
78	12.384	3526	3528	3530	rBV3	1068	609	0.07%	0.008%
79	12.464	3551	3553	3555	rBV3	1307	774	0.09%	0.011%
80	12.705	3625	3628	3629	rBV3	976	601	0.07%	0.008%
81	13.037	3729	3731	3732	rBV2	1366	608	0.07%	0.008%
82	13.056	3735	3737	3739	rBV2	1612	961	0.12%	0.013%
83	13.082	3743	3745	3750	rVB5	1800	1144	0.14%	0.016%
84	13.104	3750	3752	3753	rBV2	1172	438	0.05%	0.006%
85	13.313	3815	3817	3818	rBV2	638	224	0.03%	0.003%
86	13.352	3825	3829	3830	rBV3	1342	905	0.11%	0.012%
87	13.570	3894	3897	3899	rBV4	2041	992	0.12%	0.014%
88	13.664	3922	3926	3929	rBV5	1399	1409	0.17%	0.019%
89	13.734	3946	3948	3949	rBV2	1368	581	0.07%	0.008%
90	13.853	3982	3985	3989	rBV4	1556	882	0.11%	0.012%
91	13.918	4002	4005	4008	rBV5	1490	1080	0.13%	0.015%
92	13.937	4009	4011	4015	rVV5	1065	768	0.09%	0.011%
93	14.043	4042	4044	4047	rBV2	1710	1040	0.12%	0.014%
94	14.654	4232	4234	4236	rBV3	1670	649	0.08%	0.009%
95	14.731	4256	4258	4261	rBV3	1538	994	0.12%	0.014%
96	15.162	4389	4392	4393	rBV3	1887	1165	0.14%	0.016%




Sum of corrected areas: 7250904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030600.D
Acq On : 17 Apr 2023 19:48
Operator : SY/MD
Sample : 02360-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

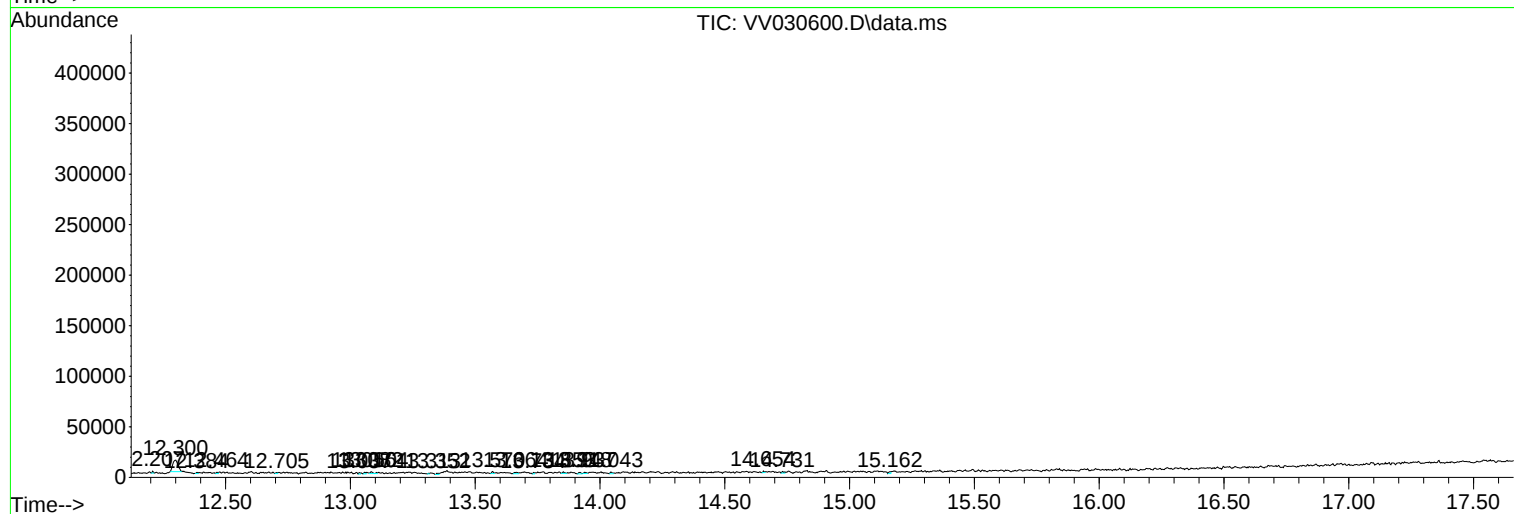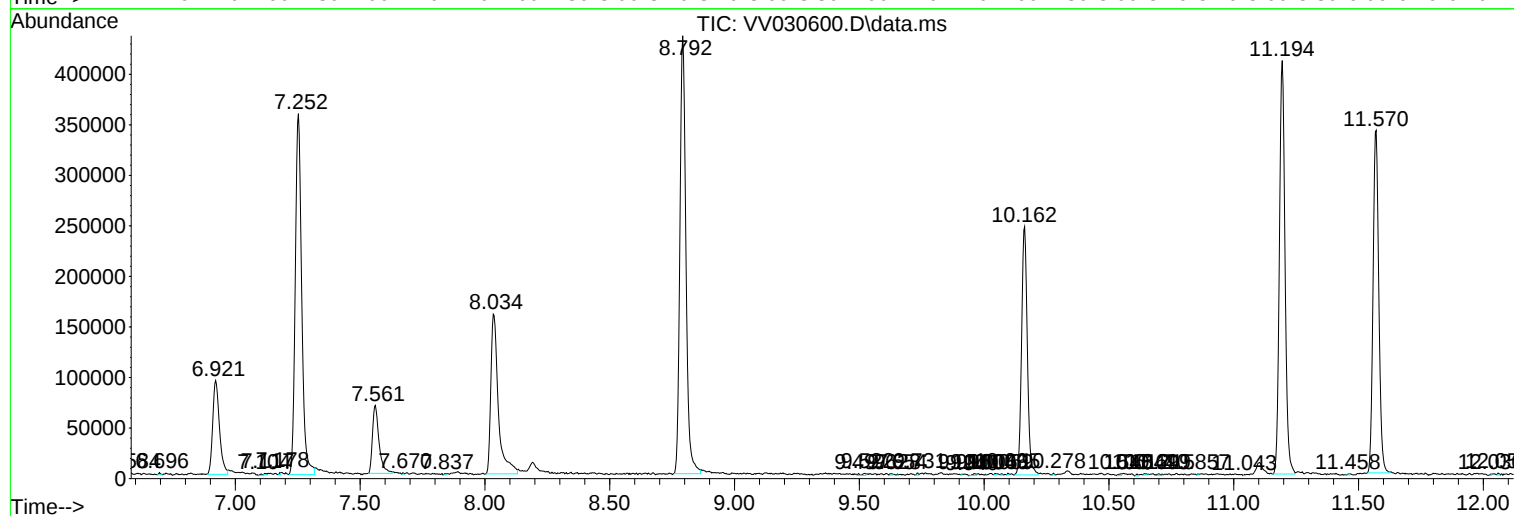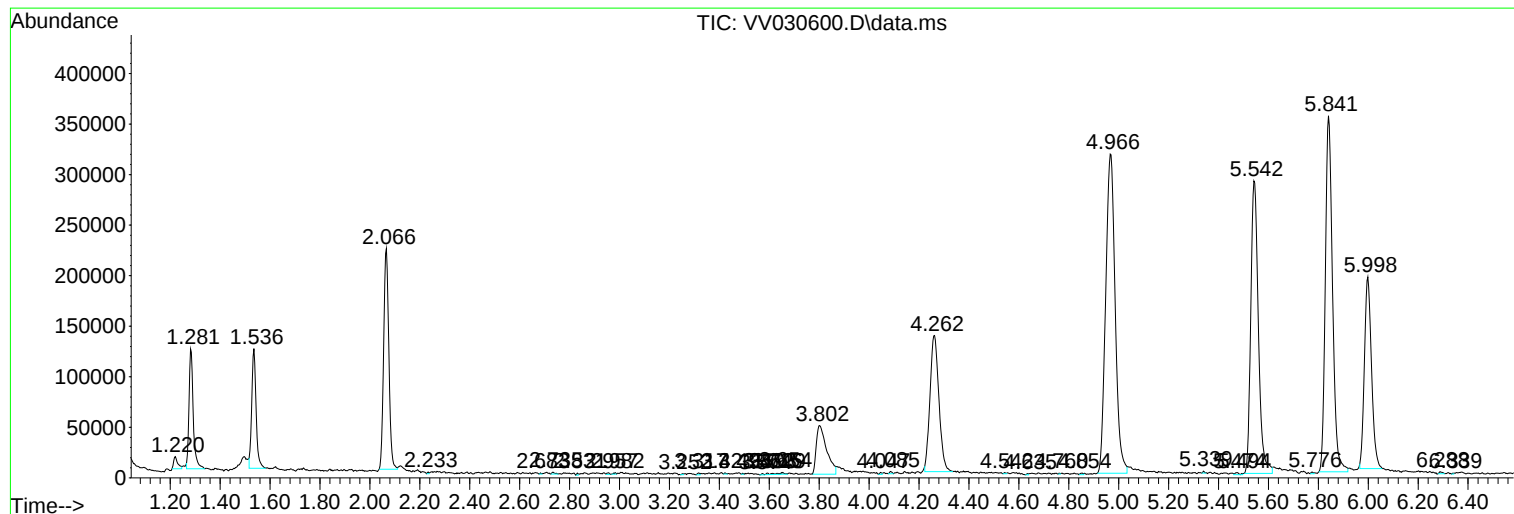

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030600.D
Acq On : 17 Apr 2023 19:48
Operator : SY/MD
Sample : 02360-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030600.D
Acq On : 17 Apr 2023 19:48
Operator : SY/MD
Sample : 02360-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc