

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030605.D
 Acq On : 17 Apr 2023 21:51
 Operator : SY/MD
 Sample : 02360-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	92	rVB	125474	136295	0.12%	0.110%
2	1.532	147	153	166	rVB	104155	128028	0.11%	0.103%
3	2.066	309	319	335	rBV2	254768	409002	0.35%	0.329%
4	2.500	452	454	458	rVB5	1738	864	0.00%	0.001%
5	2.520	458	460	462	rBV3	2229	1247	0.00%	0.001%
6	2.700	511	516	519	rBV7	2121	2276	0.00%	0.002%
7	2.770	536	538	539	rBV2	1042	432	0.00%	0.000%
8	2.867	565	568	571	rVB4	1588	976	0.00%	0.001%
9	2.886	571	574	576	rBV3	1640	1136	0.00%	0.001%
10	2.931	585	588	591	rBV4	1457	1094	0.00%	0.001%
11	2.999	607	609	612	rBV4	1243	663	0.00%	0.001%
12	3.044	621	623	625	rBV3	812	539	0.00%	0.000%
13	3.198	666	671	674	rBV6	1882	1932	0.00%	0.002%
14	3.272	690	694	697	rBV6	1048	914	0.00%	0.001%
15	3.294	699	701	702	rBV3	1170	554	0.00%	0.000%
16	3.349	716	718	720	rBV3	850	447	0.00%	0.000%
17	3.449	746	749	752	rBV5	1450	1012	0.00%	0.001%
18	3.503	765	766	767	rBV	720	258	0.00%	0.000%
19	3.519	769	771	773	rVB3	1294	432	0.00%	0.000%
20	3.536	775	776	778	rBV	1350	527	0.00%	0.000%
21	3.574	786	788	792	rBV4	1165	999	0.00%	0.001%
22	3.745	835	841	843	rBV6	1652	1549	0.00%	0.001%
23	3.822	849	865	886	rBV2	121833	386399	0.33%	0.311%
24	4.259	988	1001	1028	rVB	137173	356258	0.30%	0.287%
25	4.523	1068	1083	1100	rBV3	42704	113027	0.10%	0.091%
26	4.712	1139	1142	1145	rBV5	1677	1616	0.00%	0.001%
27	4.796	1165	1168	1170	rBV4	1653	1062	0.00%	0.001%
28	4.854	1184	1186	1189	rBV4	1326	626	0.00%	0.001%
29	4.873	1189	1192	1194	rBV4	1129	651	0.00%	0.001%
30	4.899	1198	1200	1203	rVB3	1895	969	0.00%	0.001%
31	4.966	1203	1221	1244	rBV2	321346	859618	0.73%	0.692%
32	5.362	1342	1344	1349	rBV6	1182	916	0.00%	0.001%
33	5.542	1388	1400	1421	rBV	280260	589496	0.50%	0.474%
34	5.854	1476	1497	1533	rBV	59836346	117826328	100.00%	94.793%
35	6.921	1819	1829	1844	rBV	95437	171088	0.15%	0.138%
36	7.111	1887	1888	1890	rBV2	1111	611	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030605.D
 Acq On : 17 Apr 2023 21:51
 Operator : SY/MD
 Sample : 02360-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1921	1932	1950	rBV	339722	601267	0.51%	0.484%
38	7.471	1996	2000	2002	rBV4	2115	1699	0.00%	0.001%
39	7.561	2019	2028	2041	rBV	69852	119077	0.10%	0.096%
40	7.712	2072	2075	2076	rBV3	1118	658	0.00%	0.001%
41	8.034	2166	2175	2188	rBV	164624	296185	0.25%	0.238%
42	8.355	2273	2275	2279	rBV4	1463	1140	0.00%	0.001%
43	8.584	2344	2346	2348	rVB3	1596	579	0.00%	0.000%
44	8.641	2360	2364	2366	rBV6	1571	1332	0.00%	0.001%
45	8.793	2400	2411	2428	rBV	419641	683771	0.58%	0.550%
46	9.288	2560	2565	2566	rBV4	1278	985	0.00%	0.001%
47	9.384	2593	2595	2596	rBV2	1317	513	0.00%	0.000%
48	9.455	2616	2617	2619	rBV2	1024	392	0.00%	0.000%
49	9.989	2781	2783	2788	rVB5	1302	899	0.00%	0.001%
50	10.162	2826	2837	2854	rBV	229883	364935	0.31%	0.294%
51	10.252	2863	2865	2867	rBV3	1638	940	0.00%	0.001%
52	10.317	2882	2885	2888	rBV4	1533	1159	0.00%	0.001%
53	10.403	2910	2912	2915	rBV4	1430	1031	0.00%	0.001%
54	10.529	2948	2951	2954	rBV3	1313	919	0.00%	0.001%
55	10.670	2992	2995	2996	rBV3	927	464	0.00%	0.000%
56	10.699	3002	3004	3008	rVB6	1664	757	0.00%	0.001%
57	10.725	3008	3012	3013	rBV3	1558	748	0.00%	0.001%
58	10.760	3022	3023	3027	rVB3	1206	527	0.00%	0.000%
59	10.799	3032	3035	3037	rVV3	1119	703	0.00%	0.001%
60	10.821	3040	3042	3044	rVB3	1250	451	0.00%	0.000%
61	10.953	3080	3083	3090	rVB7	2323	2185	0.00%	0.002%
62	10.985	3090	3093	3095	rBV3	1563	912	0.00%	0.001%
63	11.101	3120	3129	3140	rBV3	8769	17235	0.01%	0.014%
64	11.194	3147	3158	3175	rBV	386533	613339	0.52%	0.493%
65	11.407	3222	3224	3225	rBV2	1476	565	0.00%	0.000%
66	11.571	3263	3275	3290	rBV	335706	532134	0.45%	0.428%
67	11.709	3315	3318	3321	rBV5	1613	1403	0.00%	0.001%
68	11.825	3350	3354	3355	rBV4	930	710	0.00%	0.001%
69	11.905	3377	3379	3383	rBV5	2192	2054	0.00%	0.002%
70	11.966	3397	3398	3399	rBV	869	281	0.00%	0.000%
71	12.101	3439	3440	3441	rBV	1436	414	0.00%	0.000%
72	12.194	3465	3469	3470	rBV2	1105	790	0.00%	0.001%
73	12.297	3493	3501	3512	rBV10	14278	24071	0.02%	0.019%
74	12.397	3530	3532	3535	rVB4	1234	789	0.00%	0.001%
75	12.413	3535	3537	3540	rBV4	890	570	0.00%	0.000%
76	12.503	3563	3565	3566	rBV2	1171	478	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030605.D
 Acq On : 17 Apr 2023 21:51
 Operator : SY/MD
 Sample : 02360-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.587	3589	3591	3594	rBV4	1736	1117	0.00%	0.001%
78	12.654	3609	3612	3613	rBV2	1277	593	0.00%	0.000%
79	12.725	3632	3634	3636	rVB3	1347	579	0.00%	0.000%
80	12.902	3687	3689	3693	rVB4	1045	653	0.00%	0.001%
81	12.918	3693	3694	3696	rBV2	865	369	0.00%	0.000%
82	13.046	3732	3734	3738	rVB5	861	278	0.00%	0.000%
83	13.098	3747	3750	3752	rBV4	1560	1051	0.00%	0.001%
84	13.156	3766	3768	3769	rBV2	1041	482	0.00%	0.000%
85	13.210	3783	3785	3787	rBV3	1243	562	0.00%	0.000%
86	13.326	3819	3821	3823	rBV3	1705	1019	0.00%	0.001%
87	13.378	3834	3837	3840	rBV4	2332	1541	0.00%	0.001%
88	13.397	3840	3843	3845	rBV4	1516	1294	0.00%	0.001%
89	13.506	3875	3877	3879	rBV3	1399	714	0.00%	0.001%
90	13.567	3893	3896	3898	rBV4	1624	984	0.00%	0.001%
91	13.625	3912	3914	3917	rBV4	1506	803	0.00%	0.001%
92	13.734	3945	3948	3950	rVB4	773	427	0.00%	0.000%
93	13.751	3950	3953	3954	rBV3	991	407	0.00%	0.000%
94	13.767	3955	3958	3964	rBV7	1778	1241	0.00%	0.001%
95	13.796	3965	3967	3971	rVV4	1088	548	0.00%	0.000%
96	13.870	3987	3990	3992	rBV4	1391	870	0.00%	0.001%
97	13.943	4011	4013	4018	rVB5	1484	786	0.00%	0.001%
98	14.230	4098	4102	4106	rBV7	1423	1702	0.00%	0.001%
99	14.615	4220	4222	4226	rVB6	1961	1133	0.00%	0.001%
100	14.734	4257	4259	4260	rBV2	1403	561	0.00%	0.000%




Sum of corrected areas: 124298616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030605.D
Acq On : 17 Apr 2023 21:51
Operator : SY/MD
Sample : 02360-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

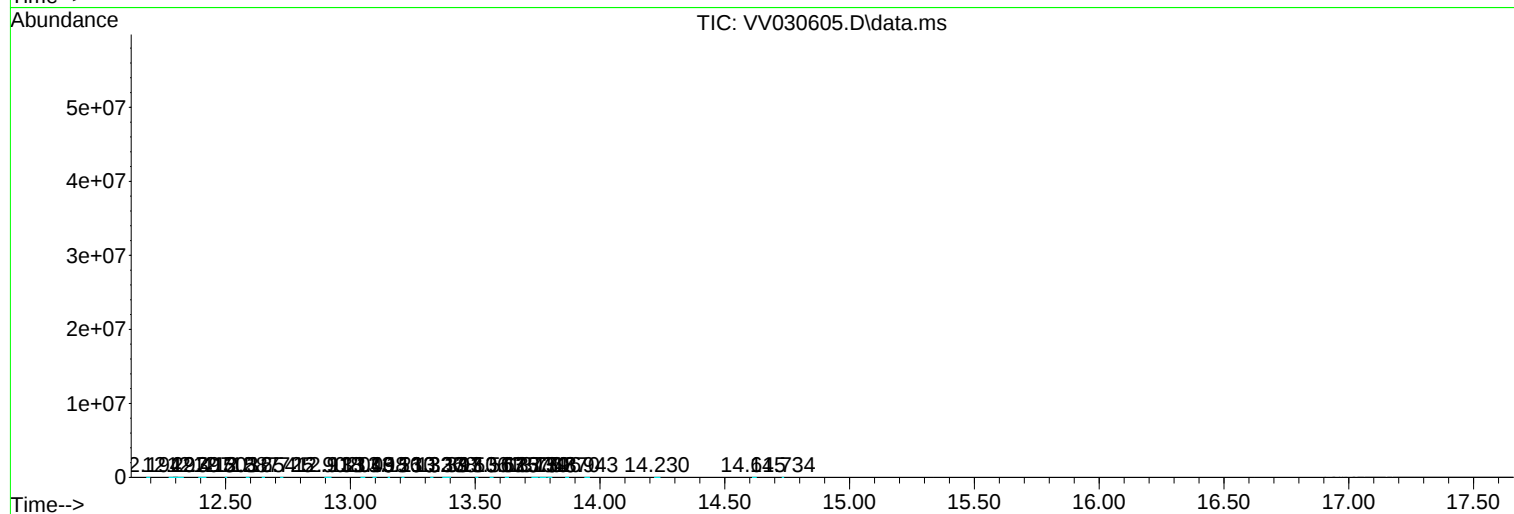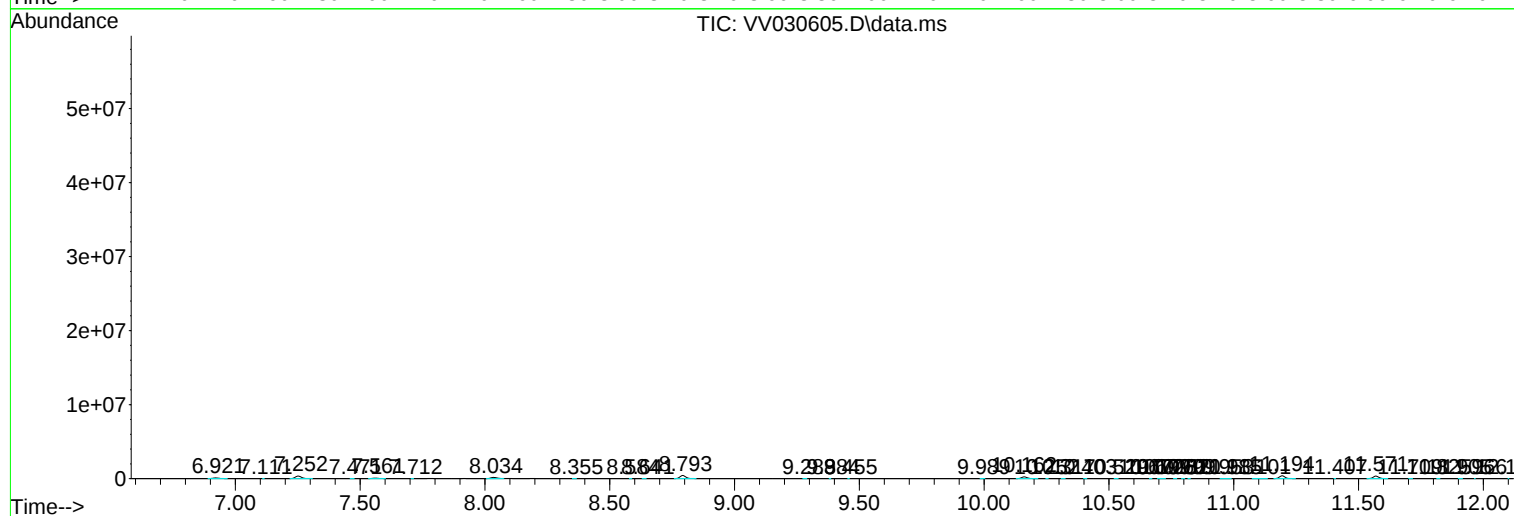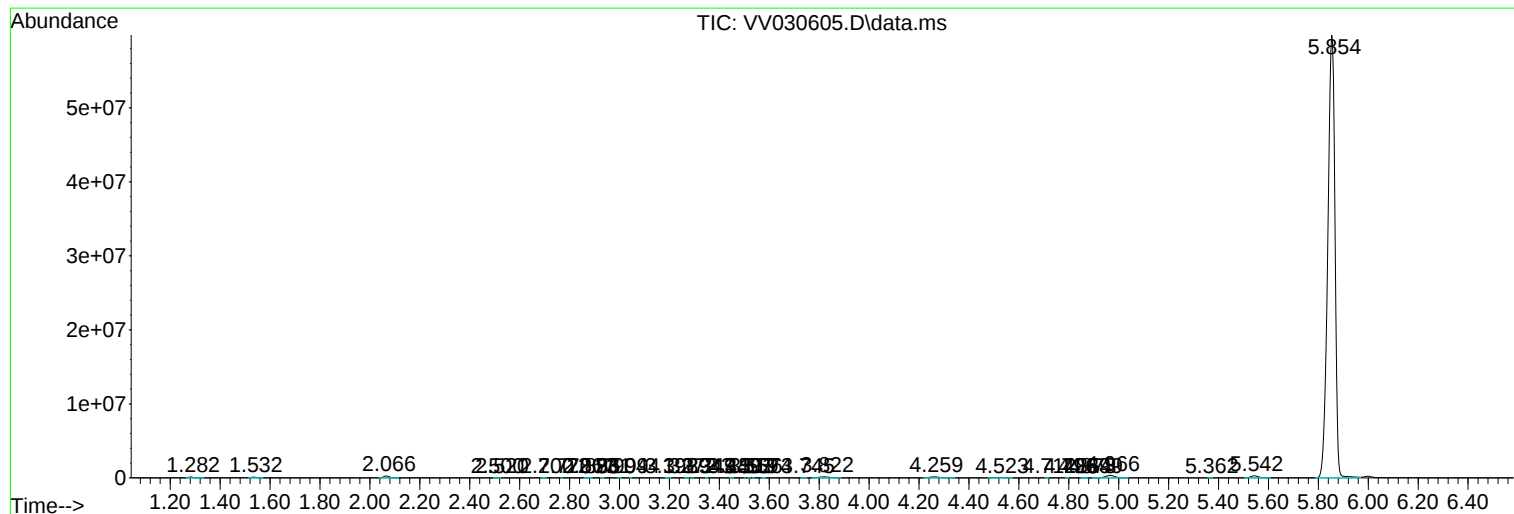

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030605.D
Acq On : 17 Apr 2023 21:51
Operator : SY/MD
Sample : 02360-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030605.D
Acq On : 17 Apr 2023 21:51
Operator : SY/MD
Sample : 02360-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------