

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030608.D
 Acq On : 18 Apr 2023 00:42
 Operator : SY/MD
 Sample : VV0417WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK322

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	65	rBV	14238	20700	2.44%	0.318%
2	1.281	69	75	96	rVB	123674	142423	16.76%	2.185%
3	1.532	148	153	166	rVB	112168	135266	15.92%	2.076%
4	2.063	309	318	334	rVB	225255	328899	38.71%	5.047%
5	2.317	395	397	399	rBV3	1198	760	0.09%	0.012%
6	2.690	510	513	514	rBV2	1750	1029	0.12%	0.016%
7	2.712	518	520	524	rVB5	1392	784	0.09%	0.012%
8	3.021	612	616	619	rBV5	1264	1120	0.13%	0.017%
9	3.069	629	631	636	rVB6	1142	828	0.10%	0.013%
10	3.095	636	639	642	rBV5	1753	1284	0.15%	0.020%
11	3.146	651	655	656	rBV3	1393	1222	0.14%	0.019%
12	3.185	664	667	669	rBV4	875	676	0.08%	0.010%
13	3.220	675	678	681	rBV5	1327	873	0.10%	0.013%
14	3.375	723	726	728	rVB3	1419	836	0.10%	0.013%
15	3.387	728	730	732	rBV3	1346	794	0.09%	0.012%
16	3.410	734	737	738	rBV2	1424	802	0.09%	0.012%
17	3.455	747	751	752	rBV4	1251	840	0.10%	0.013%
18	3.545	775	779	780	rBV4	2141	1128	0.13%	0.017%
19	3.593	790	794	799	rBV6	1330	1704	0.20%	0.026%
20	3.658	810	814	816	rBV5	1204	875	0.10%	0.013%
21	3.703	826	828	831	rVB3	1367	625	0.07%	0.010%
22	3.802	849	859	887	rBV	52504	156278	18.39%	2.398%
23	4.149	965	967	970	rBV4	1077	619	0.07%	0.009%
24	4.259	983	1001	1024	rBV2	139105	364924	42.95%	5.600%
25	4.494	1071	1074	1076	rBV4	1562	659	0.08%	0.010%
26	4.728	1145	1147	1149	rBV3	963	679	0.08%	0.010%
27	4.809	1169	1172	1174	rBV4	1527	695	0.08%	0.011%
28	4.886	1192	1196	1198	rBV4	1806	1342	0.16%	0.021%
29	4.966	1203	1221	1244	rBV2	318497	849654	100.00%	13.038%
30	5.394	1352	1354	1356	rBV3	1289	731	0.09%	0.011%
31	5.442	1366	1369	1371	rBV4	1110	771	0.09%	0.012%
32	5.542	1386	1400	1426	rBV	271282	570677	67.17%	8.757%
33	5.998	1529	1542	1559	rBV	190544	390831	46.00%	5.997%
34	6.426	1673	1675	1679	rBV5	925	751	0.09%	0.012%
35	6.571	1716	1720	1721	rBV4	1140	643	0.08%	0.010%
36	6.731	1765	1770	1772	rBV6	1722	1608	0.19%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030608.D
 Acq On : 18 Apr 2023 00:42
 Operator : SY/MD
 Sample : VV0417WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK322

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.747	1772	1775	1778	rVV4	1149	607	0.07%	0.009%
38	6.815	1791	1796	1798	rBV6	1739	1273	0.15%	0.020%
39	6.841	1801	1804	1806	rBV4	1249	842	0.10%	0.013%
40	6.921	1818	1829	1848	rBV2	92631	176263	20.75%	2.705%
41	7.059	1870	1872	1875	rBV4	1360	1028	0.12%	0.016%
42	7.252	1917	1932	1950	rBV	356396	637511	75.03%	9.783%
43	7.561	2015	2028	2046	rBV	67322	124800	14.69%	1.915%
44	7.712	2072	2075	2076	rBV3	1691	831	0.10%	0.013%
45	7.995	2160	2163	2165	rBV4	1127	741	0.09%	0.011%
46	8.037	2165	2176	2205	rBV	168605	349085	41.09%	5.357%
47	8.558	2336	2338	2343	rVB5	1339	928	0.11%	0.014%
48	8.648	2360	2366	2367	rBV6	1714	1842	0.22%	0.028%
49	8.673	2371	2374	2376	rVV3	1965	1271	0.15%	0.020%
50	8.686	2376	2378	2385	rVB8	2016	1764	0.21%	0.027%
51	8.792	2399	2411	2437	rBV	401644	681931	80.26%	10.464%
52	9.165	2524	2527	2531	rVB5	1896	1211	0.14%	0.019%
53	9.204	2531	2539	2540	rBV7	1683	2061	0.24%	0.032%
54	9.323	2573	2576	2578	rBV4	1330	786	0.09%	0.012%
55	9.583	2653	2657	2658	rBV4	1380	898	0.11%	0.014%
56	9.837	2733	2736	2739	rVB4	1031	686	0.08%	0.011%
57	9.870	2742	2746	2749	rBV6	1487	1526	0.18%	0.023%
58	9.947	2767	2770	2773	rVB6	2078	1548	0.18%	0.024%
59	10.050	2793	2802	2803	rBV8	1384	2199	0.26%	0.034%
60	10.082	2808	2812	2820	rVB10	1828	1828	0.22%	0.028%
61	10.117	2820	2823	2824	rBV3	1176	641	0.08%	0.010%
62	10.162	2826	2837	2856	rVV	252384	403114	47.44%	6.186%
63	10.329	2886	2889	2893	rVB5	1966	1340	0.16%	0.021%
64	10.432	2917	2921	2922	rBV4	1089	627	0.07%	0.010%
65	10.442	2922	2924	2928	rBV4	1317	785	0.09%	0.012%
66	10.525	2945	2950	2956	rVB8	2104	2029	0.24%	0.031%
67	10.632	2979	2983	2984	rBV4	1284	915	0.11%	0.014%
68	10.648	2984	2988	2991	rVV6	1380	1175	0.14%	0.018%
69	10.702	3002	3005	3008	rBV5	1505	1089	0.13%	0.017%
70	10.734	3011	3015	3019	rVB6	1747	1443	0.17%	0.022%
71	10.760	3019	3023	3024	rBV3	1123	883	0.10%	0.014%
72	10.998	3095	3097	3101	rVB5	1181	838	0.10%	0.013%
73	11.037	3107	3109	3112	rBV4	1517	922	0.11%	0.014%
74	11.066	3117	3118	3122	rVB4	1418	640	0.08%	0.010%
75	11.088	3122	3125	3129	rBV6	1742	1254	0.15%	0.019%
76	11.194	3147	3158	3175	rBV	361797	564158	66.40%	8.657%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030608.D
 Acq On : 18 Apr 2023 00:42
 Operator : SY/MD
 Sample : VV0417WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK322

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.371	3210	3213	3215	rBV4	1018	785	0.09%	0.012%
78	11.461	3238	3241	3244	rBV5	1465	781	0.09%	0.012%
79	11.570	3261	3275	3289	rBV	325344	532279	62.65%	8.168%
80	11.988	3400	3405	3408	rBV6	1263	1412	0.17%	0.022%
81	12.181	3462	3465	3467	rBV4	1707	1340	0.16%	0.021%
82	12.239	3481	3483	3487	rVB5	1303	746	0.09%	0.011%
83	12.262	3487	3490	3493	rBV5	1234	991	0.12%	0.015%
84	12.426	3538	3541	3545	rBV6	1488	1588	0.19%	0.024%
85	12.496	3560	3563	3568	rVB7	2330	1785	0.21%	0.027%
86	12.529	3568	3573	3574	rBV5	1418	828	0.10%	0.013%
87	12.541	3574	3577	3579	rBV4	1499	931	0.11%	0.014%
88	12.644	3606	3609	3612	rBV4	1563	1283	0.15%	0.020%
89	12.779	3648	3651	3652	rBV3	1106	663	0.08%	0.010%
90	13.049	3734	3735	3742	rVB6	1817	1260	0.15%	0.019%
91	13.091	3745	3748	3750	rBV3	1101	635	0.07%	0.010%
92	13.123	3757	3758	3761	rVB2	1531	625	0.07%	0.010%
93	13.275	3799	3805	3806	rBV5	1971	1697	0.20%	0.026%
94	13.599	3904	3906	3908	rBV2	1192	651	0.08%	0.010%
95	13.676	3926	3930	3931	rBV4	1458	1223	0.14%	0.019%
96	13.963	4017	4019	4024	rVV6	1379	1201	0.14%	0.018%
97	14.008	4029	4033	4035	rBV5	1882	1628	0.19%	0.025%
98	14.284	4117	4119	4120	rBV2	1355	624	0.07%	0.010%
99	14.294	4120	4122	4127	rVB4	1653	1053	0.12%	0.016%
100	14.368	4142	4145	4147	rVV3	1969	1149	0.14%	0.018%




Sum of corrected areas: 6516801

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030608.D
Acq On : 18 Apr 2023 00:42
Operator : SY/MD
Sample : VV0417WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

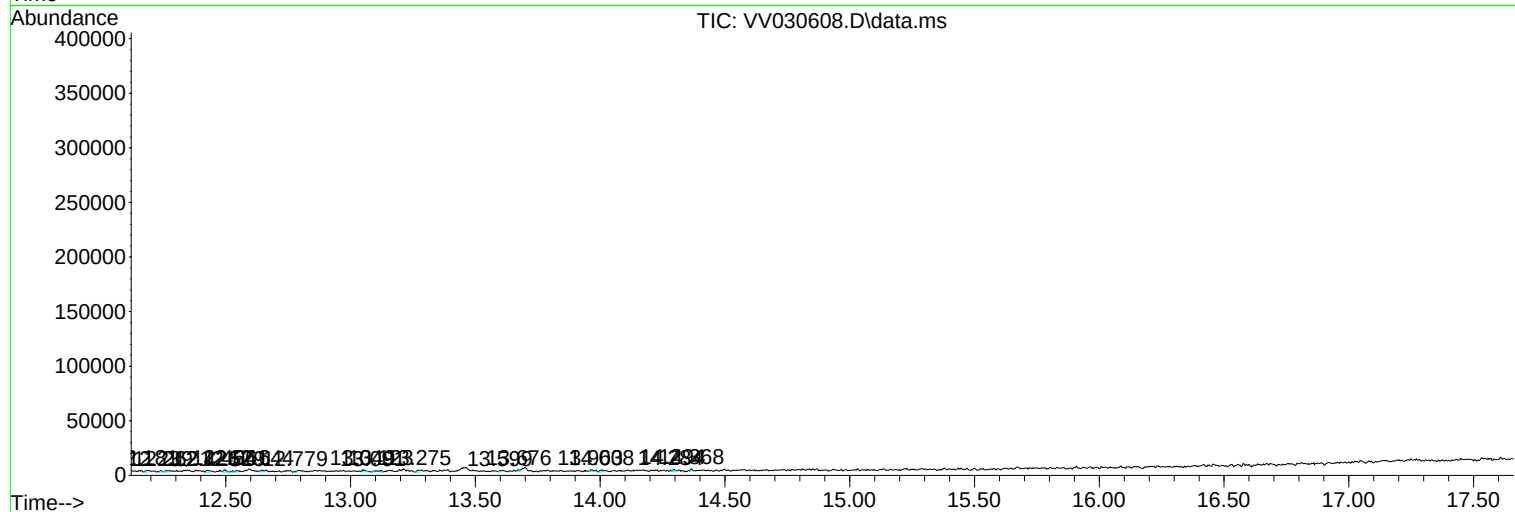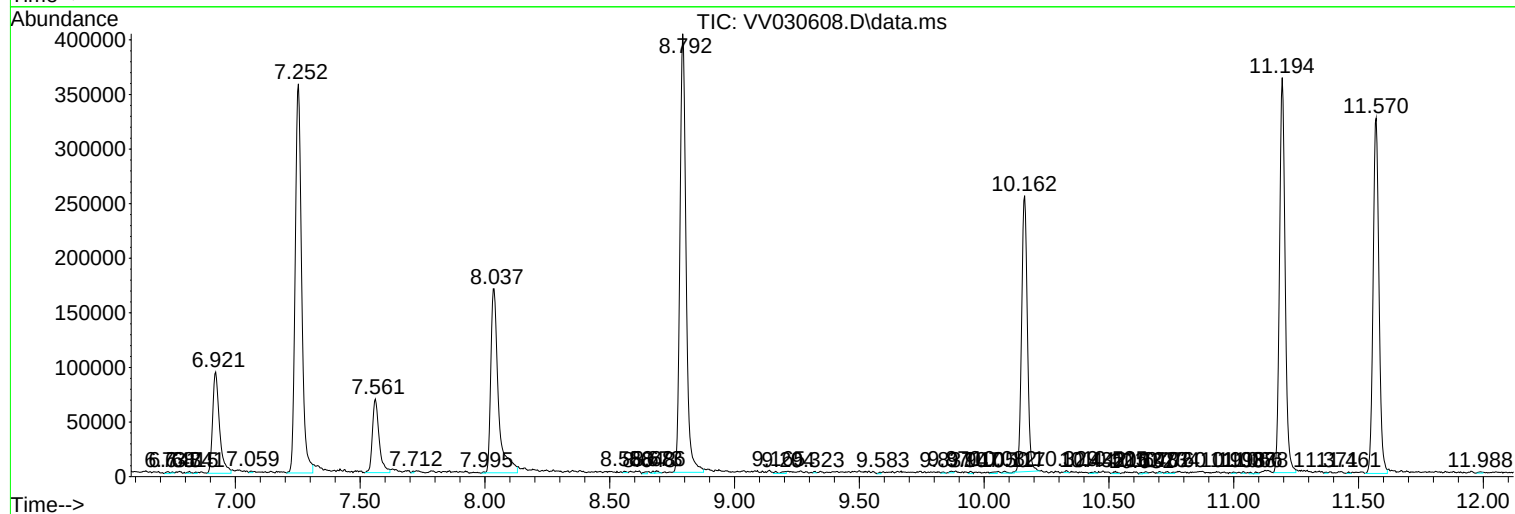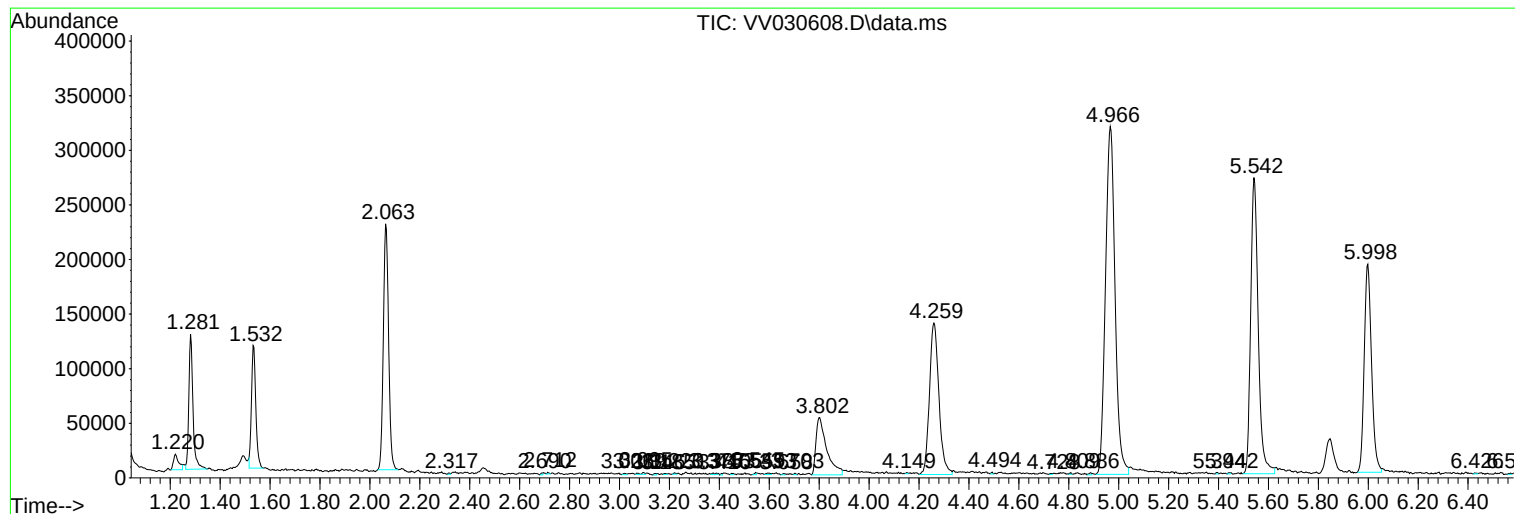

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030608.D
Acq On : 18 Apr 2023 00:42
Operator : SY/MD
Sample : VV0417WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030608.D
Acq On : 18 Apr 2023 00:42
Operator : SY/MD
Sample : VV0417WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------