

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030609.D
 Acq On : 18 Apr 2023 01:06
 Operator : SY/MD
 Sample : 02360-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	62	rBV	16599	19915	0.05%	0.044%
2	1.281	70	75	90	rVB	75934	87238	0.22%	0.195%
3	2.063	309	318	332	rBV2	157711	244039	0.61%	0.544%
4	2.558	468	472	473	rBV4	1469	1090	0.00%	0.002%
5	2.584	478	480	484	rVB4	1913	981	0.00%	0.002%
6	2.609	484	488	490	rVB5	1065	853	0.00%	0.002%
7	2.680	507	510	511	rBV3	1469	728	0.00%	0.002%
8	2.751	531	532	537	rVB6	1417	1043	0.00%	0.002%
9	2.780	537	541	544	rBV6	1635	1205	0.00%	0.003%
10	2.976	600	602	605	rBV4	1184	781	0.00%	0.002%
11	3.063	627	629	632	rBV4	1495	808	0.00%	0.002%
12	3.185	664	667	668	rBV3	1145	594	0.00%	0.001%
13	3.233	680	682	684	rBV3	1521	921	0.00%	0.002%
14	3.272	690	694	698	rVB7	1496	1104	0.00%	0.002%
15	3.432	742	744	746	rBV2	1220	573	0.00%	0.001%
16	3.548	778	780	784	rBV5	1291	752	0.00%	0.002%
17	3.645	807	810	811	rBV3	1379	728	0.00%	0.002%
18	3.725	832	835	837	rBV4	1284	584	0.00%	0.001%
19	3.822	849	865	892	rBV4	96584	312857	0.78%	0.698%
20	4.207	982	985	987	rBV4	1843	1247	0.00%	0.003%
21	4.259	987	1001	1022	rVV2	106224	272795	0.68%	0.608%
22	4.465	1059	1065	1066	rBV6	1714	1712	0.00%	0.004%
23	4.731	1144	1148	1151	rBV6	1494	1138	0.00%	0.003%
24	4.902	1195	1201	1202	rVV4	1222	1089	0.00%	0.002%
25	4.966	1205	1221	1246	rVV2	237257	637812	1.59%	1.422%
26	5.400	1354	1356	1358	rBV3	1074	620	0.00%	0.001%
27	5.542	1386	1400	1425	rBV	209133	450506	1.13%	1.005%
28	5.844	1476	1494	1532	rBV	21214872	40008339	100.00%	89.217%
29	6.526	1704	1706	1709	rVB4	1301	539	0.00%	0.001%
30	6.809	1791	1794	1798	rBV5	2350	1871	0.00%	0.004%
31	6.834	1799	1802	1803	rBV2	1076	586	0.00%	0.001%
32	6.921	1819	1829	1848	rBV	72992	135022	0.34%	0.301%
33	7.111	1885	1888	1889	rBV3	1261	808	0.00%	0.002%
34	7.188	1910	1912	1917	rVB5	1590	820	0.00%	0.002%
35	7.252	1920	1932	1957	rBV	256103	465787	1.16%	1.039%
36	7.561	2016	2028	2044	rBV	53562	98558	0.25%	0.220%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030609.D
 Acq On : 18 Apr 2023 01:06
 Operator : SY/MD
 Sample : 02360-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.037	2164	2176	2191	rBV	154656	289896	0.72%	0.646%
38	8.397	2287	2288	2290	rBV2	1325	520	0.00%	0.001%
39	8.500	2317	2320	2323	rBV5	1825	1263	0.00%	0.003%
40	8.564	2337	2340	2343	rVB4	1405	728	0.00%	0.002%
41	8.609	2352	2354	2358	rBV5	1694	1277	0.00%	0.003%
42	8.635	2360	2362	2365	rBV4	718	495	0.00%	0.001%
43	8.734	2391	2393	2396	rVB4	1158	542	0.00%	0.001%
44	8.792	2400	2411	2434	rVV	328600	546077	1.36%	1.218%
45	9.136	2517	2518	2521	rBV4	1286	587	0.00%	0.001%
46	9.342	2580	2582	2585	rBV4	1472	779	0.00%	0.002%
47	9.442	2611	2613	2618	rVB6	1955	1404	0.00%	0.003%
48	9.474	2620	2623	2625	rBV3	1462	795	0.00%	0.002%
49	9.612	2663	2666	2670	rBV5	759	805	0.00%	0.002%
50	9.632	2670	2672	2674	rVV3	1236	708	0.00%	0.002%
51	9.654	2677	2679	2683	rVB6	920	538	0.00%	0.001%
52	9.706	2693	2695	2697	rVB2	2091	938	0.00%	0.002%
53	9.763	2702	2713	2723	rVV2	5558	11485	0.03%	0.026%
54	9.812	2726	2728	2735	rVV7	1371	1631	0.00%	0.004%
55	10.021	2791	2793	2795	rBV2	1641	923	0.00%	0.002%
56	10.117	2820	2823	2825	rBV5	994	672	0.00%	0.001%
57	10.162	2825	2837	2851	rBV	206421	327649	0.82%	0.731%
58	10.336	2885	2891	2893	rBV7	2351	2169	0.01%	0.005%
59	10.432	2919	2921	2924	rBV4	1309	822	0.00%	0.002%
60	10.522	2947	2949	2952	rVB3	1003	549	0.00%	0.001%
61	10.554	2957	2959	2962	rVB4	1664	721	0.00%	0.002%
62	10.590	2968	2970	2973	rBV3	1320	701	0.00%	0.002%
63	10.612	2974	2977	2979	rVB4	1349	772	0.00%	0.002%
64	10.712	3007	3008	3010	rVB2	1541	534	0.00%	0.001%
65	10.738	3010	3016	3019	rBV7	2266	2380	0.01%	0.005%
66	10.853	3047	3052	3058	rBV9	2404	3100	0.01%	0.007%
67	10.892	3058	3064	3065	rBV6	1735	1783	0.00%	0.004%
68	10.963	3083	3086	3087	rBV2	924	485	0.00%	0.001%
69	11.056	3113	3115	3116	rBV2	1073	495	0.00%	0.001%
70	11.101	3123	3129	3135	rBV7	9679	13000	0.03%	0.029%
71	11.194	3148	3158	3177	rVB	280484	445186	1.11%	0.993%
72	11.358	3207	3209	3215	rVB6	1341	1064	0.00%	0.002%
73	11.426	3225	3230	3232	rVB6	1054	981	0.00%	0.002%
74	11.464	3238	3242	3243	rBV4	987	589	0.00%	0.001%
75	11.570	3262	3275	3290	rBV	243032	393480	0.98%	0.877%
76	11.648	3297	3299	3303	rVB4	1335	998	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
 Data File : VV030609.D
 Acq On : 18 Apr 2023 01:06
 Operator : SY/MD
 Sample : 02360-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.754	3328	3332	3335	rBV5	1134	936	0.00%	0.002%
78	12.066	3425	3429	3431	rBV5	1322	908	0.00%	0.002%
79	12.136	3449	3451	3453	rBV2	1194	677	0.00%	0.002%
80	12.230	3478	3480	3482	rBV3	1177	532	0.00%	0.001%
81	12.271	3487	3493	3495	rBV7	1606	1664	0.00%	0.004%
82	12.303	3495	3503	3507	rBV7	4411	7261	0.02%	0.016%
83	12.419	3535	3539	3540	rBV4	1292	730	0.00%	0.002%
84	12.554	3579	3581	3583	rBV3	882	538	0.00%	0.001%
85	12.628	3601	3604	3606	rBV3	1578	922	0.00%	0.002%
86	12.648	3606	3610	3612	rVV5	1027	813	0.00%	0.002%
87	12.715	3628	3631	3632	rBV3	1191	595	0.00%	0.001%
88	12.763	3644	3646	3649	rVB4	1182	645	0.00%	0.001%
89	12.821	3661	3664	3668	rBV6	1300	1243	0.00%	0.003%
90	13.088	3746	3747	3750	rBV3	1279	682	0.00%	0.002%
91	13.165	3768	3771	3773	rBV4	1097	763	0.00%	0.002%
92	13.606	3906	3908	3912	rBV4	1415	1152	0.00%	0.003%
93	13.676	3928	3930	3932	rBV3	1284	602	0.00%	0.001%
94	13.738	3947	3949	3951	rBV2	1217	592	0.00%	0.001%
95	14.220	4096	4099	4102	rBV5	1666	1563	0.00%	0.003%
96	14.522	4191	4193	4197	rBV4	2296	1766	0.00%	0.004%
97	14.709	4249	4251	4256	rBV6	1043	827	0.00%	0.002%
98	14.844	4290	4293	4294	rBV3	1824	881	0.00%	0.002%
99	15.014	4344	4346	4347	rBV2	1391	577	0.00%	0.001%
100	15.368	4453	4456	4458	rBV4	2245	1544	0.00%	0.003%


Sum of corrected areas: 44843977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030609.D
Acq On : 18 Apr 2023 01:06
Operator : SY/MD
Sample : 02360-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

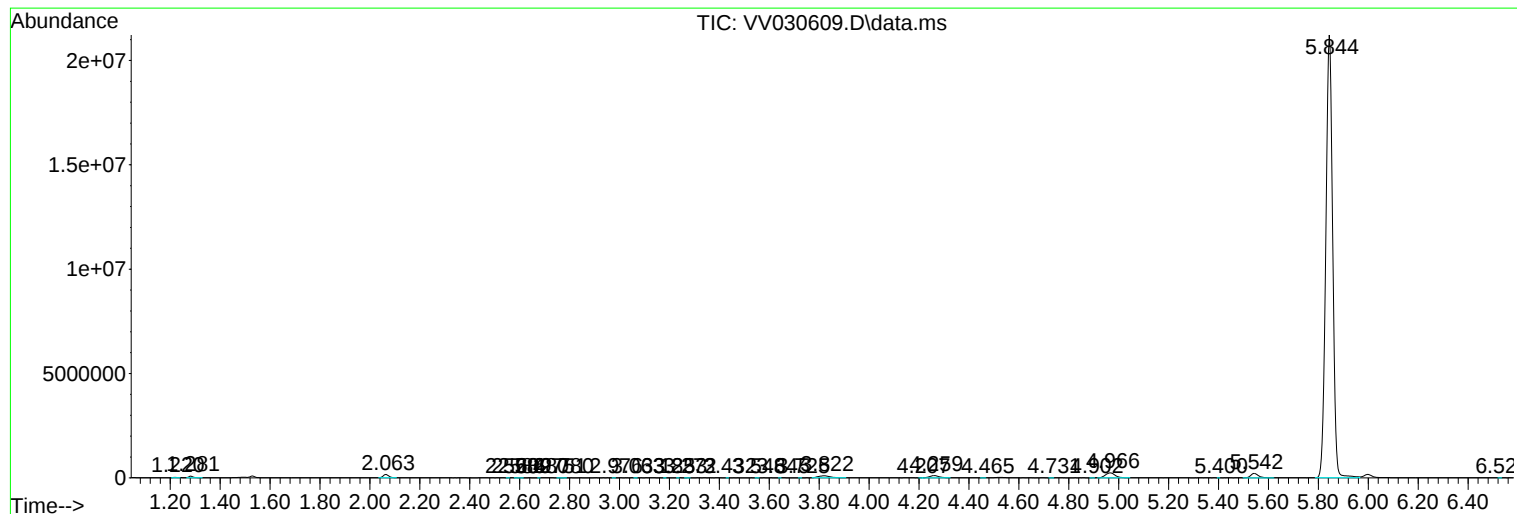

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030609.D
Acq On : 18 Apr 2023 01:06
Operator : SY/MD
Sample : 02360-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030609.D
Acq On : 18 Apr 2023 01:06
Operator : SY/MD
Sample : 02360-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc