

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041822\
 Data File : VW025605.D
 Acq On : 18 Apr 2022 13:43
 Operator : SY/MD
 Sample : N2388-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFE9

Quant Time: Apr 19 05:07:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 19 05:06:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	152772	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	153095	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73236	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	62888	4.428	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.600%
7) Chloroethane-d5	1.571	69	57754	3.822	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.400%
11) 1,1-Dichloroethene-d2	2.111	63	96060	3.376	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.600%
20) 2-Butanone-d5	3.902	46	74852	43.325	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.640%
24) Chloroform-d	4.352	84	92821	4.325	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
26) 1,2-Dichloroethane-d4	5.037	65	42758	4.624	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.400%
32) Benzene-d6	5.053	84	189778	4.284	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
36) 1,2-Dichloropropane-d6	6.072	67	55180	4.467	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.400%
41) Toluene-d8	7.316	98	165991	4.038	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.800%
43) trans-1,3-Dichloroprop...	7.625	79	16644	4.008	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.200%
46) 2-Hexanone-d5	8.088	63	53661	36.822	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.640%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31007	3.973	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	54454	4.435	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.600%
Target Compounds						
					Qvalue	
25) Chloroform	4.384	83	12671	0.638	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041822\
Data File : VV025605.D
Acq On : 18 Apr 2022 13:43
Operator : SY/MD
Sample : N2388-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFE9

Quant Time: Apr 19 05:07:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 19 05:06:28 2022
Response via : Initial Calibration

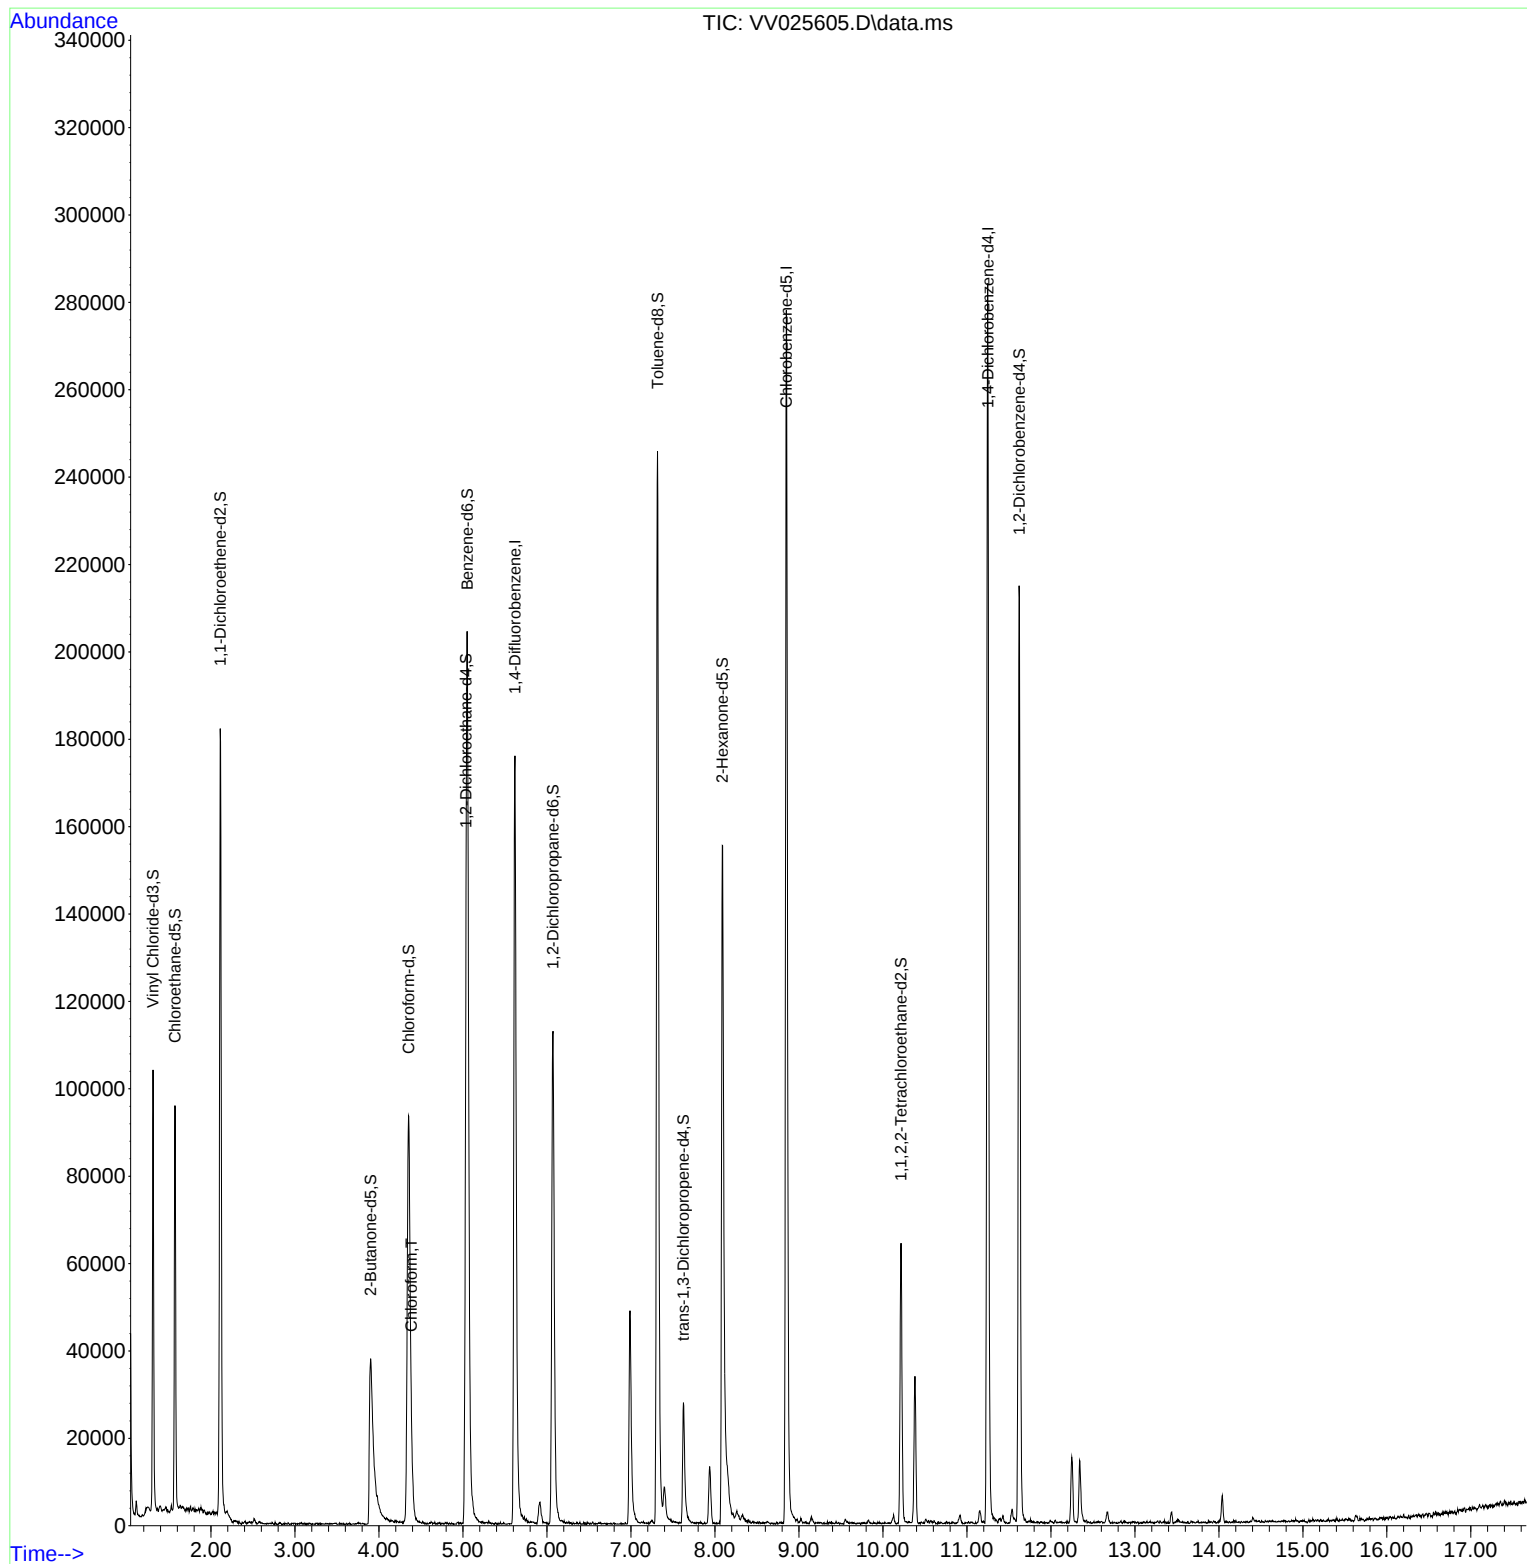

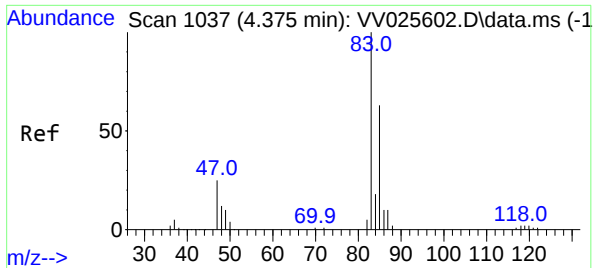

#25
Chloroform
Concen: 0.638 ug/L
RT: 4.384 min Scan# 10
Delta R.T. 0.009 min
Lab File: VV025605.D
Acq: 18 Apr 2022 13:43

Instrument :
MSVOA_V
ClientSampleId :
BFFE9

Tgt Ion: 83 Resp: 12671
Ion Ratio Lower Upper
83 100
85 64.5 43.5 80.7

