

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041822\
 Data File : VW025607.D
 Acq On : 18 Apr 2022 15:02
 Operator : SY/MD
 Sample : N2388-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFF6

Quant Time: Apr 19 05:08:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 19 05:06:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	175664	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	178013	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	83367	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	71238	4.362	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.200%
7) Chloroethane-d5	1.571	69	66060	3.802	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.000%
11) 1,1-Dichloroethene-d2	2.111	63	109654	3.352	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.000%
20) 2-Butanone-d5	3.899	46	88649	44.624	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.240%
24) Chloroform-d	4.352	84	109435	4.434	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%
26) 1,2-Dichloroethane-d4	5.037	65	50405	4.740	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
32) Benzene-d6	5.053	84	217732	4.227	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%
36) 1,2-Dichloropropane-d6	6.072	67	63820	4.443	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.800%
41) Toluene-d8	7.317	98	191589	4.008	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.200%
43) trans-1,3-Dichloroprop...	7.625	79	19455	4.030	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.600%
46) 2-Hexanone-d5	8.088	63	64567	38.104	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.200%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35749	3.939	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	62554	4.475	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.600%
Target Compounds						
25) Chloroform	4.384	83	12117	0.531	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041822\
Data File : VV025607.D
Acq On : 18 Apr 2022 15:02
Operator : SY/MD
Sample : N2388-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFF6

Quant Time: Apr 19 05:08:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 19 05:06:28 2022
Response via : Initial Calibration

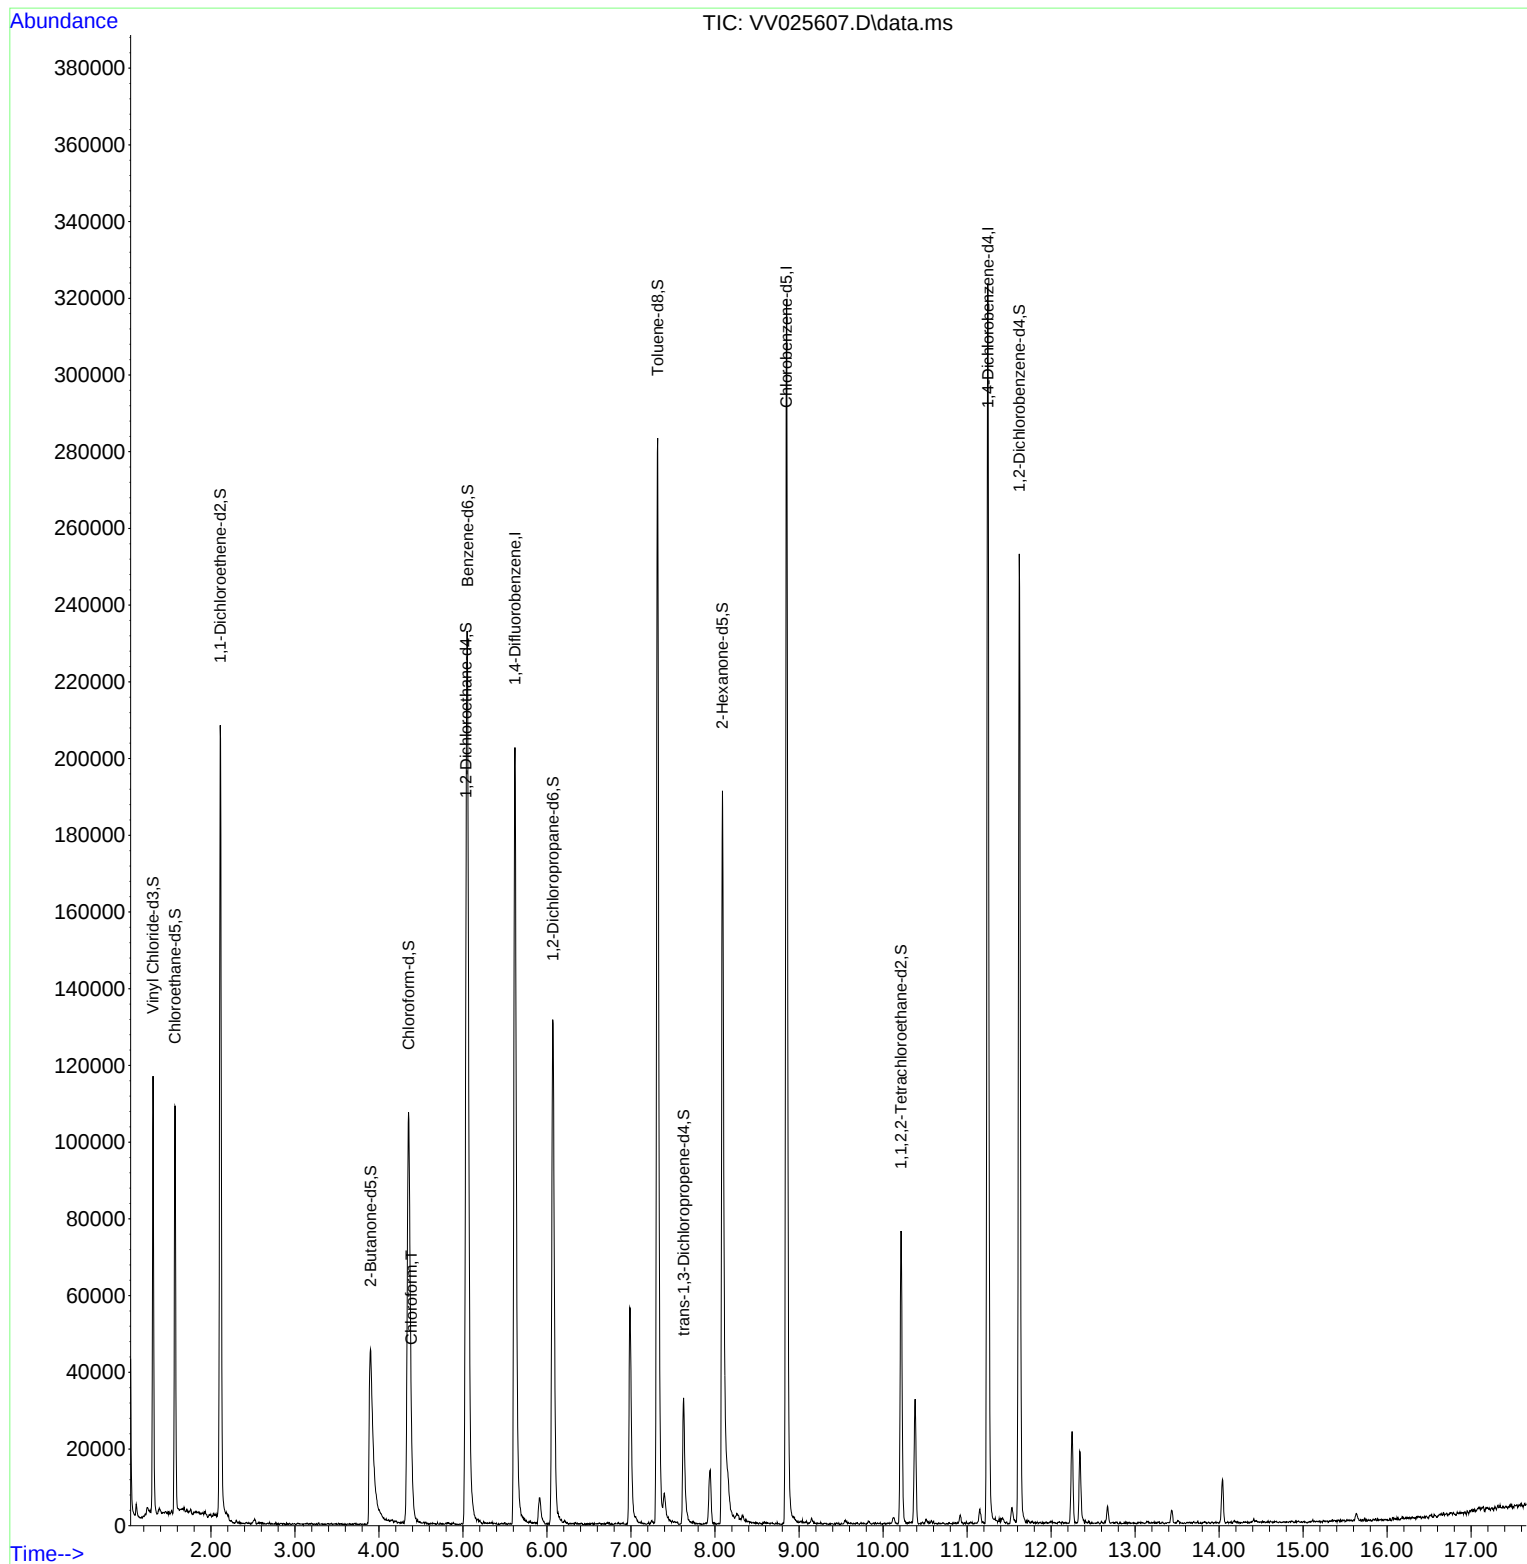

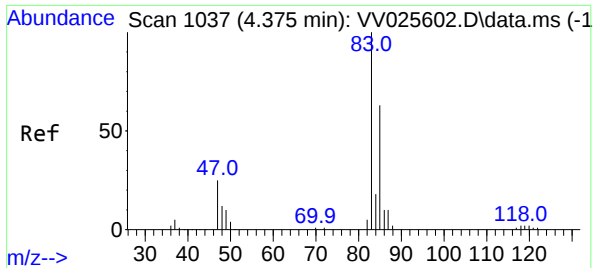

#25
Chloroform
Concen: 0.531 ug/L
RT: 4.384 min Scan# 10
Delta R.T. 0.009 min
Lab File: VV025607.D
Acq: 18 Apr 2022 15:02

Instrument :
MSVOA_V
ClientSampleId :
BFFF6

Tgt Ion: 83 Resp: 12117
Ion Ratio Lower Upper
83 100
85 57.3 43.5 80.7

