

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041822\
 Data File : VW025610.D
 Acq On : 18 Apr 2022 16:12
 Operator : SY/MD
 Sample : N2388-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFE1

Quant Time: Apr 19 05:08:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 19 05:06:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	144392	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	142390	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64568	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	60096	4.477	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.600%
7) Chloroethane-d5	1.571	69	56973	3.989	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.800%
11) 1,1-Dichloroethene-d2	2.111	63	91197	3.391	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.800%
20) 2-Butanone-d5	3.892	46	71645	43.875	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.760%
24) Chloroform-d	4.352	84	92936	4.581	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	5.034	65	43456	4.972	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	5.050	84	185165	4.494	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%
36) 1,2-Dichloropropane-d6	6.069	67	55741	4.851	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.317	98	157689	4.124	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%
43) trans-1,3-Dichloroprop...	7.625	79	15900	4.117	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.400%
46) 2-Hexanone-d5	8.088	63	55357	40.842	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.680%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	31710	4.368	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	52759	4.874	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.400%
Target Compounds					Qvalue	
13) Acetone	2.182	43	5071	4.575	ug/L	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041822\
Data File : VV025610.D
Acq On : 18 Apr 2022 16:12
Operator : SY/MD
Sample : N2388-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFE1

Quant Time: Apr 19 05:08:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 19 05:06:28 2022
Response via : Initial Calibration

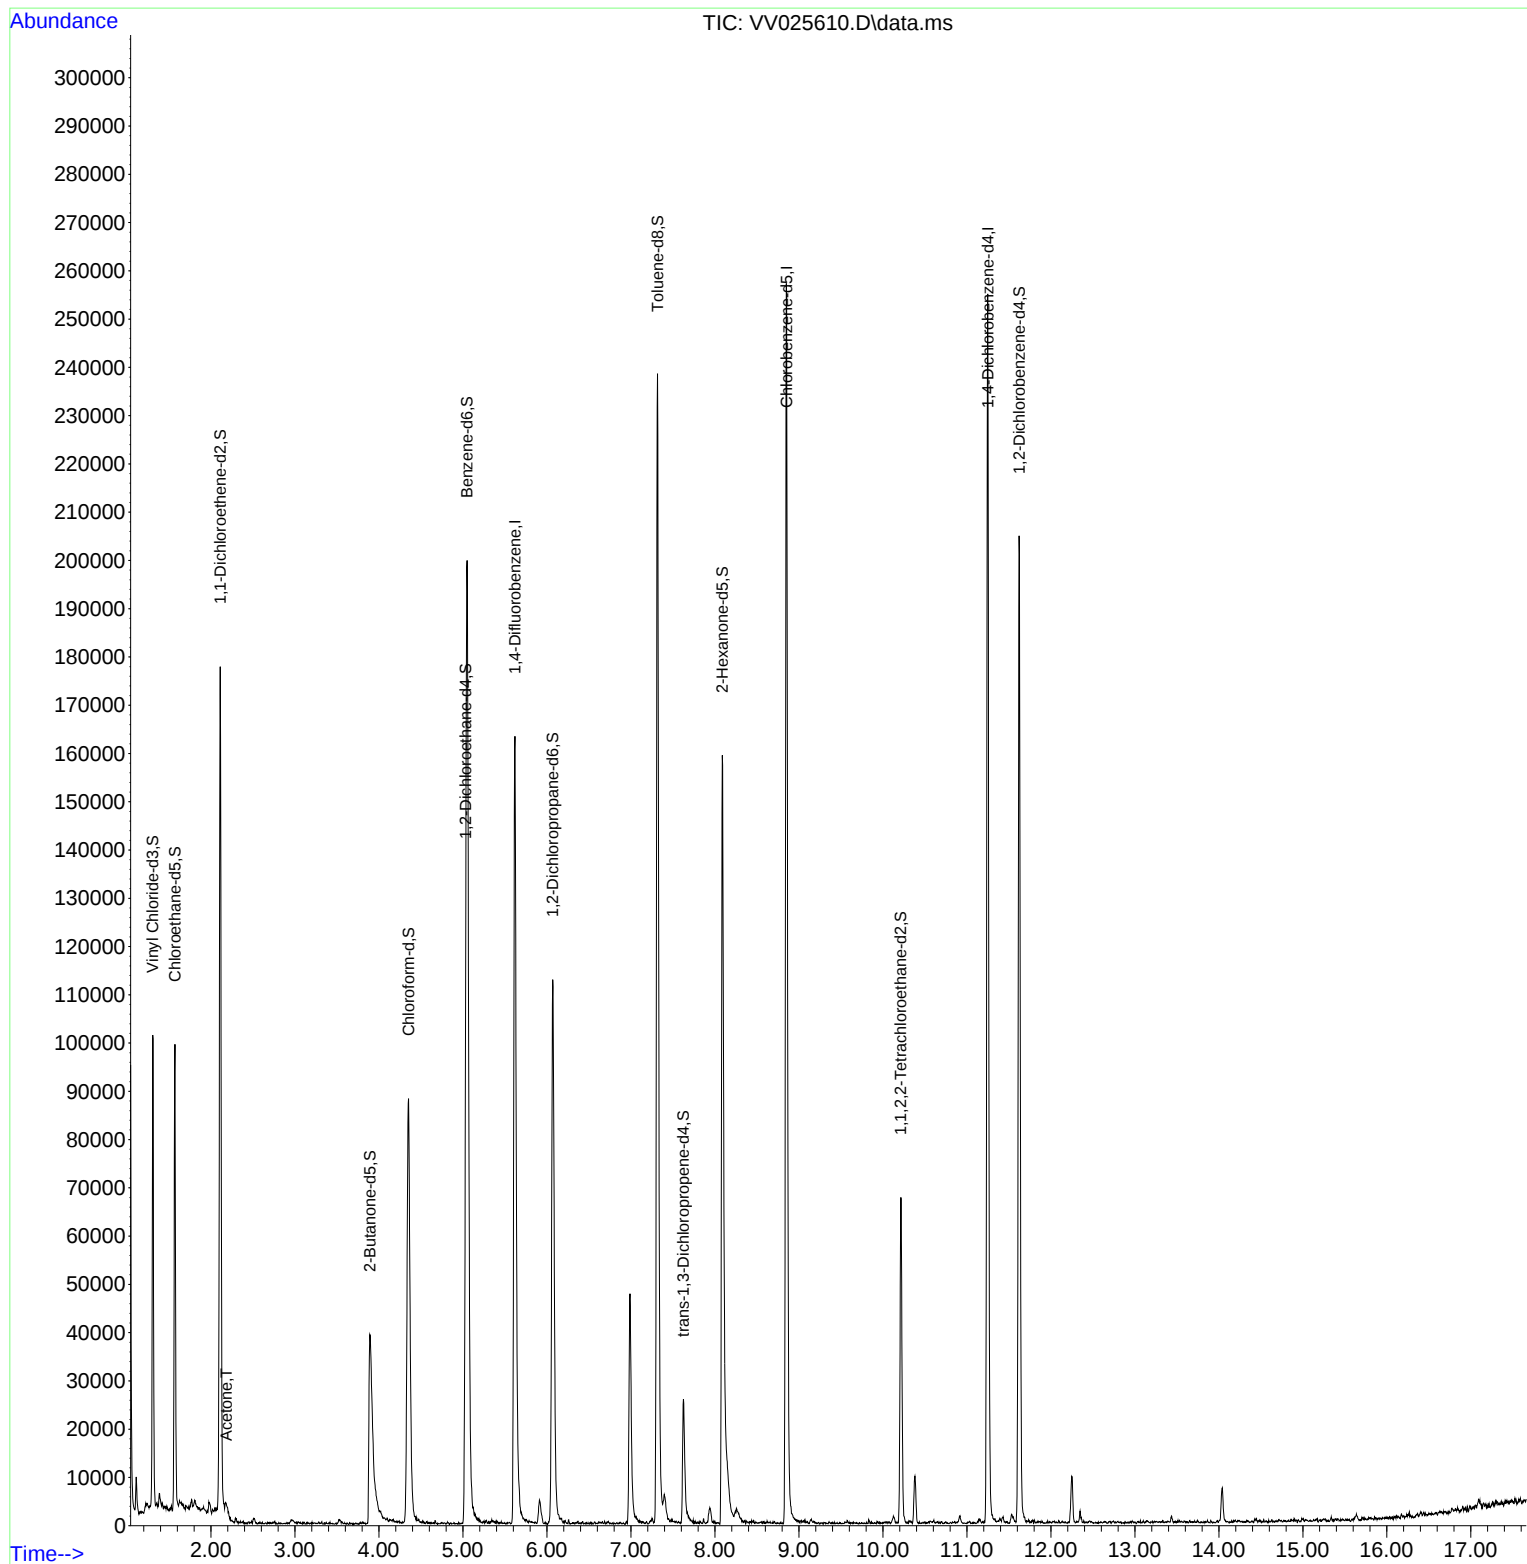

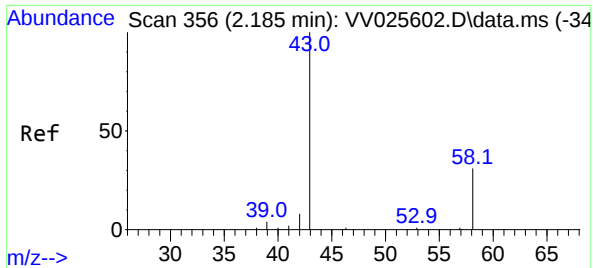

#13
 Acetone
 Concen: 4.575 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV025610.D
 Acq: 18 Apr 2022 16:12

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFE1

Tgt Ion: 43 Resp: 5071
 Ion Ratio Lower Upper
 43 100
 58 19.1 0.0 72.2

