

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041822\
 Data File : VW025614.D
 Acq On : 18 Apr 2022 17:46
 Operator : SY/MD
 Sample : N2384-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Q3

Quant Time: Apr 19 05:09:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 19 05:06:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	126990	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	129794	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59112	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	61027	5.169	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.400%
7) Chloroethane-d5	1.571	69	57291	4.561	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.200%
11) 1,1-Dichloroethene-d2	2.111	63	91708	3.878	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.600%
20) 2-Butanone-d5	3.895	46	74156	51.636	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.280%
24) Chloroform-d	4.352	84	91955	5.154	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
26) 1,2-Dichloroethane-d4	5.034	65	41710	5.426	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.600%
32) Benzene-d6	5.053	84	183720	4.892	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
36) 1,2-Dichloropropane-d6	6.069	67	53694	5.127	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.600%
41) Toluene-d8	7.316	98	155440	4.460	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.200%
43) trans-1,3-Dichloroprop...	7.625	79	15102	4.290	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.800%
46) 2-Hexanone-d5	8.088	63	54778	44.337	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.680%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32084	4.849	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	50076	5.053	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.000%
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	63645	7.986	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041822\
Data File : VV025614.D
Acq On : 18 Apr 2022 17:46
Operator : SY/MD
Sample : N2384-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q3


Quant Time: Apr 19 05:09:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 19 05:06:28 2022
Response via : Initial Calibration

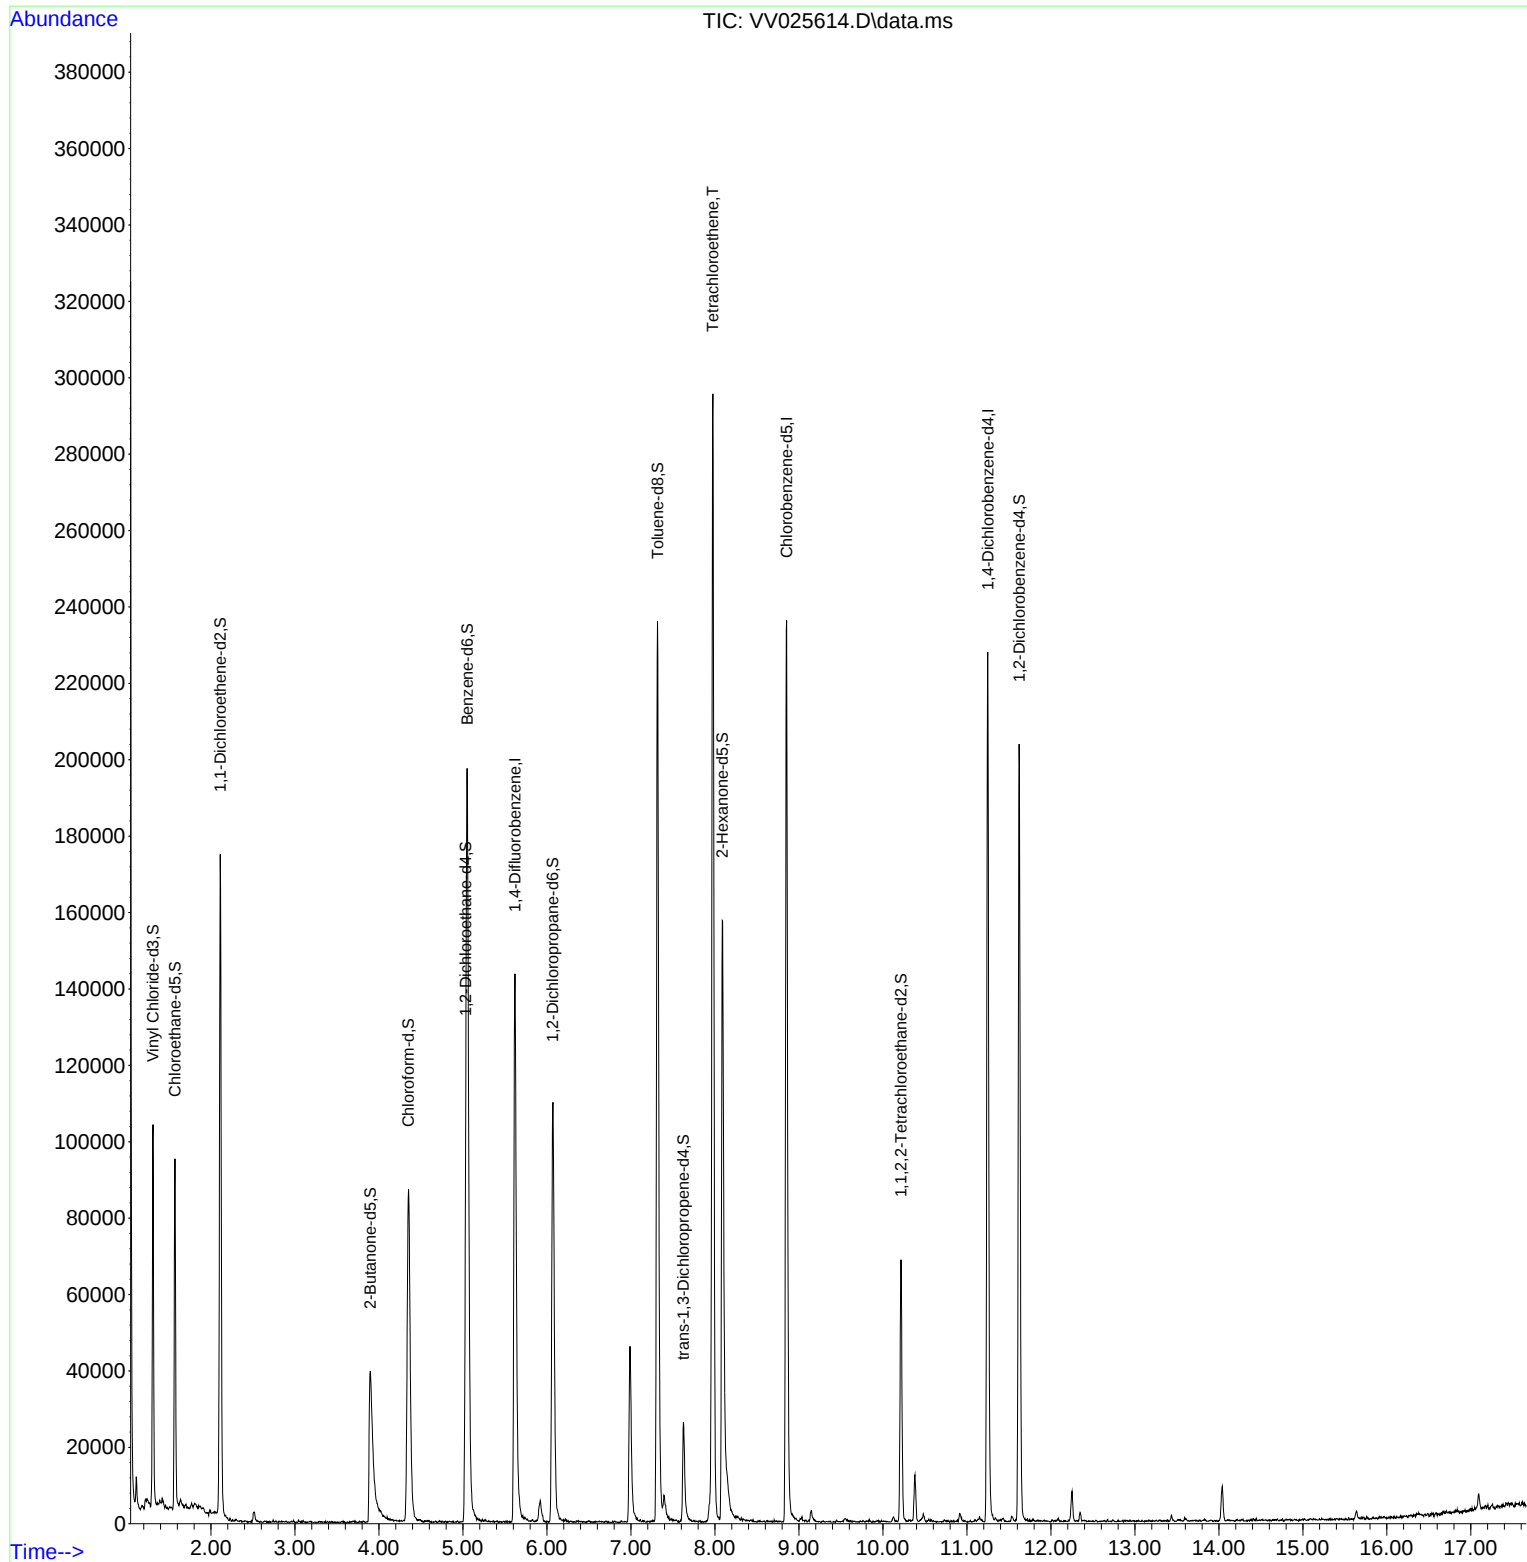

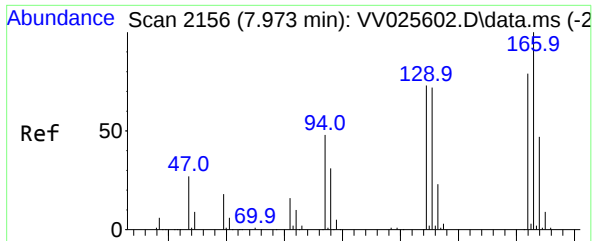

#47
Tetrachloroethene
Concen: 7.986 ug/L
RT: 7.976 min Scan# 2156
Delta R.T. 0.003 min
Lab File: VV025614.D
Acq: 18 Apr 2022 17:46

Instrument :
MSVOA_V
ClientSampleId :
EW6Q3

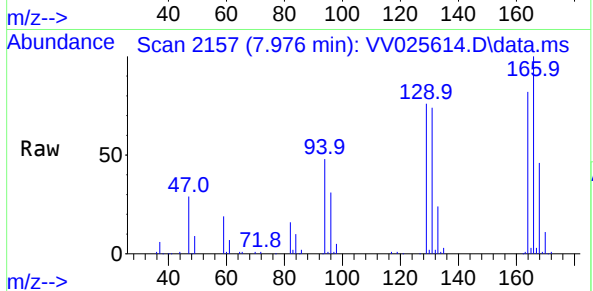

Tgt Ion:	164	Resp:	63645
Ion	Ratio	Lower	Upper
164	100		
129	93.6	66.8	124.2
131	90.5	66.4	123.4
166	122.4	91.7	170.3

