

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041822\
 Data File : VW025615.D
 Acq On : 18 Apr 2022 18:09
 Operator : SY/MD
 Sample : N2384-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Q5

Quant Time: Apr 19 05:09:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 19 05:06:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	131736	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	137162	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60021	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	59228	4.836	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.800%
7) Chloroethane-d5	1.571	69	55980	4.296	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.000%
11) 1,1-Dichloroethene-d2	2.111	63	92704	3.778	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.600%
20) 2-Butanone-d5	3.896	46	72550	48.698	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.400%
24) Chloroform-d	4.352	84	90268	4.877	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
26) 1,2-Dichloroethane-d4	5.034	65	42588	5.341	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.800%
32) Benzene-d6	5.053	84	183477	4.623	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
36) 1,2-Dichloropropane-d6	6.072	67	54304	4.906	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.200%
41) Toluene-d8	7.317	98	153843	4.177	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%
43) trans-1,3-Dichloroprop...	7.625	79	16181	4.350	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.000%
46) 2-Hexanone-d5	8.088	63	55259	42.323	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.640%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32410	4.635	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	49293	4.898	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.000%
Target Compounds						Qvalue
34) Trichloroethene	5.921	95	7473	0.695	ug/L	98
47) Tetrachloroethene	7.976	164	3976	0.472	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041822\
Data File : VV025615.D
Acq On : 18 Apr 2022 18:09
Operator : SY/MD
Sample : N2384-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q5

Quant Time: Apr 19 05:09:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 19 05:06:28 2022
Response via : Initial Calibration

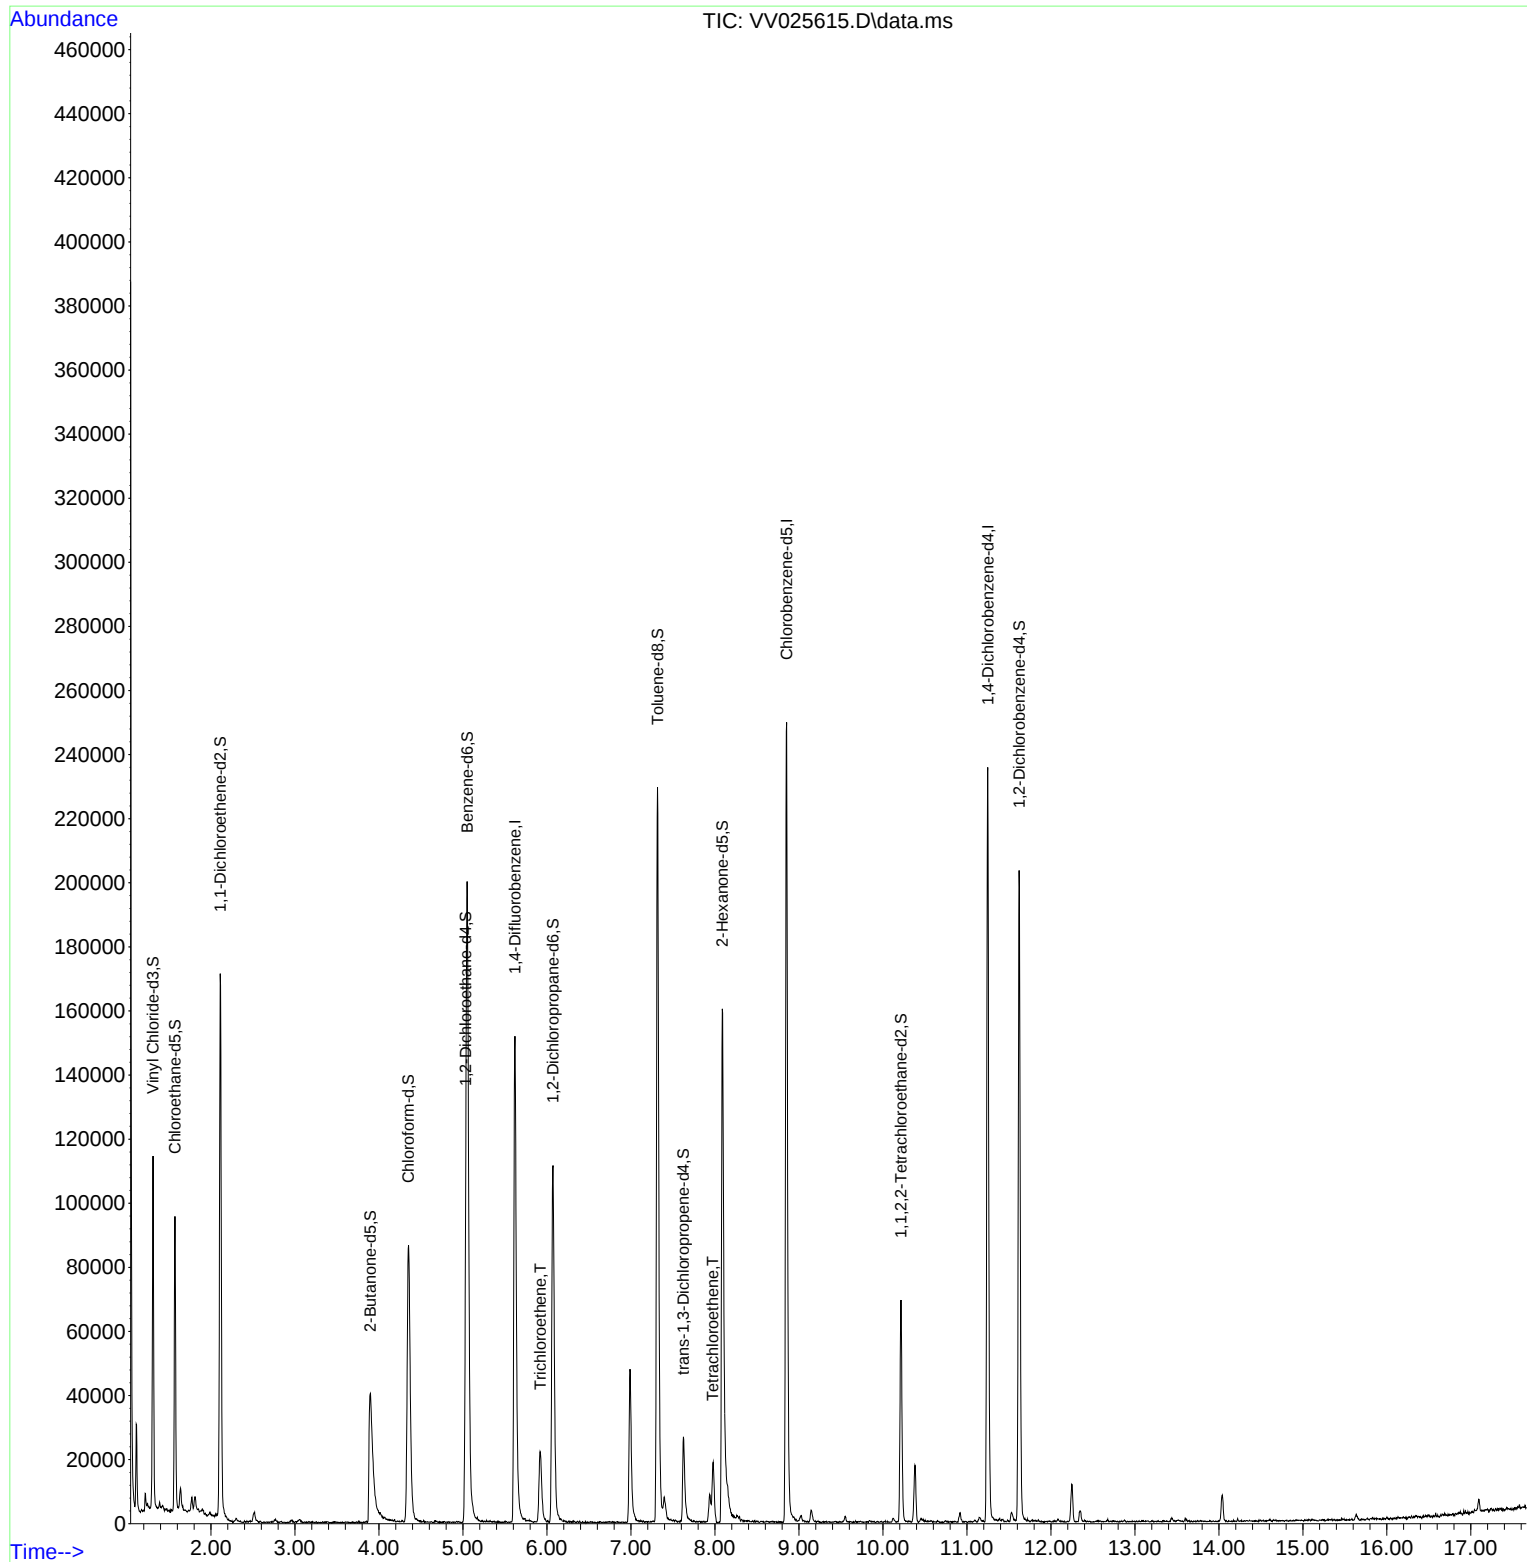




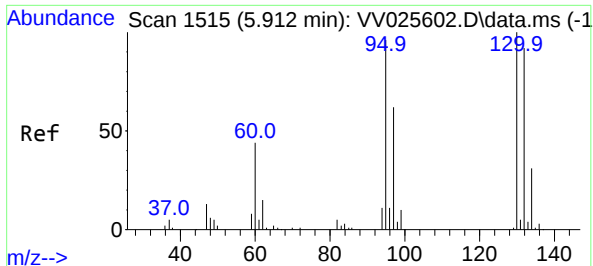


#34
Trichloroethene
Concen: 0.695 ug/L
RT: 5.921 min Scan# 11
Delta R.T. 0.010 min
Lab File: VV025615.D
Acq: 18 Apr 2022 18:09

Instrument :
MSVOA_V
ClientSampleId :
EW6Q5

Tgt Ion: 95 Resp: 7473

Ion	Ratio	Lower	Upper
95	100		
97	68.2	45.8	85.2
132	95.9	68.0	126.4
130	100.4	71.9	133.5

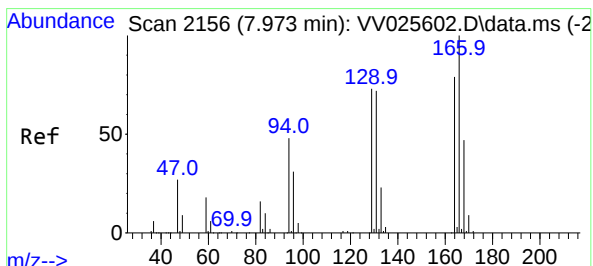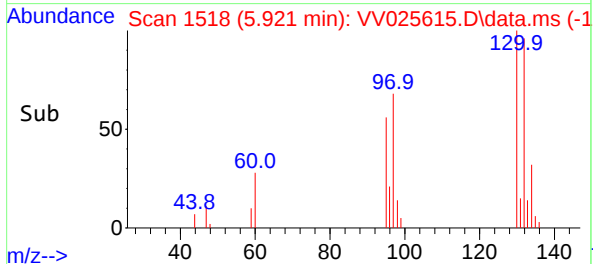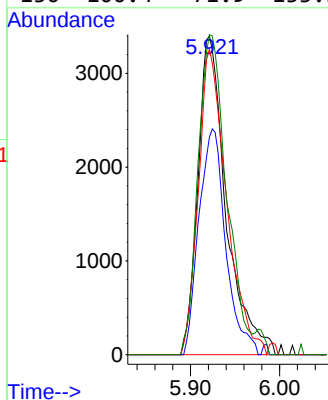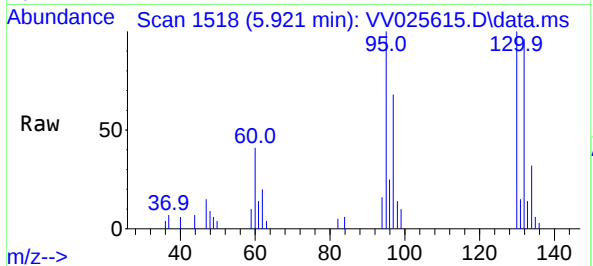

#47
Tetrachloroethene
Concen: 0.472 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. 0.003 min
Lab File: VV025615.D
Acq: 18 Apr 2022 18:09

Tgt Ion: 164 Resp: 3976

Ion	Ratio	Lower	Upper
164	100		
129	95.4	66.8	124.2
131	88.5	66.4	123.4
166	132.4	91.7	170.3

