

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041822\
 Data File : VW025618.D
 Acq On : 18 Apr 2022 19:20
 Operator : SY/MD
 Sample : N2384-20DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6S0DL

Quant Time: Apr 19 05:10:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 19 05:06:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117193	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	115678	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52877	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.311	65	55370	5.082	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.600%
7) Chloroethane-d5	1.571	69	56429	4.868	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.400%
11) 1,1-Dichloroethene-d2	2.111	63	84110	3.854	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.000%
20) 2-Butanone-d5	3.896	46	71939	54.280	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.560%
24) Chloroform-d	4.352	84	84879	5.155	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%
26) 1,2-Dichloroethane-d4	5.037	65	39896	5.624	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.400%
32) Benzene-d6	5.053	84	166093	4.962	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	6.072	67	51295	5.495	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.000%
41) Toluene-d8	7.317	98	140592	4.526	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.600%
43) trans-1,3-Dichloroprop...	7.625	79	14213	4.530	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.600%
46) 2-Hexanone-d5	8.088	63	51326	46.612	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.220%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	28863	4.894	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	45606	5.144	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.800%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.513	84	3599	0.365	ug/L	95
47) Tetrachloroethene	7.976	164	30944	4.356	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041822\
Data File : VV025618.D
Acq On : 18 Apr 2022 19:20
Operator : SY/MD
Sample : N2384-20DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6S0DL

Quant Time: Apr 19 05:10:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 19 05:06:28 2022
Response via : Initial Calibration




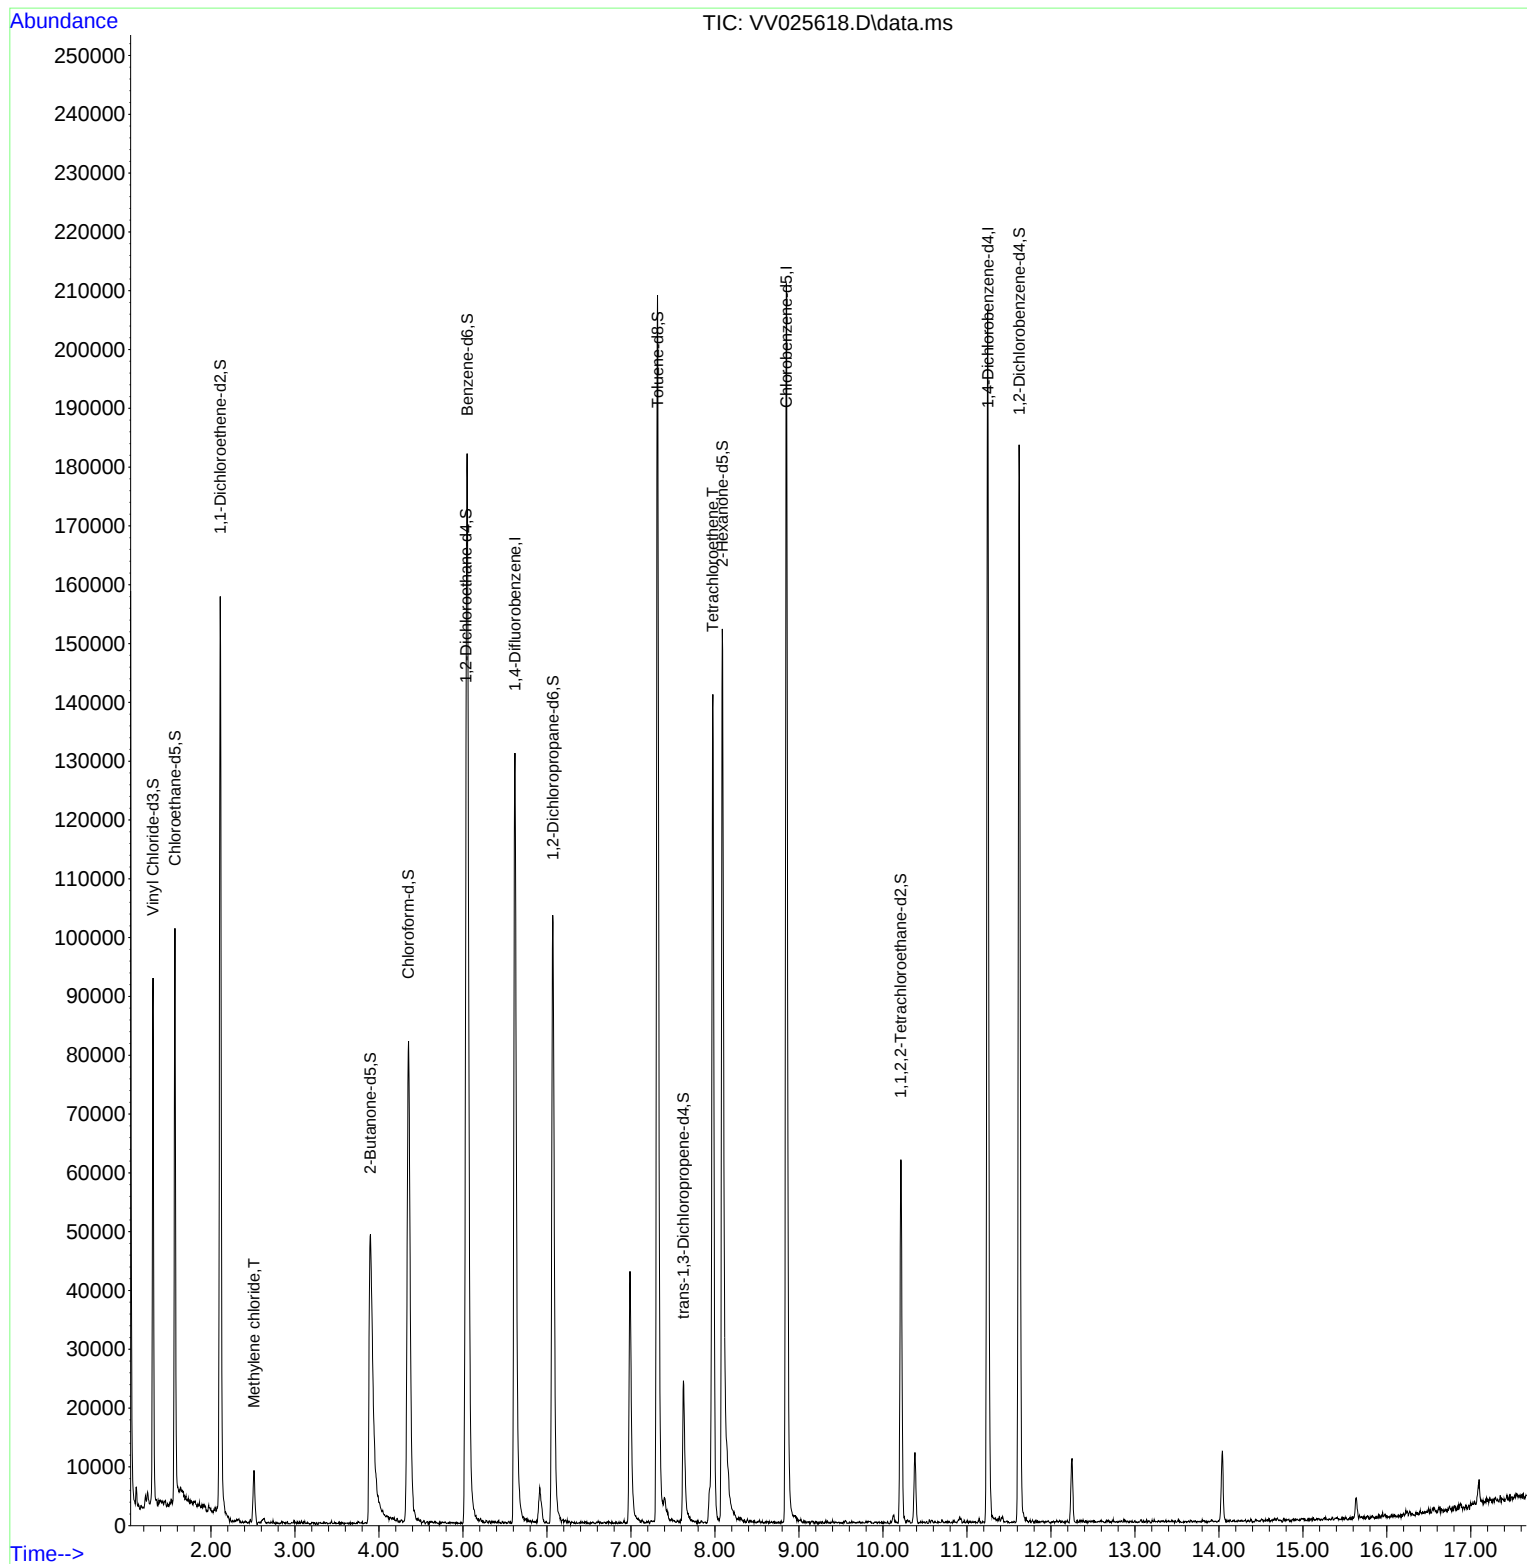


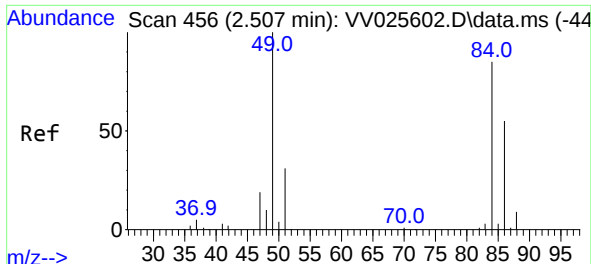

#16
Methylene chloride
Concen: 0.365 ug/L
RT: 2.513 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV025618.D
Acq: 18 Apr 2022 19:20

Instrument :
MSVOA_V
ClientSampleId :
EW6S0DL

Tgt Ion: 84 Resp: 3599
Ion Ratio Lower Upper
84 100
86 70.8 45.9 85.3
49 113.0 76.6 142.3

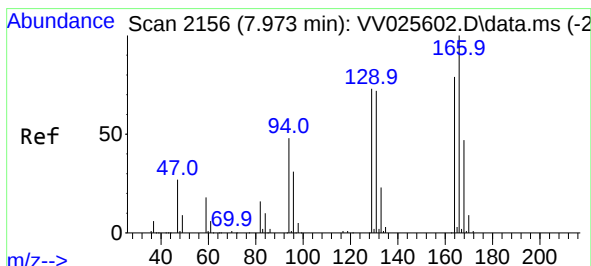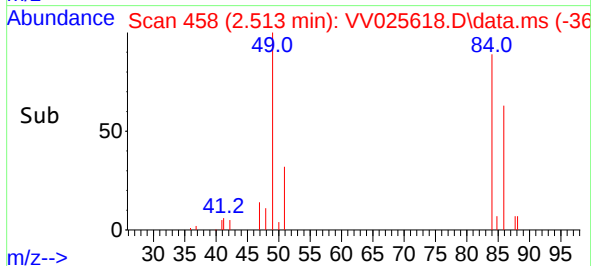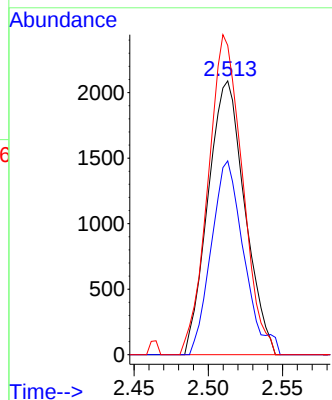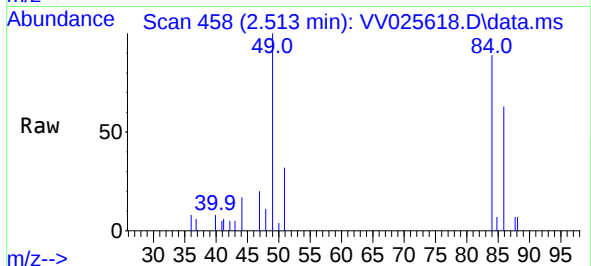

#47
Tetrachloroethene
Concen: 4.356 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. 0.003 min
Lab File: VV025618.D
Acq: 18 Apr 2022 19:20

Tgt Ion: 164 Resp: 30944
Ion Ratio Lower Upper
164 100
129 92.9 66.8 124.2
131 91.3 66.4 123.4
166 122.3 91.7 170.3

