
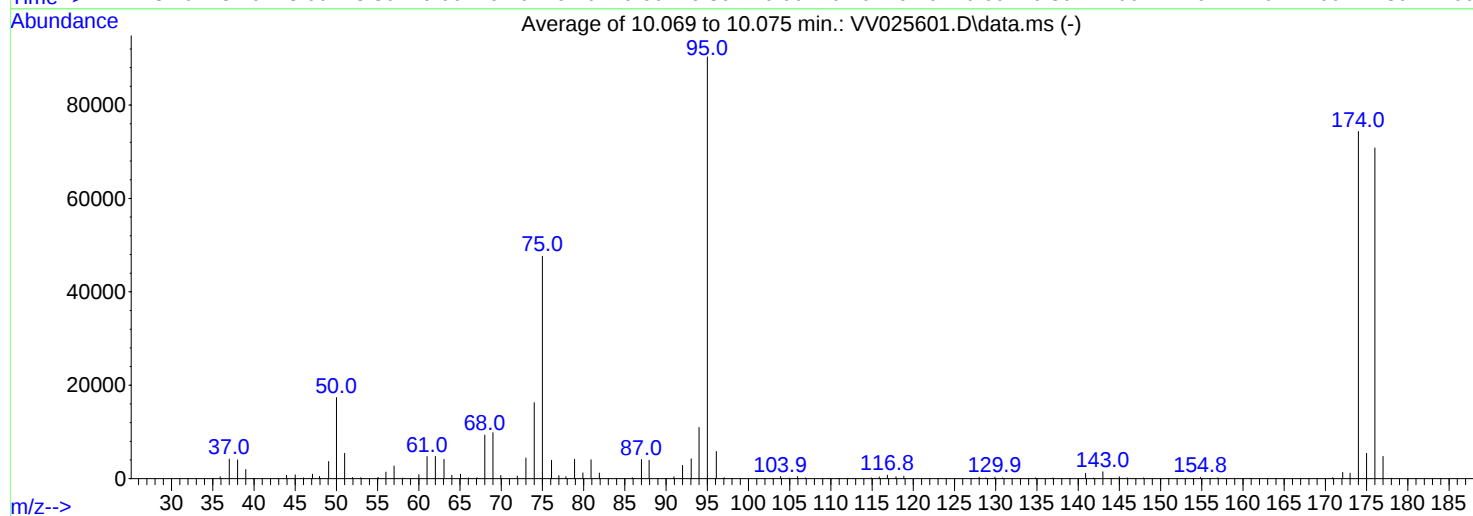


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041822\
 Data File : VV025601.D
 Acq On : 18 Apr 2022 08:58
 Operator : SY/MD
 Sample : BFB304
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB304

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Apr 20 02:46:45 2022

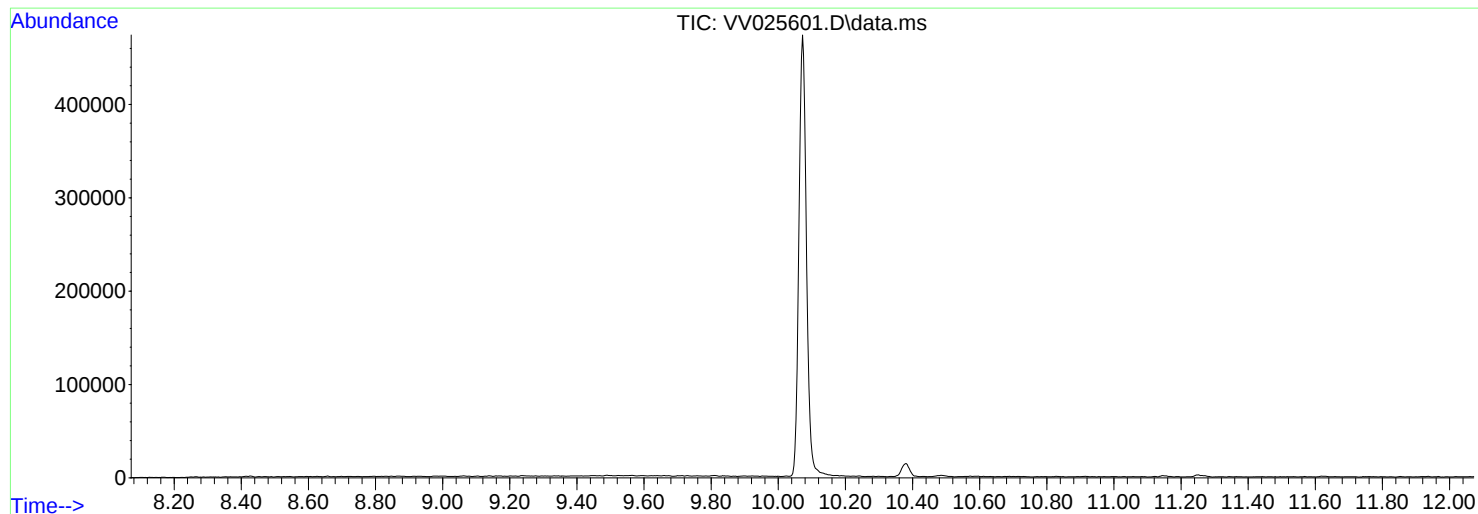

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	17381	PASS
75	95	30	80	52.7	47637	PASS
95	95	100	100	100.0	90312	PASS
96	95	5	9	6.4	5818	PASS
173	174	0.00	2	1.6	1159	PASS
174	95	50	120	82.3	74333	PASS
175	174	5	9	7.3	5416	PASS
176	174	95	105	95.3	70824	PASS
177	176	5	10	6.8	4782	PASS

m/z	Abundance
35.90	996.0
38.00	392.0
39.90	180.0
43.90	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB304

m/z	Abundance
36.00	1427.0
37.00	4109.0
38.00	4453.0
39.00	1991.0
40.10	226.0
44.00	928.0
45.00	807.0
46.00	189.0
47.10	864.0
47.90	480.0
49.10	3651.0
50.00	17152.0
51.00	5305.0
51.90	273.0
52.90	196.0
55.00	266.0
56.00	1402.0
57.00	2624.0
58.10	130.0
60.00	839.0
61.00	4608.0
62.00	4661.0
63.10	4091.0
64.00	733.0
65.10	928.0
66.10	163.0
67.00	205.0
68.00	9006.0
69.00	9775.0
70.00	779.0
72.00	526.0
73.00	4365.0
74.00	16222.0
75.00	47432.0
76.10	4062.0
77.00	614.0
77.90	370.0
78.90	4191.0
79.90	1250.0
80.90	4116.0
81.90	1246.0
85.90	274.0
87.00	4035.0
88.00	3872.0
90.90	373.0
92.00	2692.0
93.10	4297.0
94.00	10696.0
95.00	88896.0
96.10	5876.0
97.10	204.0
103.90	412.0
104.90	164.0
106.00	392.0
107.00	136.0
114.90	188.0
115.90	377.0
116.90	698.0
117.90	367.0
118.80	500.0
128.00	293.0
128.80	207.0
129.90	335.0
130.80	185.0
134.80	167.0
137.00	172.0
140.90	1116.0
141.80	115.0
143.00	1582.0
145.00	372.0
145.90	170.0
146.90	102.0
148.00	188.0
153.10	102.0
154.90	277.0
157.00	178.0
158.90	110.0
160.80	101.0
170.90	210.0
172.10	1317.0
173.00	1151.0
174.00	71280.0
175.00	5374.0
176.00	67808.0
177.00	4595.0
178.10	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB304

m/z	Abundance
35.10	213.0
36.00	1434.0
37.00	4324.0
38.00	4577.0
39.00	2041.0
40.10	203.0
44.00	951.0
45.00	849.0
46.00	176.0
47.10	981.0
48.00	493.0
49.00	3722.0
50.00	17936.0
51.00	5651.0
51.90	222.0
52.90	219.0
55.00	253.0
56.00	1482.0
57.00	2833.0
58.10	142.0
60.00	894.0
61.00	4886.0
62.00	4934.0
63.10	4298.0
64.00	727.0
65.10	993.0
66.10	177.0
67.00	221.0
68.00	9715.0
69.00	10142.0
70.00	697.0
71.90	580.0
73.00	4601.0
74.00	16904.0
75.00	49232.0
76.10	4090.0
77.00	650.0
77.90	408.0
78.90	4320.0
79.90	1274.0
80.90	4169.0
81.90	1242.0
85.90	310.0
87.00	4259.0
88.00	4120.0
91.00	404.0
92.00	2994.0
93.10	4387.0
94.00	11360.0
95.00	93296.0
96.10	6027.0
97.10	202.0
103.90	477.0
104.90	142.0
105.90	446.0
106.90	168.0
112.10	138.0
112.80	112.0
114.90	155.0
115.90	382.0
116.80	801.0
117.90	424.0
118.80	580.0
128.00	321.0
128.80	165.0
129.90	347.0
130.80	210.0
134.90	183.0
136.90	168.0
140.90	1192.0
141.90	146.0
143.00	1542.0
143.90	101.0
145.00	439.0
145.90	184.0
148.00	164.0
153.10	102.0
154.80	286.0
157.00	176.0
159.00	125.0
160.80	109.0
170.90	249.0
172.10	1377.0
173.00	1208.0
174.00	76936.0
175.00	5577.0
176.00	72936.0
177.00	4982.0
178.00	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB304

m/z	Abundance
36.00	1397.0
37.00	4070.0
38.00	4180.0
39.00	1865.0
40.00	192.0
42.90	106.0
44.00	946.0
45.00	771.0
46.00	157.0
47.10	1011.0
48.00	440.0
49.00	3676.0
50.00	17056.0
51.00	5244.0
52.00	228.0
53.00	235.0
55.10	261.0
56.00	1367.0
57.00	2627.0
58.00	153.0
60.00	848.0
61.00	4678.0
62.00	4733.0
63.00	4085.0
64.00	698.0
65.00	918.0
66.00	157.0
67.10	185.0
68.00	9288.0
69.00	9575.0
69.90	609.0
71.90	546.0
73.00	4299.0
74.00	15704.0
75.00	46248.0
76.10	3708.0
77.00	650.0
77.80	409.0
78.90	3964.0
79.90	1153.0
80.90	3833.0
81.90	1086.0
83.10	110.0
86.10	249.0
87.00	4030.0
87.90	3857.0
91.00	429.0
92.00	2848.0
93.00	4086.0
94.00	10871.0
95.00	88744.0
96.10	5550.0
97.00	213.0
102.90	103.0
103.90	515.0
105.00	138.0
105.90	495.0
106.90	168.0
109.70	105.0
110.80	125.0
112.10	119.0
112.80	125.0
114.90	136.0
115.80	335.0
116.80	777.0
117.90	410.0
118.90	564.0
128.00	313.0
128.80	155.0
129.90	332.0
130.90	168.0
134.90	174.0
136.90	175.0
140.90	1140.0
141.90	137.0
143.00	1329.0
143.90	115.0
145.00	436.0
146.00	184.0
147.90	162.0
153.90	116.0
154.80	273.0
156.90	151.0
159.00	127.0
160.90	103.0
170.90	236.0
172.10	1350.0
173.00	1119.0
174.00	74784.0
175.00	5296.0
176.00	71728.0
177.00	4768.0

Instrument :
MSVOA_V
ClientSampleId :
BFB304

177.90

107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB304