

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041824\
 Data File : VW035278.D
 Acq On : 18 Apr 2024 13:14
 Operator : SY/MD
 Sample : P2144-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 19 01:42:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:53:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	345985	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	338214	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	141612	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	147948	44.278	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.560%		
7) Chloroethane-d5	1.523	69	132417	45.626	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.260%		
11) 1,1-Dichloroethene-d2	2.056	65	64843	44.271	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.540%		
21) 2-Butanone-d5	3.786	46	194578	98.188	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.190%		
24) Chloroform-d	4.246	84	283516	50.466	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.940%		
26) 1,2-Dichloroethane-d4	4.937	65	181929	51.007	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.020%		
32) Benzene-d6	4.957	84	566614	49.875	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.740%		
36) 1,2-Dichloropropane-d6	5.986	67	185932	51.539	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	103.080%		
41) Toluene-d8	7.240	98	469384	45.877	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.760%		
43) trans-1,3-Dichloroprop...	7.551	79	75028	42.780	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.560%		
47) 2-Hexanone-d5	8.024	63	118040	86.541	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.540%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	250690	50.462	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	100.920%		
66) 1,2-Dichlorobenzene-d4	11.558	152	169936	53.447	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.900%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.915	75	4025	0.838	ug/L	# 57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035278.D
Acq On : 18 Apr 2024 13:14
Operator : SY/MD
Sample : P2144-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 19 01:42:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

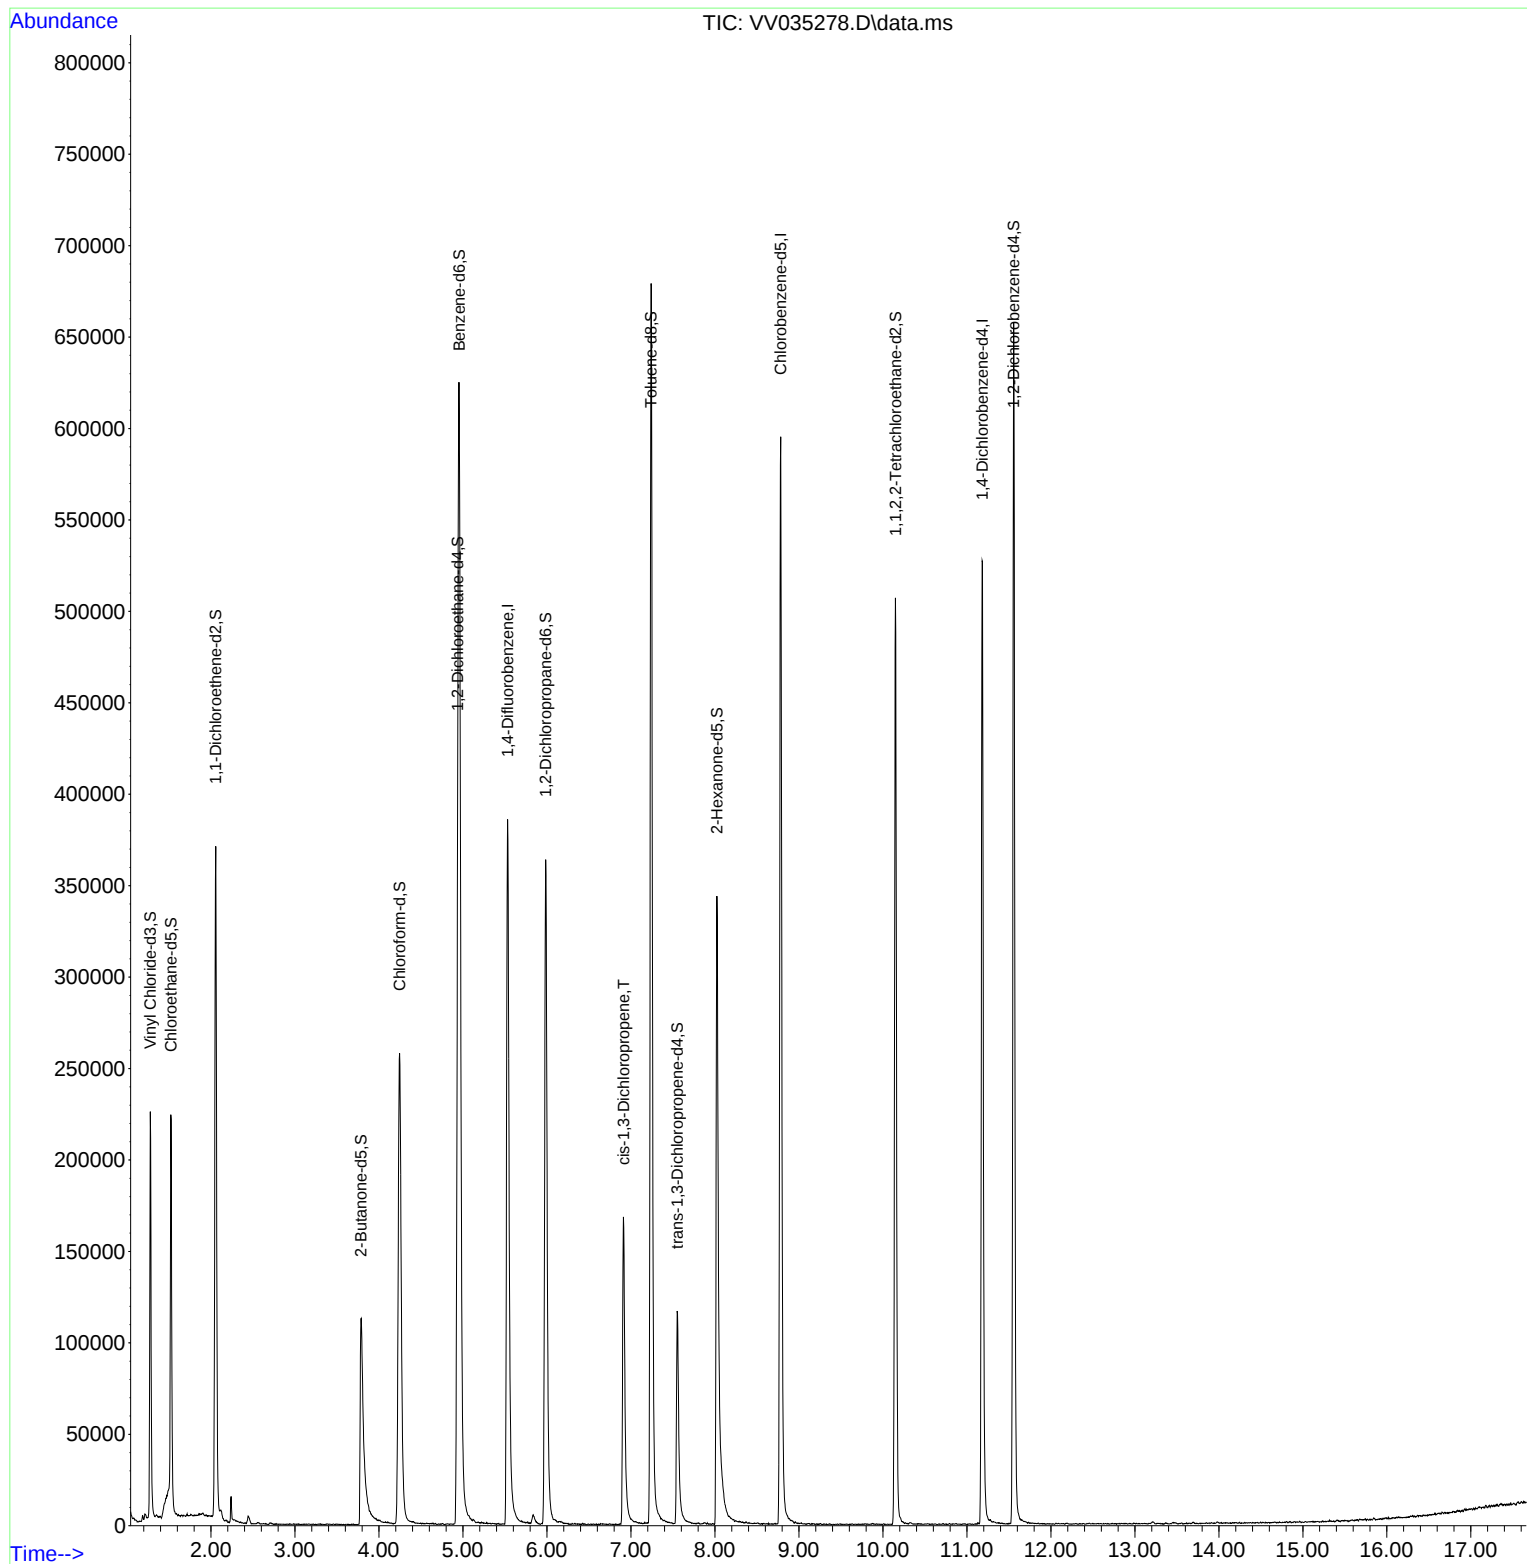

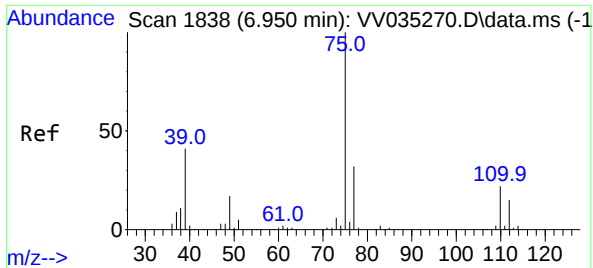

#39
 cis-1,3-Dichloropropene
 Concen: 0.838 ug/L
 RT: 6.915 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV035278.D
 Acq: 18 Apr 2024 13:14

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion:	75	Resp:	4025
Ion Ratio	Lower	Upper	
75	100		
77	55.2	21.9	40.7#

