




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035288.D
Acq On : 18 Apr 2024 17:14
Operator : SY/MD
Sample : P2158-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/23/2024
Supervised By :Semsettin Yesilyurt 04/23/2024

Quant Time: Apr 19 01:43:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

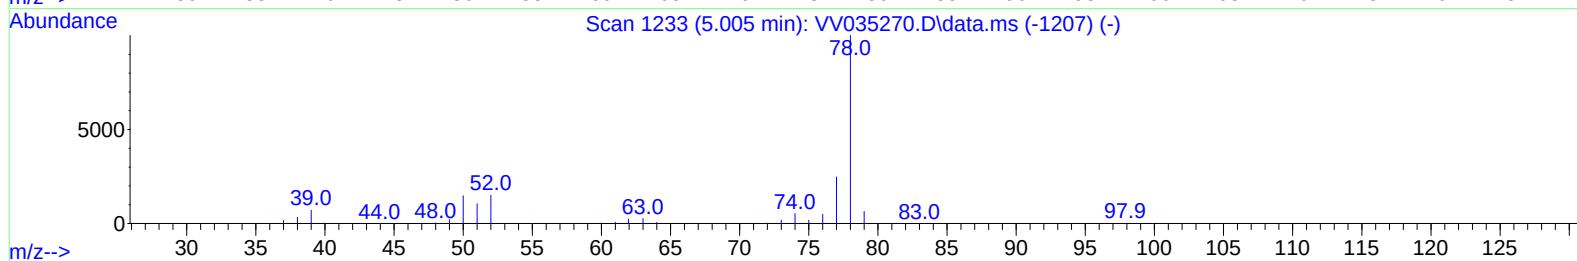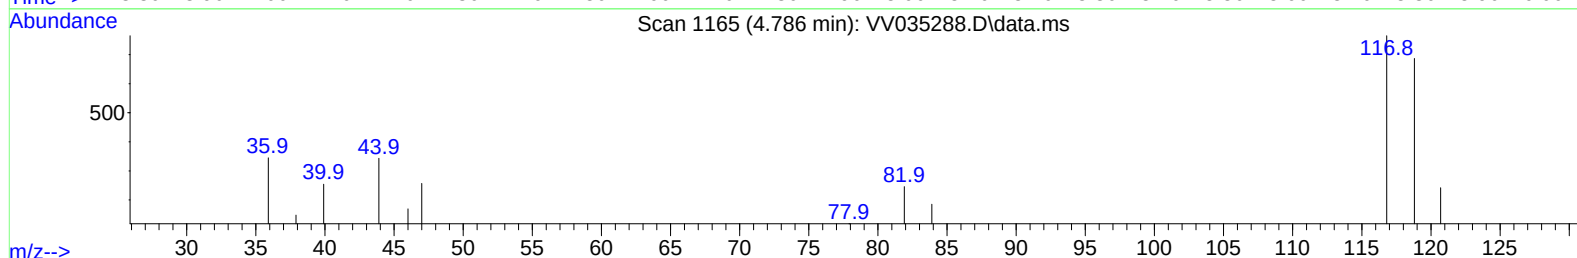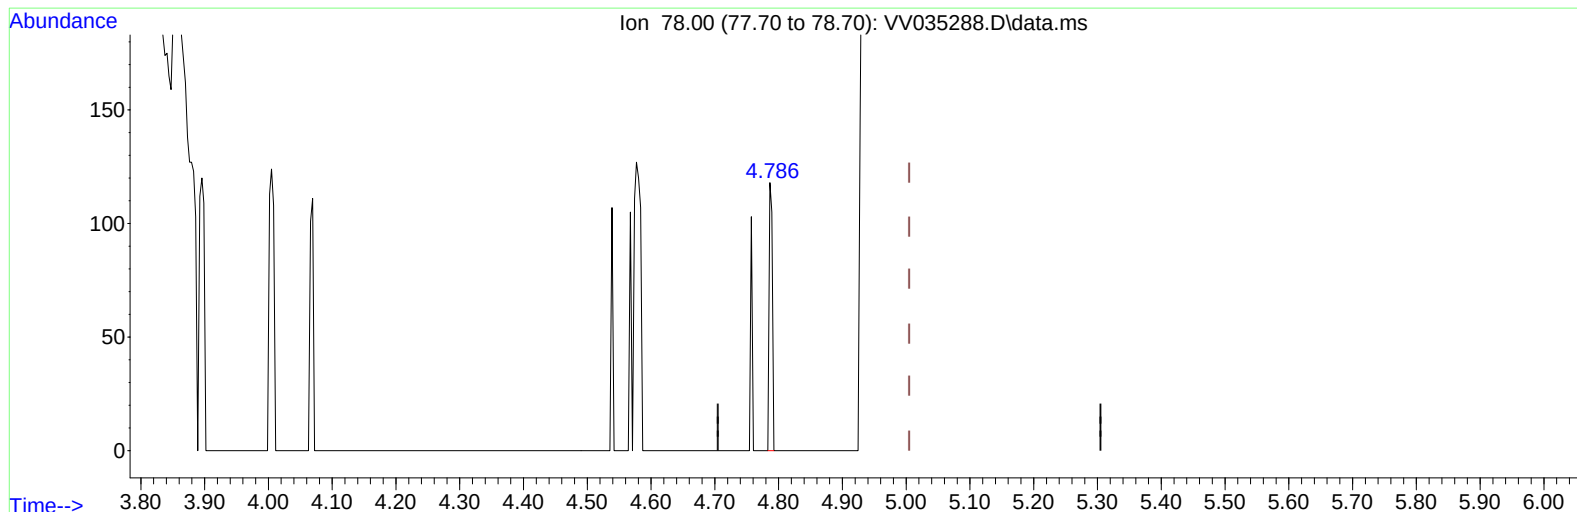

TIC: VV035288.D\data.ms

(33) Benzene (T)

4.786min (-0.219) 0.00 ug/L

response 43		
Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035288.D
Acq On : 18 Apr 2024 17:14
Operator : SY/MD
Sample : P2158-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE2

Manual IntegrationsAPPROVED

Quant Time: Apr 19 01:43:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/23/2024
Supervised By :Semsettin Yesilyurt 04/23/2024

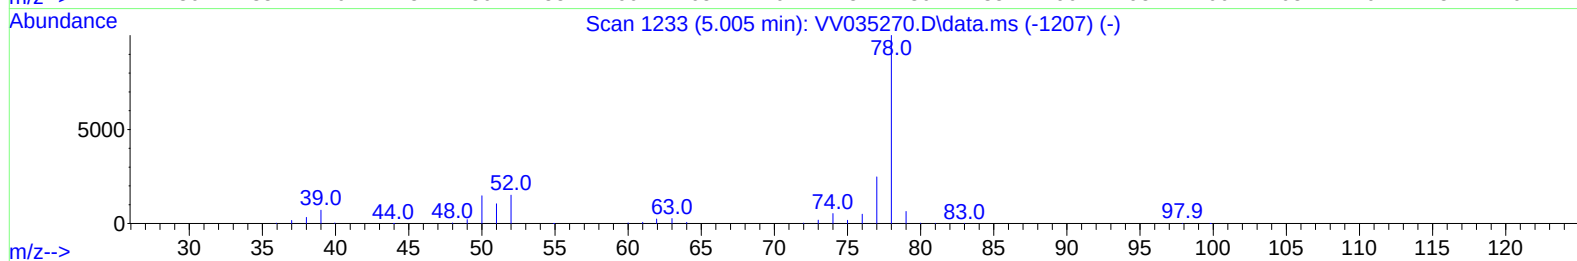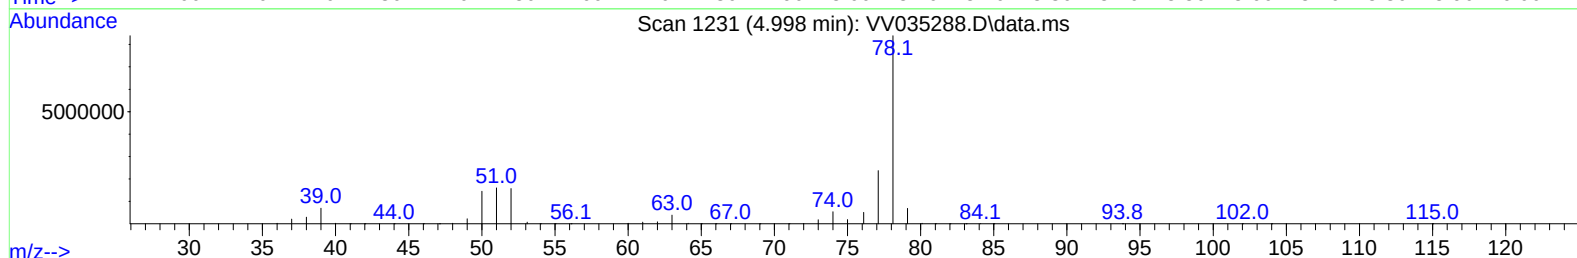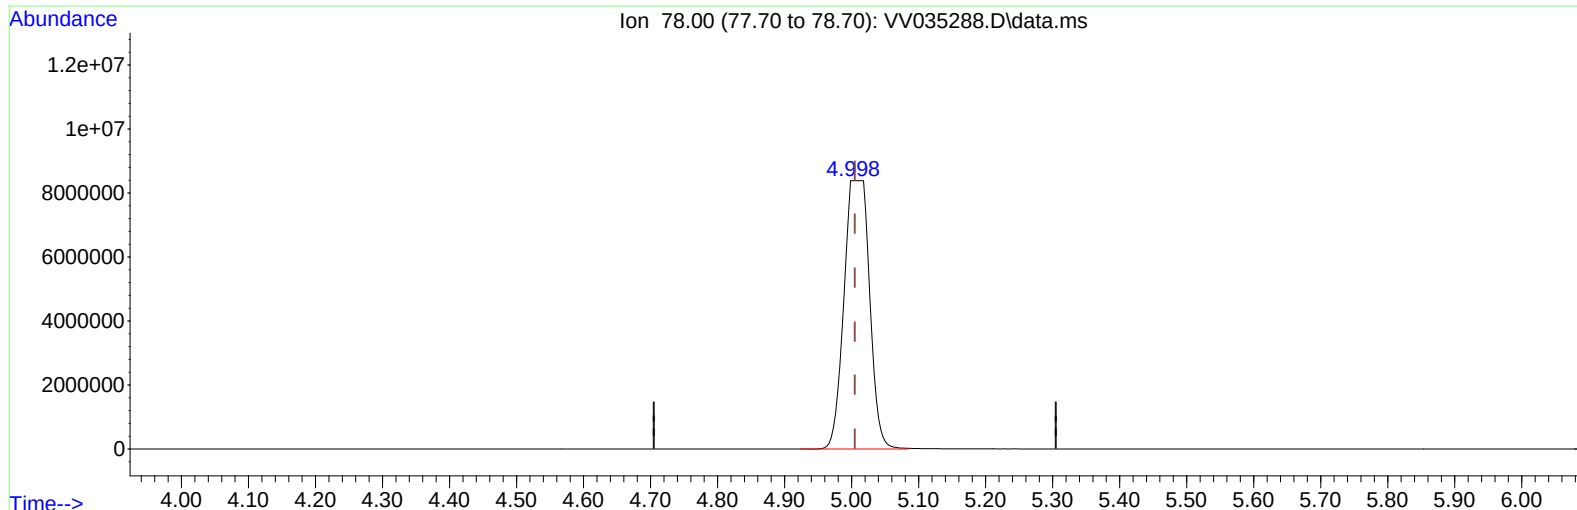

TIC: VV035288.D\data.ms

(33) Benzene (T)

4.998min (-0.006) 1865.71 ug/L m

response 22337166

Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035288.D
Acq On : 18 Apr 2024 17:14
Operator : SY/MD
Sample : P2158-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/23/2024
Supervised By :Semsettin Yesilyurt 04/23/2024

Quant Time: Apr 19 01:43:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

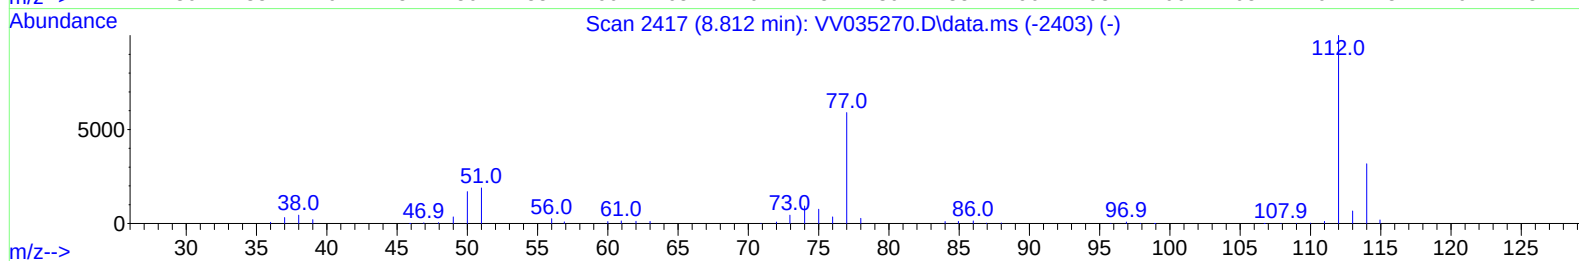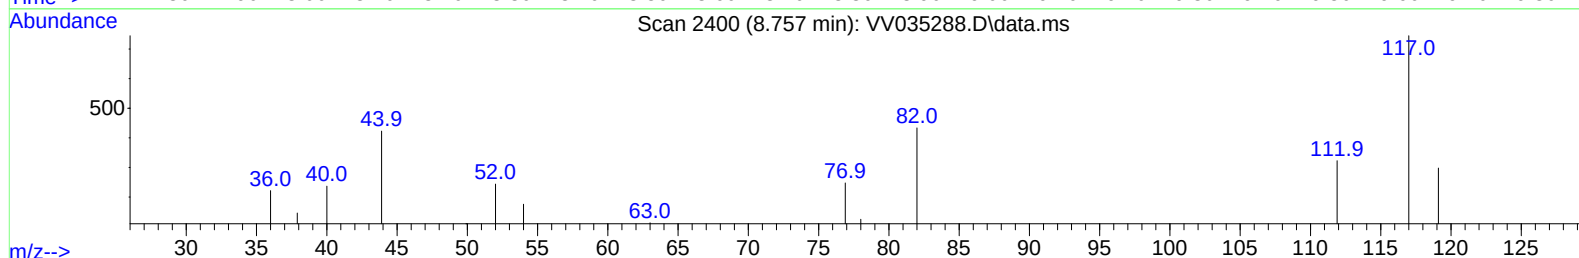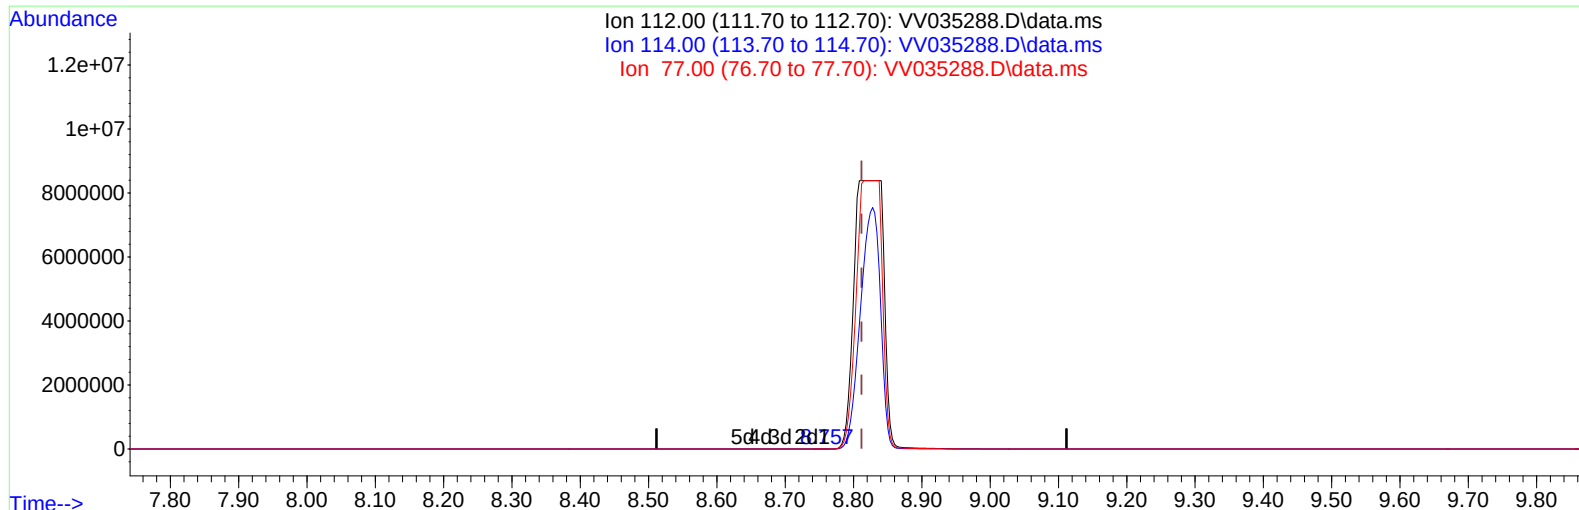

TIC: VV035288.D\data.ms

(51) Chlorobenzene (T)

8.757min (-0.055) 0.01 ug/L

response

114

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	31.50	0.00#
77.00	59.30	76.78#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035288.D
Acq On : 18 Apr 2024 17:14
Operator : SY/MD
Sample : P2158-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/23/2024
Supervised By :Semsettin Yesilyurt 04/23/2024

Quant Time: Apr 19 01:43:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

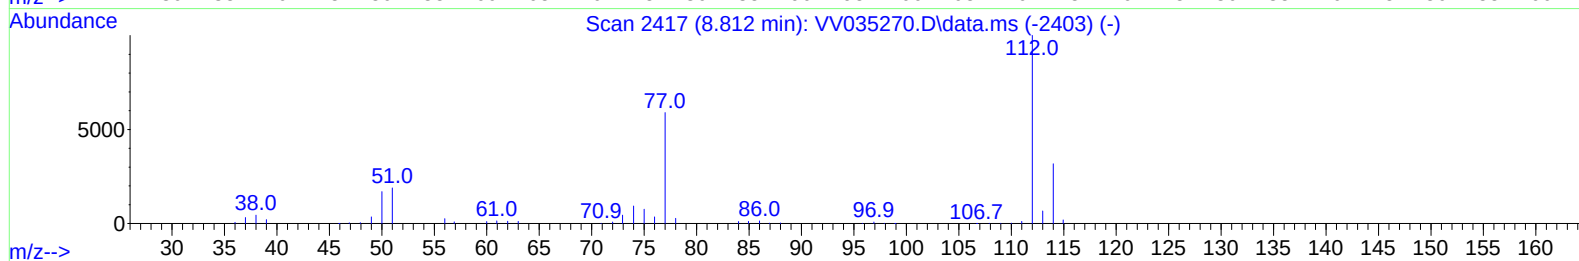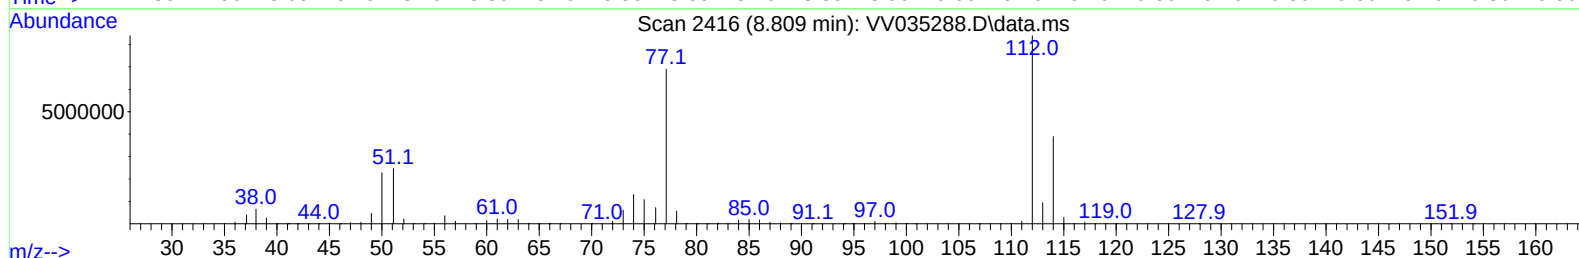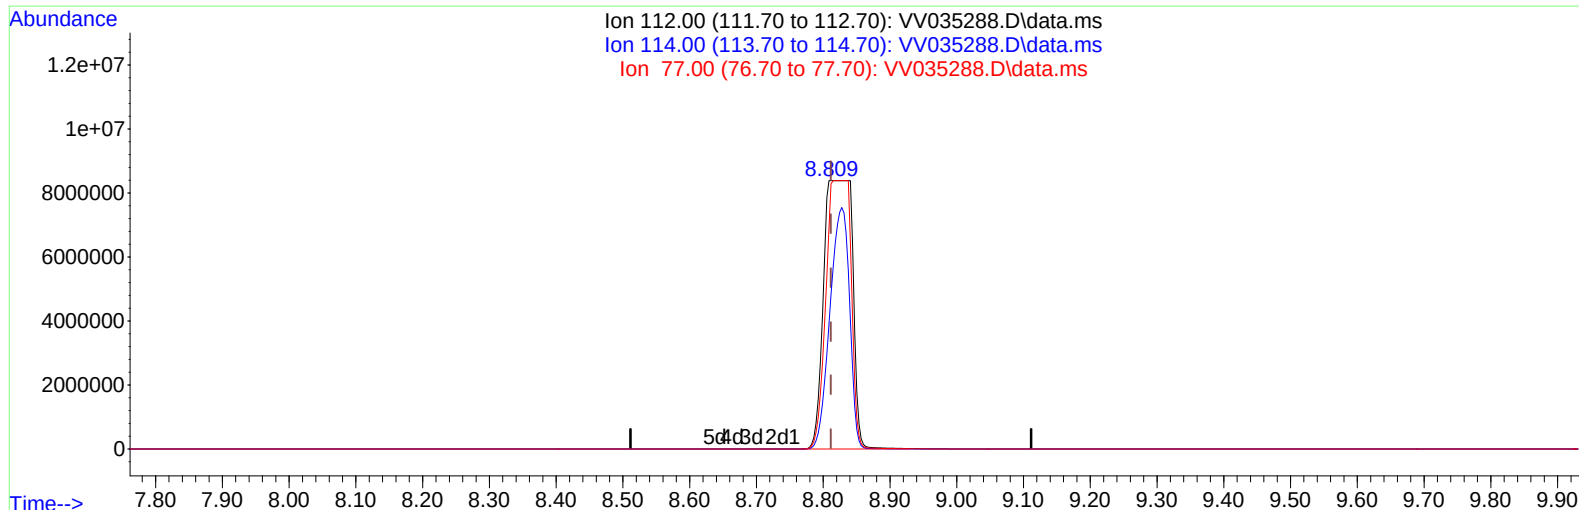

TIC: VV035288.D\data.ms

(51) Chlorobenzene (T)

8.809min (-0.003) 3080.45 ug/L m

response 25025009

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	31.50	46.40#
77.00	59.30	82.14#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035288.D
 Acq On : 18 Apr 2024 17:14
 Operator : SY/MD
 Sample : P2158-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE2

Manual IntegrationsAPPROVED

Quant Time: Apr 19 01:43:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:53:36 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/23/2024
 Supervised By :Semsettin Yesilyurt 04/23/2024

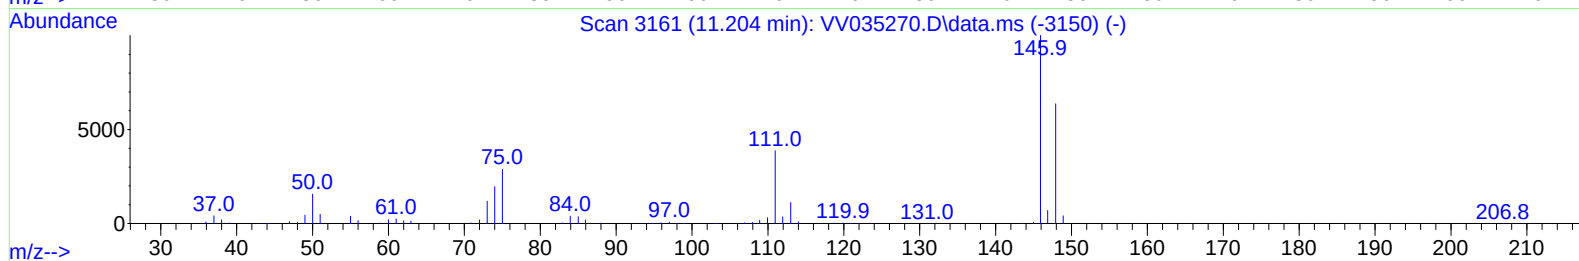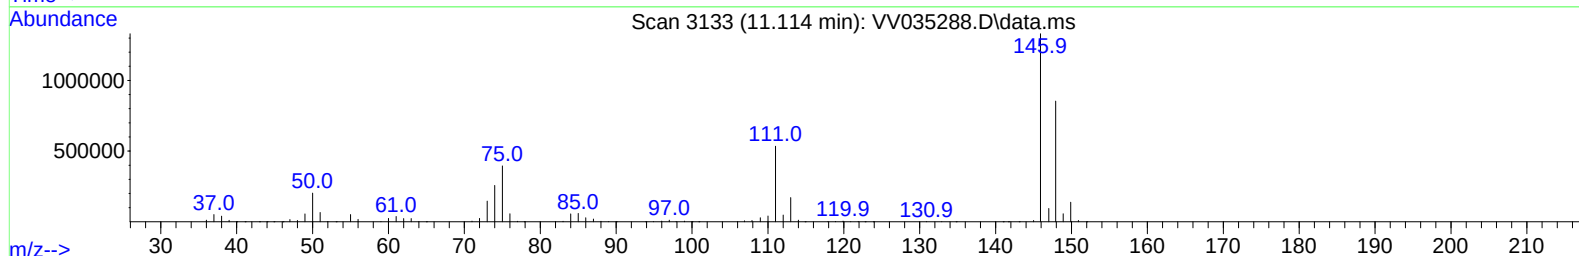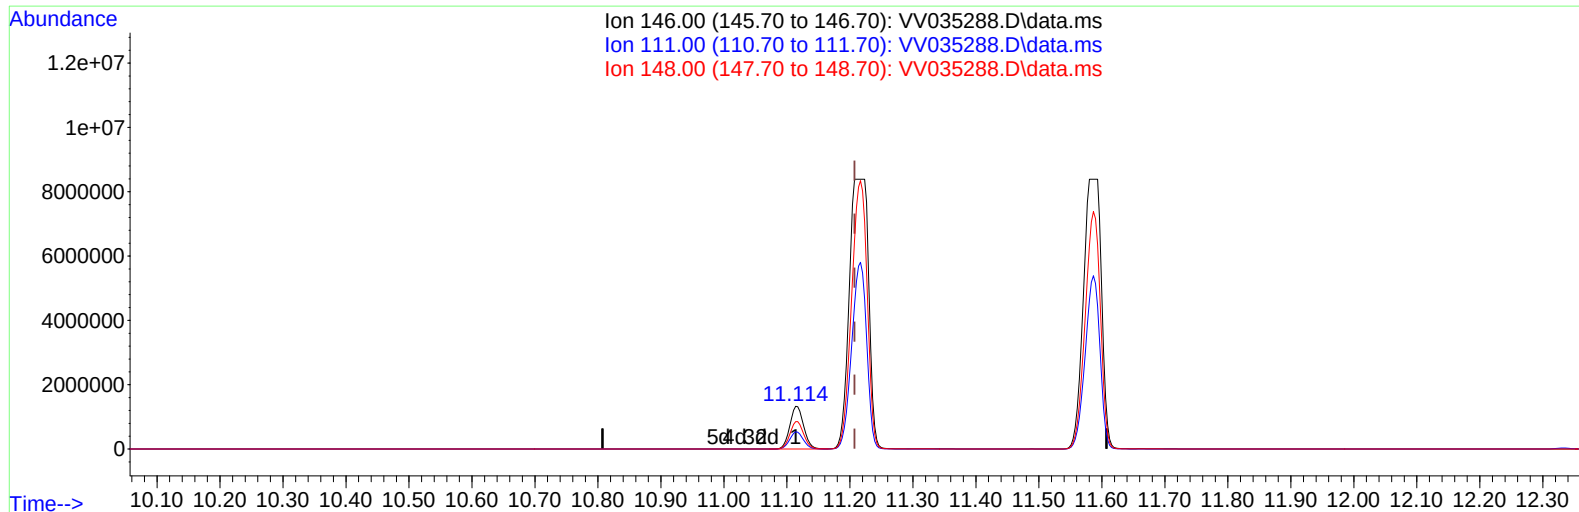

TIC: VV035288.D\data.ms

(65) 1,4-Dichlorobenzene (T)

11.114min (-0.093) 268.07 ug/L

response 2015905

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	39.10	40.17
148.00	63.20	64.20
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035288.D
Acq On : 18 Apr 2024 17:14
Operator : SY/MD
Sample : P2158-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE2

Manual IntegrationsAPPROVED

Quant Time: Apr 19 01:43:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/23/2024
Supervised By :Semsettin Yesilyurt 04/23/2024

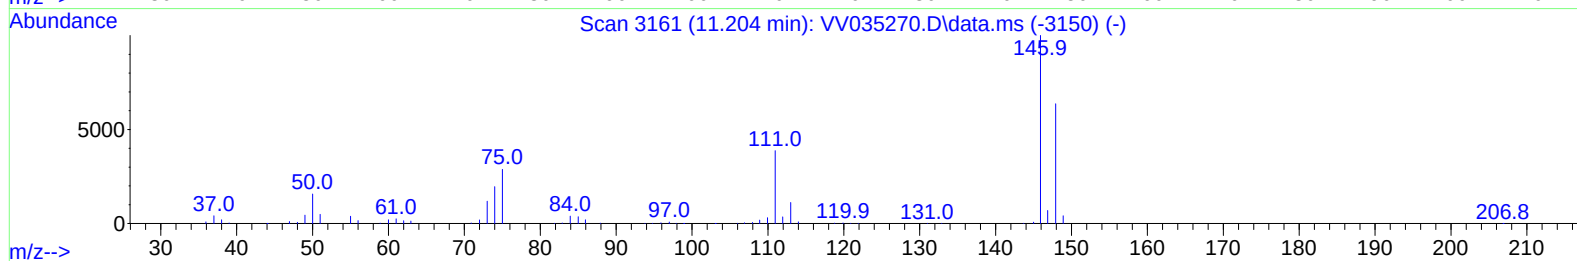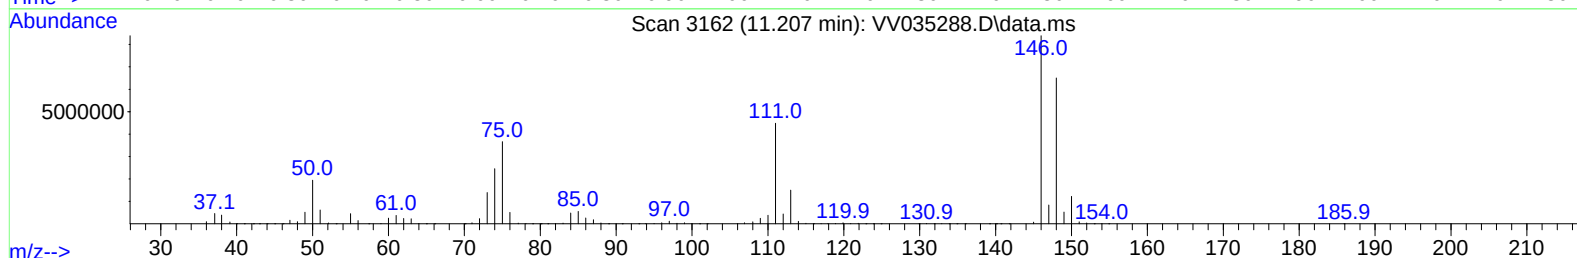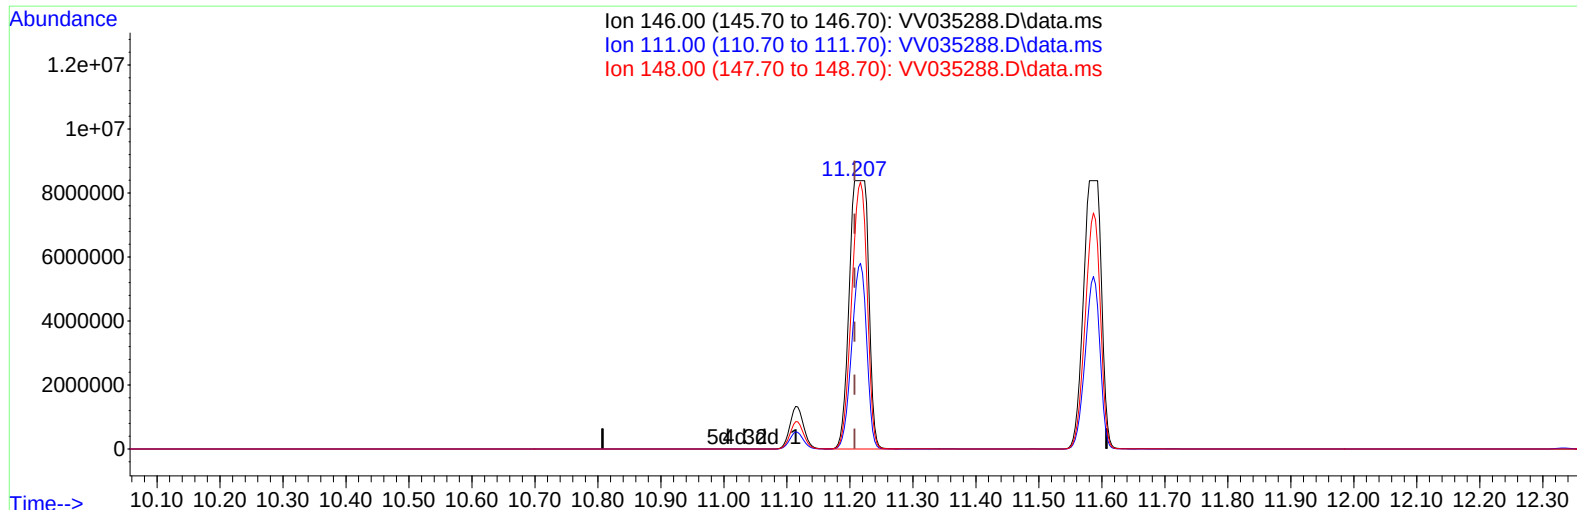

TIC: VV035288.D\data.ms

(65) 1,4-Dichlorobenzene (T)

11.207min (+ 0.000) 2376.68 ug/L m

response 17873113

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	39.10	53.45#
148.00	63.20	77.56
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035288.D
Acq On : 18 Apr 2024 17:14
Operator : SY/MD
Sample : P2158-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE2

Manual IntegrationsAPPROVED

Quant Time: Apr 19 01:43:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/23/2024
Supervised By :Semsettin Yesilyurt 04/23/2024

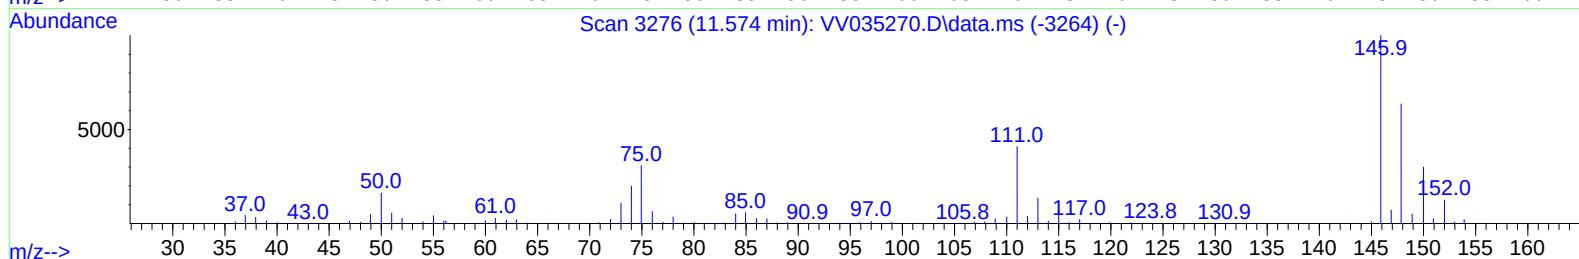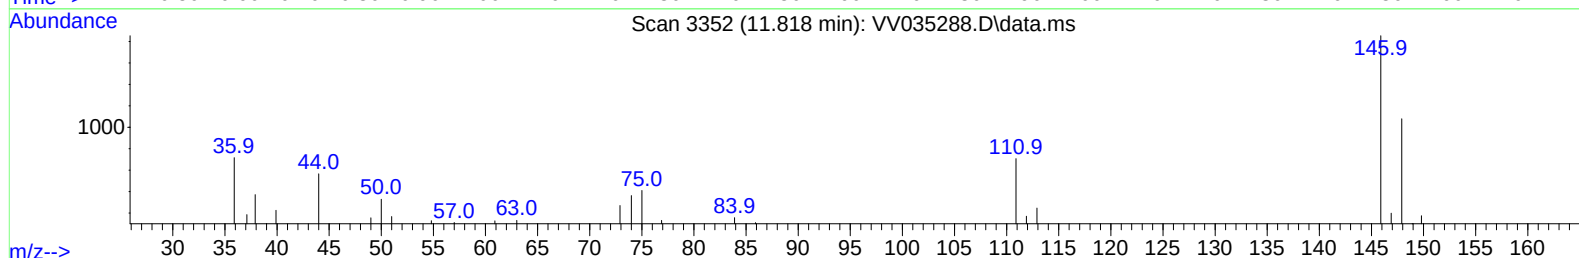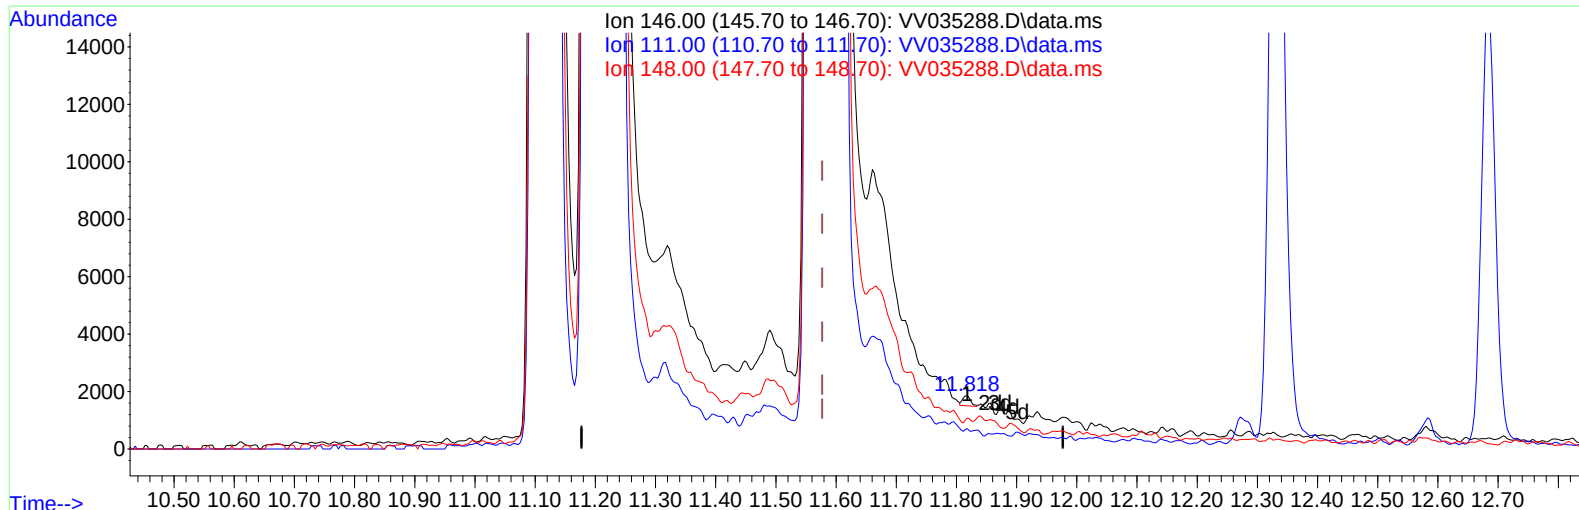

TIC: VV035288.D\data.ms

(67) 1,2-Dichlorobenzene (T)

11.818min (+ 0.241) 0.04 ug/L

response 322

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	43.30	38.19
148.00	64.40	58.20
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035288.D
Acq On : 18 Apr 2024 17:14
Operator : SY/MD
Sample : P2158-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/23/2024
Supervised By :Semsettin Yesilyurt 04/23/2024

Quant Time: Apr 19 01:43:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

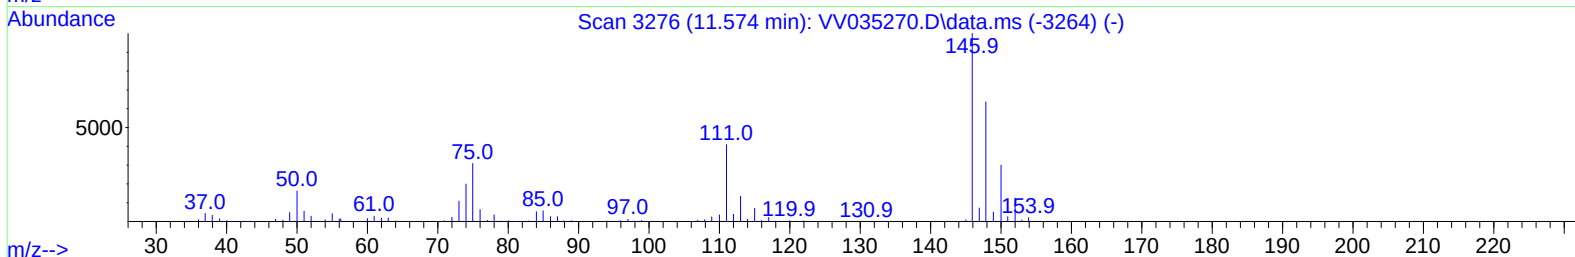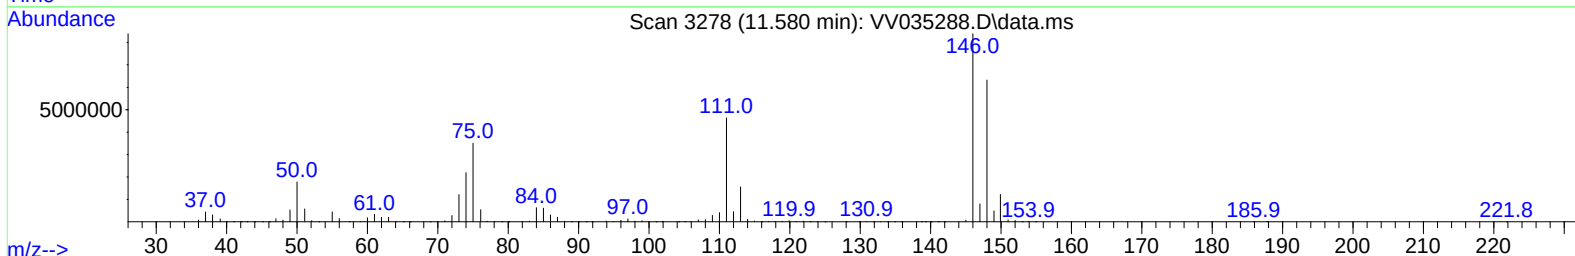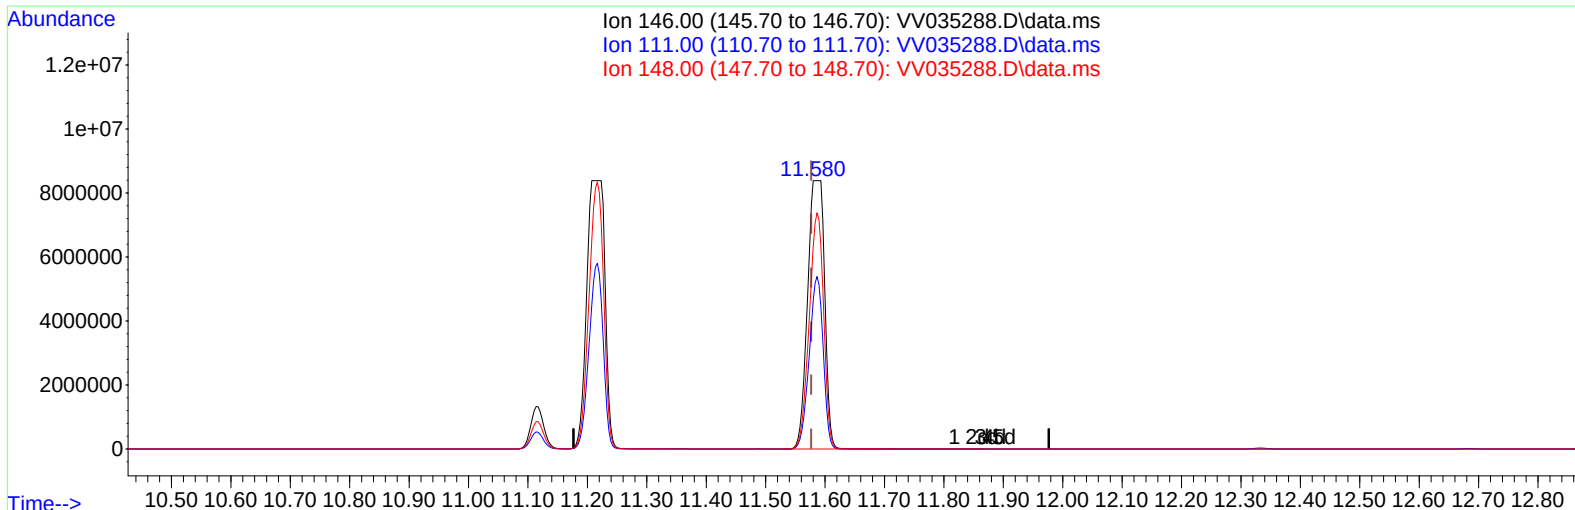

TIC: VV035288.D\data.ms

(67) 1,2-Dichlorobenzene (T)

11.580min (+ 0.003) 2279.99 ug/L m

response 16796107

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	43.30	55.23#
148.00	64.40	75.37
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041824\
 Data File : VW035288.D
 Acq On : 18 Apr 2024 17:14
 Operator : SY/MD
 Sample : P2158-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE2

Manual IntegrationsAPPROVED

Quant Time: Apr 19 01:43:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:53:36 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/23/2024
 Supervised By :Semsettin Yesilyurt 04/23/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	361443	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	367158	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	219503	50.000	ug/L	# 0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	157125	45.013	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	90.020%	
7) Chloroethane-d5	1.526	69	134168	44.253	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	88.500%	
11) 1,1-Dichloroethene-d2	2.056	65	67984	44.430	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.860%	
21) 2-Butanone-d5	3.786	46	213077	102.924	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	102.920%	
24) Chloroform-d	4.246	84	287573	48.999	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.000%	
26) 1,2-Dichloroethane-d4	4.941	65	184517	49.520	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.040%	
32) Benzene-d6	4.960	84	586007	47.515	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.040%	
36) 1,2-Dichloropropane-d6	5.986	67	184360	47.075	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.140%	
41) Toluene-d8	7.243	98	498328	44.866	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	89.740%	
43) trans-1,3-Dichloroprop...	7.555	79	81560	42.838	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.680%	
47) 2-Hexanone-d5	8.024	63	150444	101.603	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	101.600%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	266011	49.324	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.640%	
66) 1,2-Dichlorobenzene-d4	11.564	152	239839	48.665	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	97.340%	
Target Compounds						
29) Cyclohexane	4.580	56	7445	1.619	ug/L	99
31) Carbon tetrachloride	4.735	117	58153	14.336	ug/L	98
33) Benzene	4.998	78	22337166m	1865.706	ug/L	
51) Chlorobenzene	8.809	112	25025009m	3080.454	ug/L	
64) 1,3-Dichlorobenzene	11.114	146	2015905	272.603	ug/L	98
65) 1,4-Dichlorobenzene	11.207	146	17873113m	2376.680	ug/L	
67) 1,2-Dichlorobenzene	11.580	146	16796107m	2279.985	ug/L	
69) 1,3,5-Trichlorobenzene	12.583	180	17027	3.195	ug/L	96
70) 1,2,4-trichlorobenzene	13.201	180	9057763	1850.170	ug/L	98
72) 1,2,3-Trichlorobenzene	13.677	180	2357273	488.480	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035288.D
Acq On : 18 Apr 2024 17:14
Operator : SY/MD
Sample : P2158-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/23/2024
Supervised By :Semsettin Yesilyurt 04/23/2024

Quant Time: Apr 19 01:43:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

