

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035273.D
 Acq On : 18 Apr 2024 11:12
 Operator : SY/MD
 Sample : P2170-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0001

Quant Time: Apr 19 01:42:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:53:36 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.529	114	306098	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.783	117	304678	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.185	152	131483	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	182718	61.809	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	123.620%	
7) Chloroethane-d5		1.526	69	141094	54.951	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	109.900%	
11) 1,1-Dichloroethene-d2		2.056	65	79972	61.715	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	123.420%	
21) 2-Butanone-d5		3.786	46	225105	128.394	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	128.390%	
24) Chloroform-d		4.243	84	348573	70.132	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	140.260%#	
26) 1,2-Dichloroethane-d4		4.934	65	220944	70.017	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	140.040%#	
32) Benzene-d6		4.953	84	696508	68.057	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	136.120%#	
36) 1,2-Dichloropropane-d6		5.982	67	226731	69.766	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	139.540%#	
41) Toluene-d8		7.240	98	595027	64.559	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	129.120%#	
43) trans-1,3-Dichloroprop...		7.551	79	93491	59.175	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	118.340%	
47) 2-Hexanone-d5		8.024	63	144784	117.833	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	117.830%	
56) 1,1,2,2-Tetrachloroeth...		10.149	84	297844	66.552	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	133.100%#	
66) 1,2-Dichlorobenzene-d4		11.558	152	212503	71.984	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	143.960%#	
Target Compounds							Qvalue
13) Acetone		2.121	43	10552	6.556	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035273.D
Acq On : 18 Apr 2024 11:12
Operator : SY/MD
Sample : P2170-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0001

Quant Time: Apr 19 01:42:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

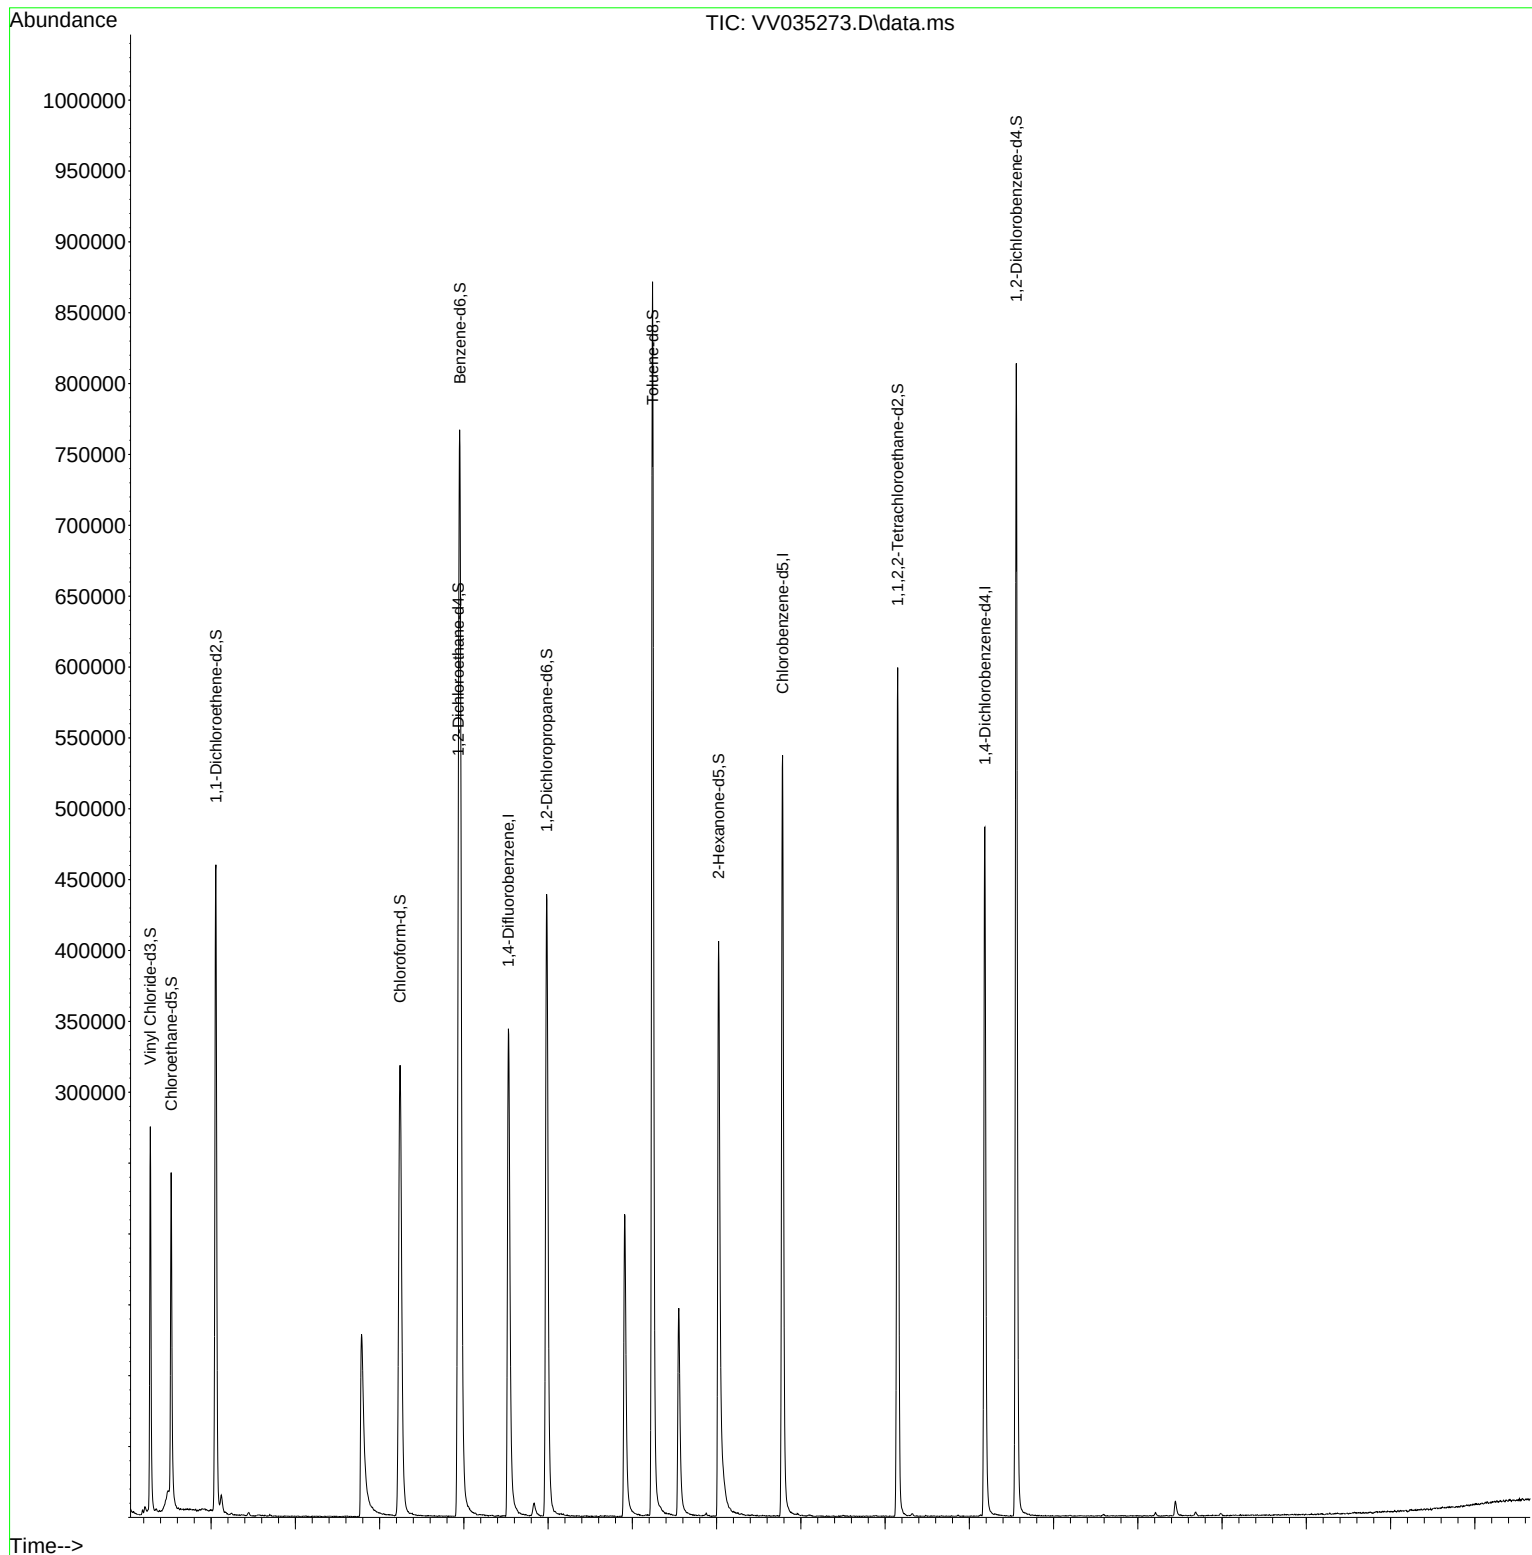

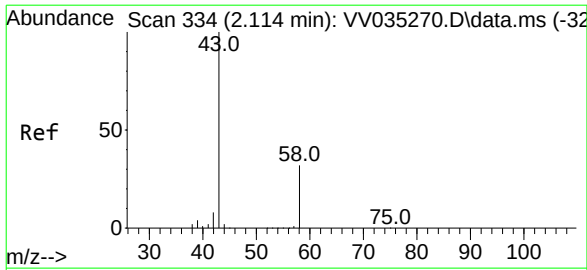

#13

Acetone

Concen: 6.556 ug/L

RT: 2.121 min Scan# 33

Delta R.T. 0.003 min

Lab File: VV035273.D


Acq: 18 Apr 2024 11:12

Instrument :

MSVOA_V

ClientSampleId :

E0001

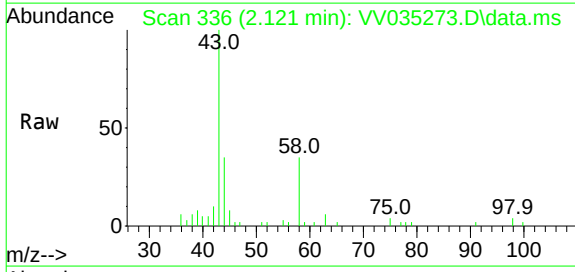

Tgt Ion: 43 Resp: 10552

Ion Ratio Lower Upper

43 100

58 33.2 0.0 66.0

