

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035273.D
 Acq On : 18 Apr 2024 11:12
 Operator : SY/MD
 Sample : P2170-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	49	rBV	3250	3113	0.15%	0.023%
2	1.214	49	54	63	rVV3	4809	7172	0.35%	0.054%
3	1.278	67	74	90	rVB	271267	297216	14.61%	2.242%
4	1.526	144	151	174	rVB	237038	298316	14.66%	2.250%
5	2.056	305	316	330	rBV	455381	662849	32.58%	4.999%
6	2.446	430	437	447	rVB5	2465	3712	0.18%	0.028%
7	2.606	485	487	494	rVB6	530	458	0.02%	0.003%
8	2.638	494	497	505	rVB4	832	849	0.04%	0.006%
9	2.696	510	515	520	rBV4	1048	1012	0.05%	0.008%
10	2.960	595	597	601	rVB3	404	263	0.01%	0.002%
11	3.127	644	649	654	rVB4	424	438	0.02%	0.003%
12	3.204	669	673	677	rBV2	417	453	0.02%	0.003%
13	3.285	694	698	700	rBV	305	271	0.01%	0.002%
14	3.455	748	751	754	rBV2	280	249	0.01%	0.002%
15	3.555	775	782	786	rBV3	375	413	0.02%	0.003%
16	3.581	786	790	793	rBV2	366	312	0.02%	0.002%
17	3.786	845	854	892	rBV	128318	379026	18.63%	2.859%
18	4.188	976	979	980	rBV	523	306	0.02%	0.002%
19	4.243	980	996	1031	rVV	317713	819307	40.27%	6.179%
20	4.561	1092	1095	1098	rBV4	449	329	0.02%	0.002%
21	4.580	1098	1101	1104	rVV2	310	247	0.01%	0.002%
22	4.706	1135	1140	1143	rBV3	497	382	0.02%	0.003%
23	4.741	1147	1151	1154	rVB3	352	288	0.01%	0.002%
24	4.799	1167	1169	1173	rVB2	454	242	0.01%	0.002%
25	4.950	1199	1216	1263	rBV2	766569	2034744	100.00%	15.346%
26	5.275	1312	1317	1318	rBV2	483	365	0.02%	0.003%
27	5.304	1323	1326	1330	rBV3	471	502	0.02%	0.004%
28	5.384	1348	1351	1354	rBV	361	277	0.01%	0.002%
29	5.407	1354	1358	1362	rVB5	607	448	0.02%	0.003%
30	5.452	1367	1372	1373	rBV2	519	314	0.02%	0.002%
31	5.529	1386	1396	1435	rBV	343917	736891	36.22%	5.557%
32	5.786	1474	1476	1480	rBV3	388	295	0.01%	0.002%
33	5.834	1480	1491	1502	rBV5	8792	19055	0.94%	0.144%
34	5.918	1515	1517	1521	rBV2	519	324	0.02%	0.002%
35	5.982	1524	1537	1565	rBV	438657	921670	45.30%	6.951%
36	6.249	1617	1620	1624	rVB3	644	572	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035273.D
 Acq On : 18 Apr 2024 11:12
 Operator : SY/MD
 Sample : P2170-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.275	1626	1628	1634	rBV4	443	419	0.02%	0.003%
38	6.404	1664	1668	1669	rVB	425	255	0.01%	0.002%
39	6.429	1669	1676	1678	rBV2	465	497	0.02%	0.004%
40	6.445	1678	1681	1682	rVV2	509	327	0.02%	0.002%
41	6.471	1687	1689	1693	rVB3	513	344	0.02%	0.003%
42	6.574	1717	1721	1723	rVB2	444	313	0.02%	0.002%
43	6.622	1730	1736	1738	rBV4	639	588	0.03%	0.004%
44	6.674	1751	1752	1757	rBV4	456	362	0.02%	0.003%
45	6.741	1770	1773	1778	rVB2	465	348	0.02%	0.003%
46	6.770	1779	1782	1785	rVB2	512	346	0.02%	0.003%
47	6.908	1815	1825	1852	rBV	213156	414077	20.35%	3.123%
48	7.240	1917	1928	1966	rBV	870466	1542809	75.82%	11.636%
49	7.551	2015	2025	2054	rBV	146157	277507	13.64%	2.093%
50	7.722	2076	2078	2082	rVB3	707	357	0.02%	0.003%
51	7.741	2082	2084	2088	rBV3	513	399	0.02%	0.003%
52	7.879	2123	2127	2133	rVB3	1890	1623	0.08%	0.012%
53	7.960	2147	2152	2156	rBV4	480	402	0.02%	0.003%
54	8.024	2163	2172	2225	rBV	405680	853751	41.96%	6.439%
55	8.452	2303	2305	2311	rVB3	512	420	0.02%	0.003%
56	8.481	2311	2314	2320	rVB4	814	692	0.03%	0.005%
57	8.629	2358	2360	2364	rVB2	449	255	0.01%	0.002%
58	8.783	2397	2408	2438	rBV	536786	905308	44.49%	6.828%
59	8.957	2460	2462	2465	rBV4	757	339	0.02%	0.003%
60	9.092	2501	2504	2506	rVV	570	368	0.02%	0.003%
61	9.191	2528	2535	2536	rBV2	346	284	0.01%	0.002%
62	9.214	2539	2542	2546	rVV3	398	366	0.02%	0.003%
63	9.262	2555	2557	2561	rVB2	409	272	0.01%	0.002%
64	9.304	2567	2570	2576	rBV3	517	434	0.02%	0.003%
65	9.500	2629	2631	2636	rVB5	568	493	0.02%	0.004%
66	9.590	2652	2659	2662	rBV3	509	420	0.02%	0.003%
67	9.632	2667	2672	2678	rVB3	355	346	0.02%	0.003%
68	9.741	2702	2706	2712	rBV3	338	336	0.02%	0.003%
69	9.776	2712	2717	2721	rBV3	377	399	0.02%	0.003%
70	9.863	2741	2744	2748	rVV2	390	361	0.02%	0.003%
71	9.886	2748	2751	2761	rVB4	658	889	0.04%	0.007%
72	10.056	2799	2804	2806	rBV2	485	318	0.02%	0.002%
73	10.149	2820	2833	2856	rBV	598886	957723	47.07%	7.223%
74	10.407	2909	2913	2915	rBV	467	328	0.02%	0.002%
75	10.481	2932	2936	2937	rBV2	636	323	0.02%	0.002%
76	10.670	2992	2995	2998	rVB	398	268	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035273.D
 Acq On : 18 Apr 2024 11:12
 Operator : SY/MD
 Sample : P2170-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.789	3029	3032	3036	rBV2	451	329	0.02%	0.002%
78	10.866	3051	3056	3064	rVB4	888	1117	0.05%	0.008%
79	11.124	3133	3136	3137	rBV2	539	366	0.02%	0.003%
80	11.133	3137	3139	3144	rVV6	780	702	0.03%	0.005%
81	11.185	3144	3155	3189	rVV	485978	781644	38.41%	5.895%
82	11.300	3189	3191	3200	rVB6	879	1168	0.06%	0.009%
83	11.442	3232	3235	3239	rBV3	350	257	0.01%	0.002%
84	11.490	3247	3250	3252	rVB2	500	247	0.01%	0.002%
85	11.558	3259	3271	3297	rBV	813195	1283700	63.09%	9.681%
86	11.809	3347	3349	3352	rBV	428	260	0.01%	0.002%
87	11.828	3352	3355	3359	rVB2	514	358	0.02%	0.003%
88	12.590	3586	3592	3595	rBV3	1070	1149	0.06%	0.009%
89	12.902	3686	3689	3692	rBV4	356	305	0.01%	0.002%
90	13.072	3738	3742	3746	rBV3	452	466	0.02%	0.004%
91	13.210	3778	3785	3795	rVB6	2482	3559	0.17%	0.027%
92	13.281	3805	3807	3811	rBV	382	298	0.01%	0.002%
93	13.445	3851	3858	3873	rVB2	9785	16349	0.80%	0.123%
94	13.686	3928	3933	3944	rVB7	2694	4192	0.21%	0.032%
95	13.763	3953	3957	3961	rVB3	705	610	0.03%	0.005%
96	13.815	3970	3973	3976	rBV2	394	280	0.01%	0.002%
97	13.985	4020	4026	4035	rVB5	1672	2613	0.13%	0.020%
98	14.217	4095	4098	4101	rVB3	828	489	0.02%	0.004%
99	14.587	4211	4213	4216	rBV3	405	242	0.01%	0.002%
100	14.886	4303	4306	4309	rBV	628	436	0.02%	0.003%

Sum of corrected areas: 13259482




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035273.D
Acq On : 18 Apr 2024 11:12
Operator : SY/MD
Sample : P2170-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

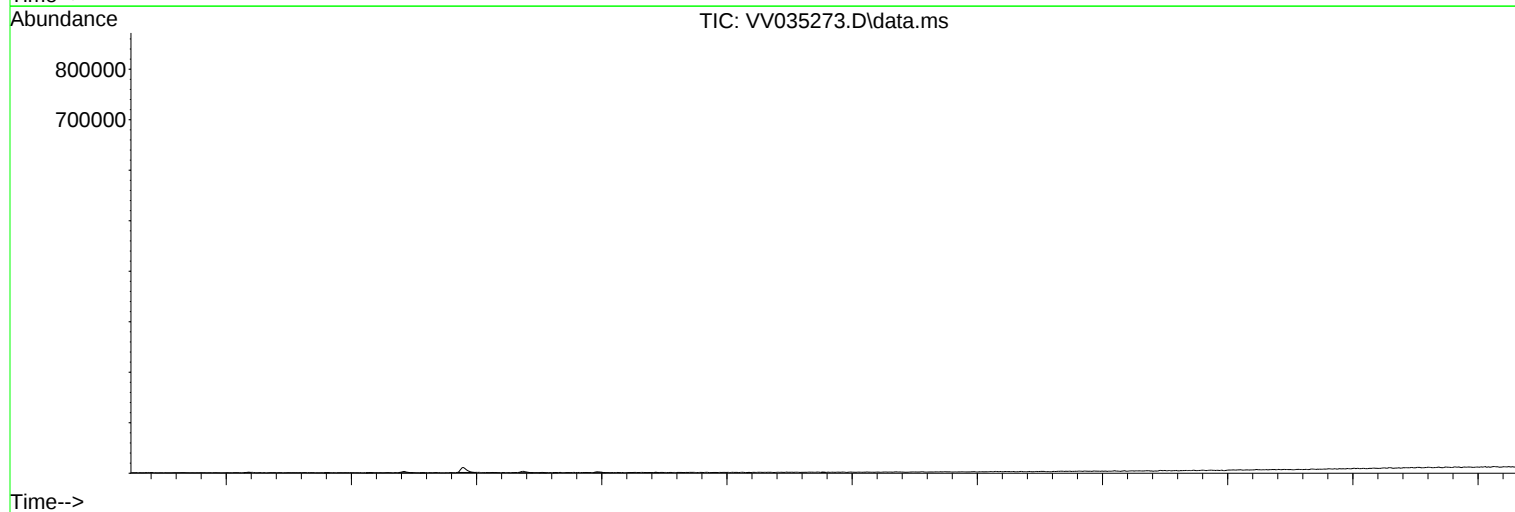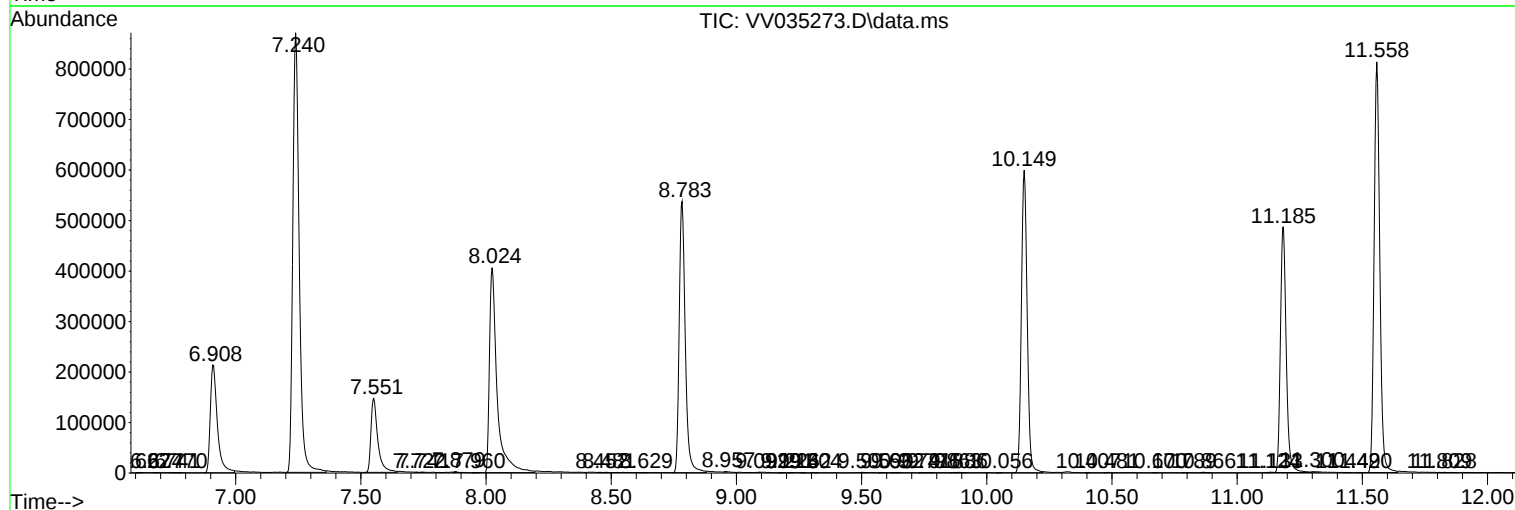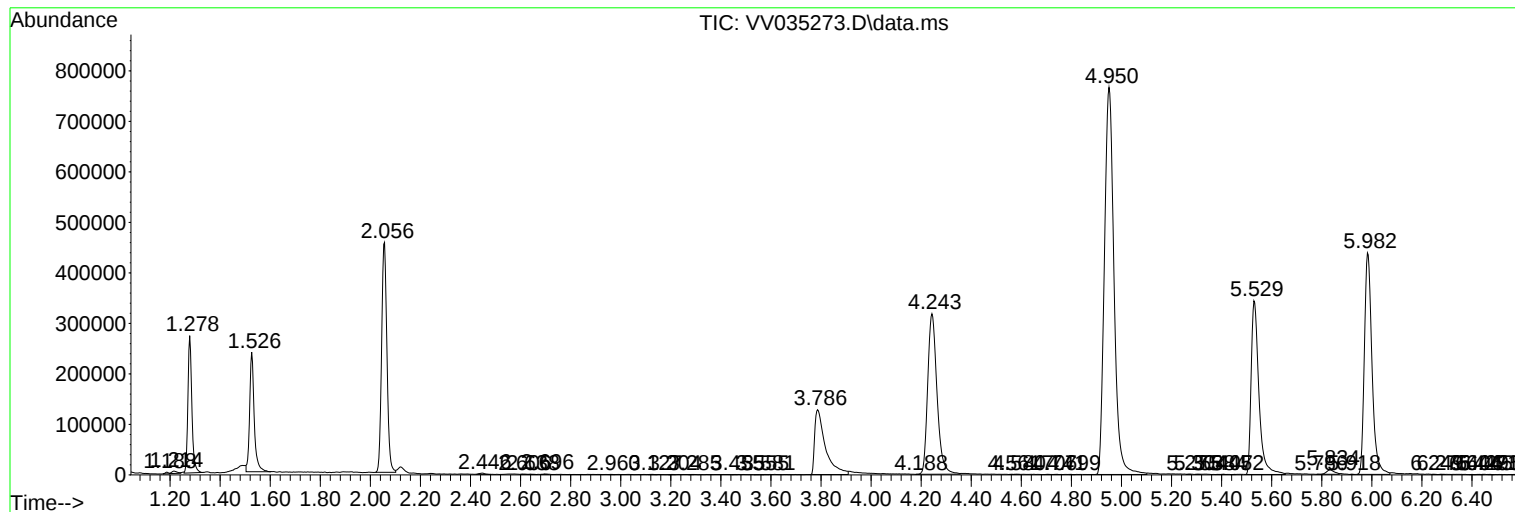

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035273.D
Acq On : 18 Apr 2024 11:12
Operator : SY/MD
Sample : P2170-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035273.D
Acq On : 18 Apr 2024 11:12
Operator : SY/MD
Sample : P2170-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------