

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035274.D
 Acq On : 18 Apr 2024 11:37
 Operator : SY/MD
 Sample : P2158-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035274.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	24	rVB3	9805	10197	0.45%	0.070%
2	1.278	67	74	87	rBV	241188	259411	11.39%	1.786%
3	1.523	144	150	165	rVB	216867	266430	11.69%	1.835%
4	2.056	306	316	331	rBV	397987	576864	25.32%	3.972%
5	2.516	457	459	461	rBV2	470	248	0.01%	0.002%
6	2.934	586	589	594	rVB3	452	329	0.01%	0.002%
7	2.960	595	597	599	rBV2	473	234	0.01%	0.002%
8	3.092	635	638	640	rBV2	268	158	0.01%	0.001%
9	3.166	656	661	665	rBV2	457	478	0.02%	0.003%
10	3.195	668	670	672	rVV2	191	65	0.00%	0.000%
11	3.220	675	678	682	rBV2	140	103	0.00%	0.001%
12	3.246	682	686	689	rBV2	286	229	0.01%	0.002%
13	3.262	689	691	694	rVB	235	89	0.00%	0.001%
14	3.291	694	700	702	rBV	255	301	0.01%	0.002%
15	3.378	723	727	729	rBV2	301	146	0.01%	0.001%
16	3.462	752	753	756	rBV2	209	69	0.00%	0.000%
17	3.494	761	763	765	rBV	161	91	0.00%	0.001%
18	3.516	767	770	772	rBV	128	92	0.00%	0.001%
19	3.545	778	779	780	rBV	112	25	0.00%	0.000%
20	3.606	791	798	799	rBV	347	258	0.01%	0.002%
21	3.642	807	809	810	rBV	155	49	0.00%	0.000%
22	3.661	813	815	816	rBV	315	92	0.00%	0.001%
23	3.716	828	832	833	rBV	253	188	0.01%	0.001%
24	3.786	846	854	899	rBV	118131	354209	15.55%	2.439%
25	4.243	981	996	1031	rBV	272918	709346	31.13%	4.885%
26	4.834	1177	1180	1182	rBV3	413	287	0.01%	0.002%
27	4.870	1188	1191	1195	rBV2	250	201	0.01%	0.001%
28	4.899	1198	1200	1201	rBV	317	167	0.01%	0.001%
29	4.950	1201	1216	1258	rBV2	658873	1767913	77.59%	12.174%
30	5.445	1368	1370	1372	rVB2	476	184	0.01%	0.001%
31	5.471	1376	1378	1381	rVB2	304	125	0.01%	0.001%
32	5.532	1386	1397	1427	rBV	342533	728921	31.99%	5.019%
33	5.986	1525	1538	1561	rBV	387261	806149	35.38%	5.551%
34	6.336	1645	1647	1650	rBV2	330	174	0.01%	0.001%
35	6.368	1653	1657	1659	rBV2	414	280	0.01%	0.002%
36	6.391	1659	1664	1668	rBV5	579	492	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035274.D
 Acq On : 18 Apr 2024 11:37
 Operator : SY/MD
 Sample : P2158-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.429	1672	1676	1678	rBV2	324	234	0.01%	0.002%
38	6.449	1681	1682	1686	rVB3	426	201	0.01%	0.001%
39	6.478	1686	1691	1694	rVB2	313	253	0.01%	0.002%
40	6.510	1698	1701	1702	rBV	146	97	0.00%	0.001%
41	6.542	1709	1711	1714	rVB2	207	75	0.00%	0.001%
42	6.561	1714	1717	1719	rBV2	216	129	0.01%	0.001%
43	6.603	1727	1730	1731	rBV	403	160	0.01%	0.001%
44	6.613	1731	1733	1736	rVV3	432	218	0.01%	0.002%
45	6.706	1757	1762	1763	rBV	416	254	0.01%	0.002%
46	6.757	1777	1778	1781	rVB2	246	94	0.00%	0.001%
47	6.777	1781	1784	1788	rVB2	452	294	0.01%	0.002%
48	6.805	1791	1793	1796	rVB2	300	141	0.01%	0.001%
49	6.834	1797	1802	1806	rBV2	199	179	0.01%	0.001%
50	6.867	1810	1812	1815	rVB2	291	167	0.01%	0.001%
51	6.912	1815	1826	1857	rBV	181760	357063	15.67%	2.459%
52	7.140	1895	1897	1901	rBV3	444	401	0.02%	0.003%
53	7.240	1917	1928	1957	rBV	738600	1323519	58.09%	9.114%
54	7.551	2016	2025	2049	rBV	126248	236082	10.36%	1.626%
55	7.876	2115	2126	2135	rBV4	3669	7140	0.31%	0.049%
56	7.985	2158	2160	2161	rBV4	142	48	0.00%	0.000%
57	8.024	2163	2172	2215	rBV	361609	745331	32.71%	5.132%
58	8.622	2355	2358	2360	rBV	264	128	0.01%	0.001%
59	8.638	2360	2363	2364	rBV3	296	171	0.01%	0.001%
60	8.783	2397	2408	2456	rBV2	559913	1182667	51.91%	8.144%
61	9.146	2517	2521	2525	rBV2	516	429	0.02%	0.003%
62	9.198	2534	2537	2540	rVB3	358	204	0.01%	0.001%
63	9.217	2541	2543	2546	rBV2	348	218	0.01%	0.002%
64	9.391	2592	2597	2598	rBV2	295	229	0.01%	0.002%
65	9.471	2619	2622	2623	rBV	230	138	0.01%	0.001%
66	9.481	2623	2625	2627	rBV2	293	175	0.01%	0.001%
67	9.731	2701	2703	2705	rBV	298	179	0.01%	0.001%
68	9.796	2721	2723	2726	rBV2	232	151	0.01%	0.001%
69	9.834	2733	2735	2740	rVB	242	128	0.01%	0.001%
70	9.866	2743	2745	2747	rBV	405	199	0.01%	0.001%
71	9.956	2771	2773	2776	rBV2	311	204	0.01%	0.001%
72	10.037	2795	2798	2800	rBV	263	177	0.01%	0.001%
73	10.149	2821	2833	2863	rBV	546712	855902	37.56%	5.894%
74	10.323	2879	2887	2896	rVB2	4323	6811	0.30%	0.047%
75	10.477	2932	2935	2936	rBV2	301	154	0.01%	0.001%
76	10.532	2949	2952	2953	rBV2	241	120	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035274.D
 Acq On : 18 Apr 2024 11:37
 Operator : SY/MD
 Sample : P2158-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.921	3070	3073	3076	rBV2	373	255	0.01%	0.002%
78	11.050	3110	3113	3114	rBV2	399	194	0.01%	0.001%
79	11.117	3123	3134	3145	rBV	218260	349101	15.32%	2.404%
80	11.204	3145	3161	3190	rVB2	967662	2278509	100.00%	15.690%
81	11.558	3260	3271	3298	rBV	765042	1269892	55.73%	8.745%
82	12.259	3484	3489	3490	rBV2	383	350	0.02%	0.002%
83	12.326	3508	3510	3512	rBV2	391	169	0.01%	0.001%
84	12.349	3512	3517	3521	rBV5	1435	1658	0.07%	0.011%
85	12.525	3562	3572	3584	rVB5	3619	8110	0.36%	0.056%
86	12.587	3584	3591	3600	rBV5	2258	3612	0.16%	0.025%
87	13.197	3770	3781	3803	rBV	174274	276863	12.15%	1.906%
88	13.452	3853	3860	3868	rBV2	4239	6996	0.31%	0.048%
89	13.680	3921	3931	3952	rBV	74308	121357	5.33%	0.836%

Sum of corrected areas: 14522124




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035274.D
Acq On : 18 Apr 2024 11:37
Operator : SY/MD
Sample : P2158-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

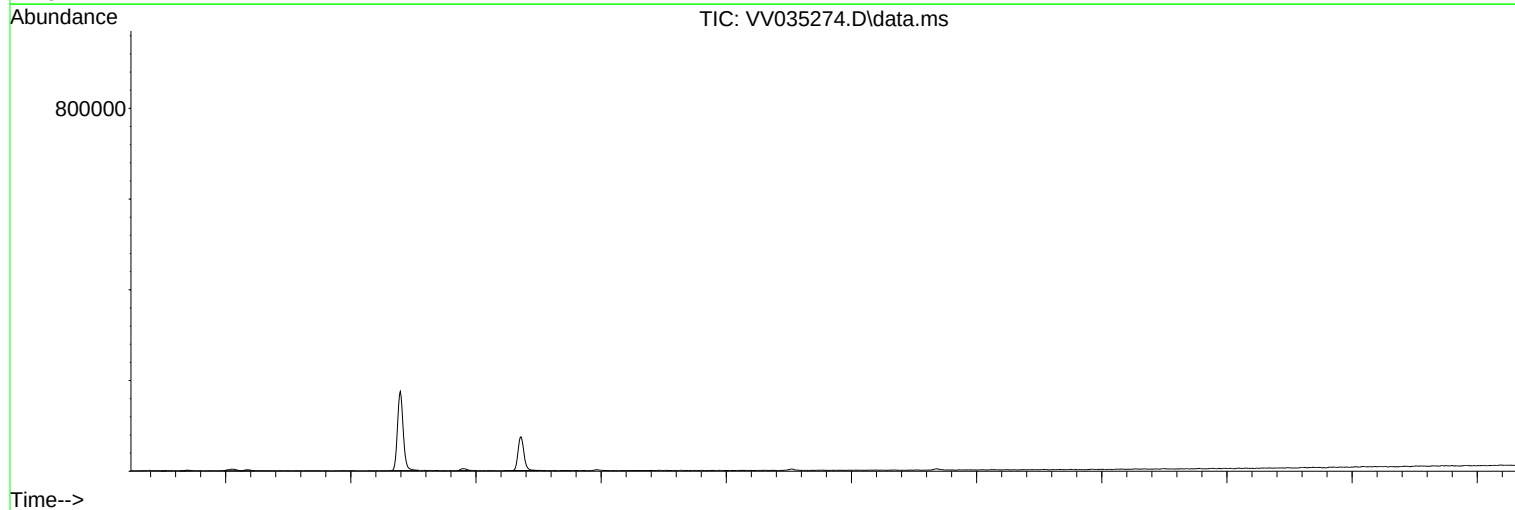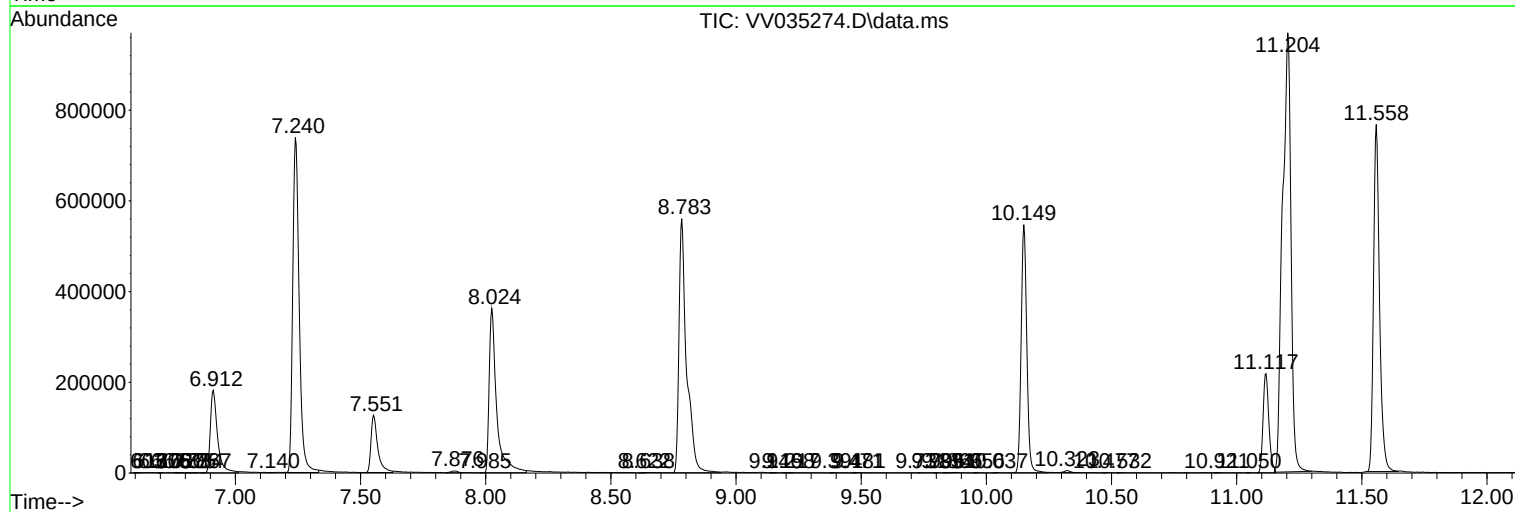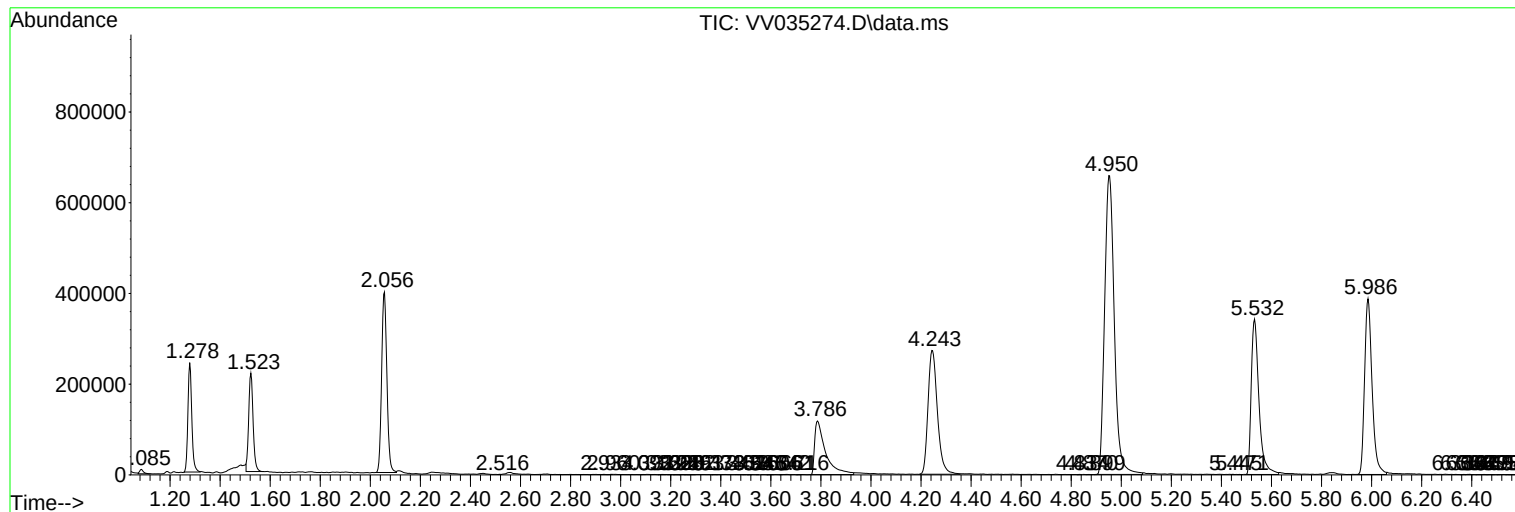

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035274.D
Acq On : 18 Apr 2024 11:37
Operator : SY/MD
Sample : P2158-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035274.D
Acq On : 18 Apr 2024 11:37
Operator : SY/MD
Sample : P2158-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
