

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035276.D
 Acq On : 18 Apr 2024 12:26
 Operator : SY/MD
 Sample : P2144-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	51	rBV2	11413	11225	0.67%	0.097%
2	1.278	67	74	92	rBV	227810	239839	14.42%	2.070%
3	1.523	145	150	166	rVB	221567	257150	15.46%	2.220%
4	2.056	307	316	329	rBV	374102	534182	32.11%	4.611%
5	2.748	528	531	533	rBV2	312	183	0.01%	0.002%
6	2.857	563	565	570	rVB	327	244	0.01%	0.002%
7	2.889	570	575	577	rBV4	683	627	0.04%	0.005%
8	2.937	587	590	591	rBV2	481	226	0.01%	0.002%
9	2.973	599	601	610	rVB3	521	438	0.03%	0.004%
10	3.011	610	613	614	rBV	396	160	0.01%	0.001%
11	3.034	618	620	621	rVV	331	132	0.01%	0.001%
12	3.060	625	628	631	rBV2	351	231	0.01%	0.002%
13	3.085	631	636	637	rVB	219	147	0.01%	0.001%
14	3.163	657	660	663	rBV	294	225	0.01%	0.002%
15	3.188	666	668	669	rBV	137	77	0.00%	0.001%
16	3.285	695	698	699	rBV	137	77	0.00%	0.001%
17	3.346	715	717	720	rBV2	272	136	0.01%	0.001%
18	3.362	720	722	724	rBV	131	80	0.00%	0.001%
19	3.375	724	726	727	rBV2	146	66	0.00%	0.001%
20	3.449	745	749	754	rVB2	390	272	0.02%	0.002%
21	3.474	754	757	761	rBV2	145	132	0.01%	0.001%
22	3.574	785	788	789	rBV2	308	175	0.01%	0.002%
23	3.674	816	819	821	rBV3	402	279	0.02%	0.002%
24	3.703	827	828	831	rBV2	229	95	0.01%	0.001%
25	3.748	838	842	846	rBV2	554	505	0.03%	0.004%
26	3.786	846	854	895	rBV2	112746	331573	19.93%	2.862%
27	4.246	982	997	1039	rBV	268119	750176	45.10%	6.476%
28	4.529	1082	1085	1086	rBV3	466	267	0.02%	0.002%
29	4.584	1100	1102	1106	rBV2	633	372	0.02%	0.003%
30	4.619	1110	1113	1114	rBV	542	276	0.02%	0.002%
31	4.738	1146	1150	1152	rBV2	301	225	0.01%	0.002%
32	4.799	1167	1169	1173	rBV3	358	199	0.01%	0.002%
33	4.847	1182	1184	1185	rBV	184	69	0.00%	0.001%
34	4.953	1201	1217	1248	rBV2	629797	1663523	100.00%	14.360%
35	5.490	1380	1384	1386	rBV2	365	318	0.02%	0.003%
36	5.532	1386	1397	1431	rBV	377219	789295	47.45%	6.813%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035276.D
 Acq On : 18 Apr 2024 12:26
 Operator : SY/MD
 Sample : P2144-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1522	1538	1566	rBV	365181	764746	45.97%	6.602%
38	6.278	1627	1629	1632	rBV3	420	269	0.02%	0.002%
39	6.317	1638	1641	1642	rVB2	352	152	0.01%	0.001%
40	6.394	1661	1665	1668	rBV3	381	353	0.02%	0.003%
41	6.442	1671	1680	1691	rVV3	7259	15504	0.93%	0.134%
42	6.542	1708	1711	1715	rVB4	706	429	0.03%	0.004%
43	6.577	1720	1722	1724	rVB	296	106	0.01%	0.001%
44	6.600	1724	1729	1730	rBV2	327	248	0.01%	0.002%
45	6.629	1736	1738	1741	rBV2	471	308	0.02%	0.003%
46	6.722	1765	1767	1768	rBV	313	99	0.01%	0.001%
47	6.780	1781	1785	1787	rBV	308	180	0.01%	0.002%
48	6.793	1787	1789	1792	rVB	234	84	0.01%	0.001%
49	6.809	1792	1794	1796	rBV	403	213	0.01%	0.002%
50	6.838	1801	1803	1806	rVV2	193	98	0.01%	0.001%
51	6.850	1806	1807	1810	rVV	167	67	0.00%	0.001%
52	6.912	1815	1826	1856	rBV	172013	336299	20.22%	2.903%
53	7.240	1917	1928	1973	rBV	700339	1255457	75.47%	10.837%
54	7.551	2016	2025	2057	rBV	118065	225725	13.57%	1.949%
55	7.873	2115	2125	2135	rBV3	2216	3651	0.22%	0.032%
56	7.915	2135	2138	2142	rBV3	655	489	0.03%	0.004%
57	7.950	2147	2149	2151	rBV2	194	93	0.01%	0.001%
58	8.024	2163	2172	2213	rBV	333754	705961	42.44%	6.094%
59	8.519	2325	2326	2328	rBV	344	129	0.01%	0.001%
60	8.545	2332	2334	2337	rVV2	401	220	0.01%	0.002%
61	8.674	2370	2374	2378	rBV4	485	452	0.03%	0.004%
62	8.728	2389	2391	2392	rBV	408	169	0.01%	0.001%
63	8.783	2397	2408	2437	rBV	580423	970059	58.31%	8.374%
64	9.217	2539	2543	2545	rBV2	765	512	0.03%	0.004%
65	9.243	2549	2551	2555	rBV3	461	309	0.02%	0.003%
66	9.291	2563	2566	2569	rVB	342	189	0.01%	0.002%
67	9.307	2569	2571	2574	rBV	454	280	0.02%	0.002%
68	9.490	2623	2628	2636	rBV4	592	740	0.04%	0.006%
69	9.677	2684	2686	2689	rBV	191	141	0.01%	0.001%
70	9.702	2692	2694	2695	rBV	238	49	0.00%	0.000%
71	9.715	2695	2698	2701	rVB	283	138	0.01%	0.001%
72	9.735	2701	2704	2705	rBV2	353	155	0.01%	0.001%
73	9.776	2715	2717	2721	rVB2	241	105	0.01%	0.001%
74	9.799	2721	2724	2727	rBV2	376	286	0.02%	0.002%
75	9.870	2744	2746	2747	rBV	499	179	0.01%	0.002%
76	9.908	2755	2758	2760	rBV	306	159	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035276.D
 Acq On : 18 Apr 2024 12:26
 Operator : SY/MD
 Sample : P2144-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.976	2776	2779	2782	rVB2	380	208	0.01%	0.002%
78	9.989	2782	2783	2784	rBV	213	61	0.00%	0.001%
79	10.059	2802	2805	2811	rBV2	255	301	0.02%	0.003%
80	10.149	2821	2833	2854	rBV	504548	802408	48.24%	6.927%
81	10.529	2948	2951	2952	rBV2	190	104	0.01%	0.001%
82	10.577	2964	2966	2968	rBV3	220	129	0.01%	0.001%
83	10.606	2973	2975	2979	rVB	220	103	0.01%	0.001%
84	10.657	2988	2991	2994	rBV	219	144	0.01%	0.001%
85	10.722	3003	3011	3017	rBV5	912	1403	0.08%	0.012%
86	10.757	3019	3022	3025	rBV	389	218	0.01%	0.002%
87	10.834	3042	3046	3049	rBV2	416	343	0.02%	0.003%
88	10.866	3054	3056	3057	rBV	534	214	0.01%	0.002%
89	10.921	3070	3073	3075	rBV3	322	240	0.01%	0.002%
90	11.043	3109	3111	3114	rBV	310	195	0.01%	0.002%
91	11.133	3129	3139	3143	rBV5	1472	1986	0.12%	0.017%
92	11.185	3144	3155	3189	rVV	528865	844185	50.75%	7.287%
93	11.558	3259	3271	3295	rBV	669822	1059767	63.71%	9.148%
94	12.439	3543	3545	3548	rBV	375	258	0.02%	0.002%
95	12.503	3563	3565	3567	rBV2	377	220	0.01%	0.002%
96	12.580	3586	3589	3590	rBV2	477	231	0.01%	0.002%
97	12.638	3603	3607	3610	rBV2	468	394	0.02%	0.003%
98	13.207	3779	3784	3791	rBV6	2519	3288	0.20%	0.028%

Sum of corrected areas: 11584398




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035276.D
Acq On : 18 Apr 2024 12:26
Operator : SY/MD
Sample : P2144-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07Z2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

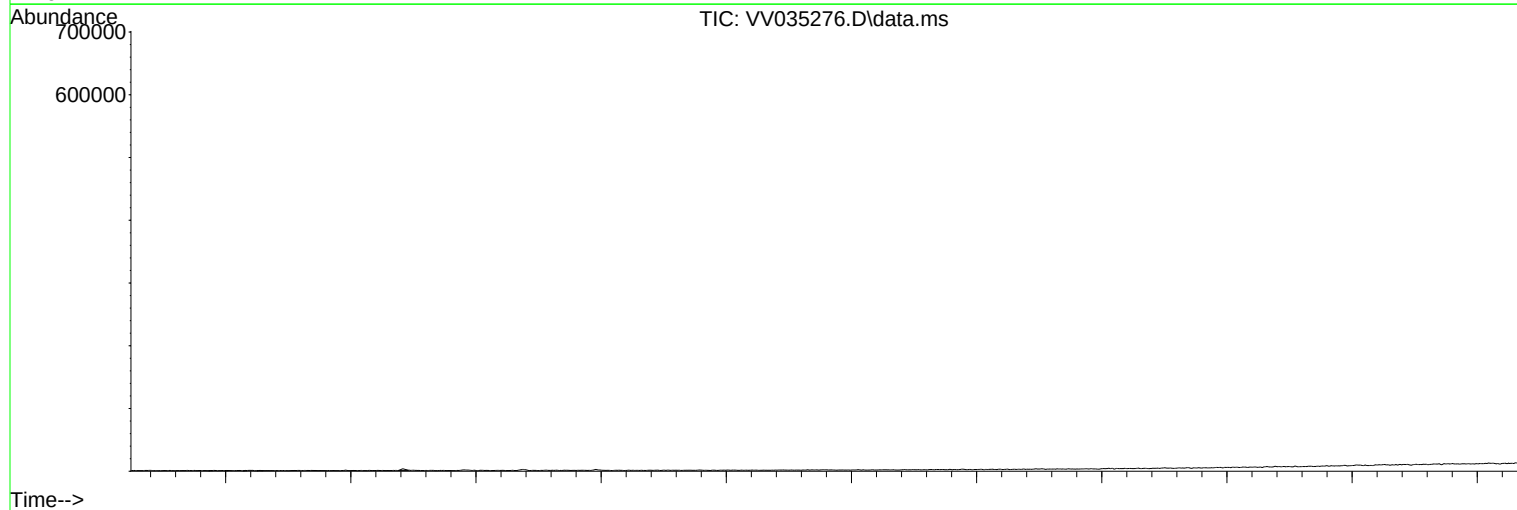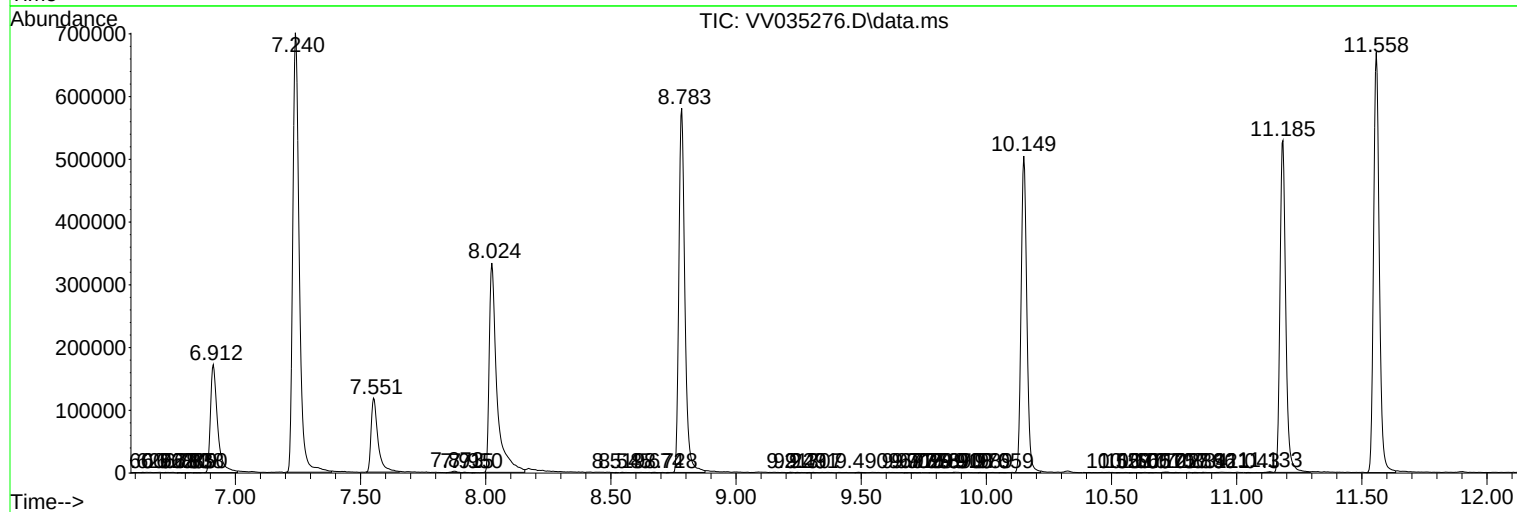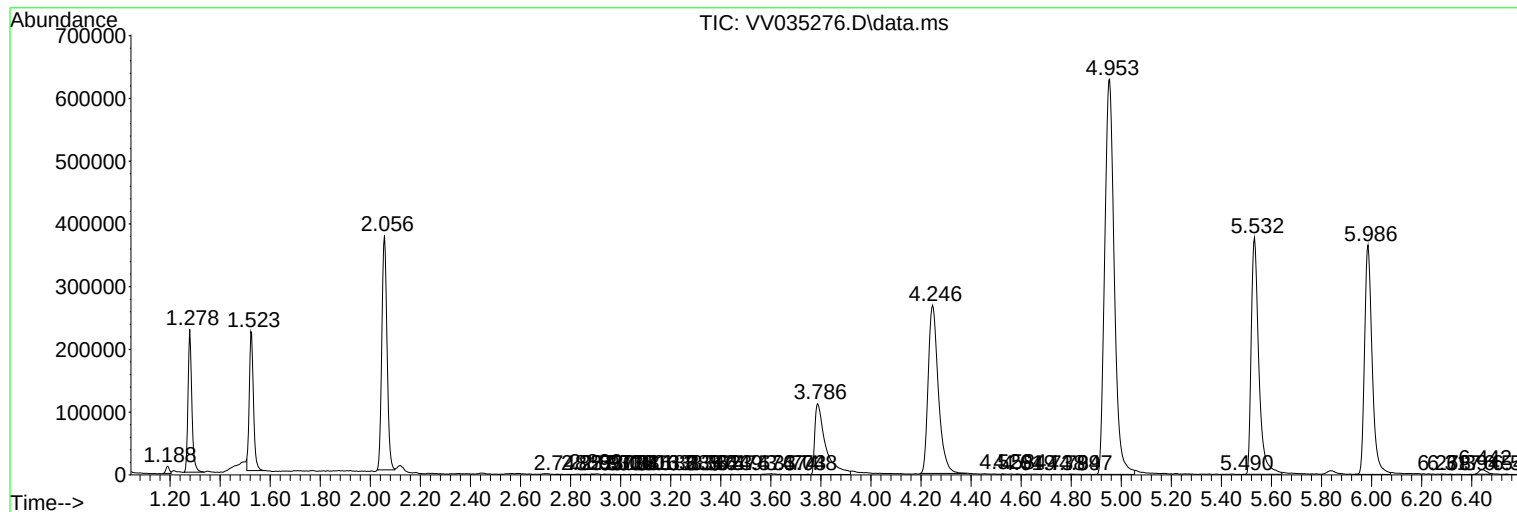

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035276.D
Acq On : 18 Apr 2024 12:26
Operator : SY/MD
Sample : P2144-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07Z2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035276.D
Acq On : 18 Apr 2024 12:26
Operator : SY/MD
Sample : P2144-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07Z2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------