

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035277.D
 Acq On : 18 Apr 2024 12:50
 Operator : SY/MD
 Sample : P2144-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	51	rBV2	10731	9699	0.59%	0.085%
2	1.278	67	74	89	rBV	218742	237501	14.51%	2.086%
3	1.523	144	150	171	rVB	192022	238897	14.59%	2.098%
4	2.056	306	316	328	rBV	368300	530221	32.39%	4.657%
5	2.696	510	515	517	rBV4	1244	1194	0.07%	0.010%
6	2.889	567	575	577	rBV4	777	1006	0.06%	0.009%
7	2.957	594	596	601	rVB3	469	213	0.01%	0.002%
8	3.073	630	632	633	rBV	296	104	0.01%	0.001%
9	3.111	641	644	647	rBV3	598	431	0.03%	0.004%
10	3.130	647	650	651	rBV	295	129	0.01%	0.001%
11	3.191	664	669	672	rVB3	238	232	0.01%	0.002%
12	3.230	677	681	683	rBV2	218	163	0.01%	0.001%
13	3.265	690	692	697	rVB3	288	209	0.01%	0.002%
14	3.298	698	702	706	rBV3	258	276	0.02%	0.002%
15	3.314	706	707	709	rVB2	362	94	0.01%	0.001%
16	3.327	709	711	714	rBV2	261	136	0.01%	0.001%
17	3.400	728	734	738	rVB3	309	297	0.02%	0.003%
18	3.471	753	756	760	rVB3	225	176	0.01%	0.002%
19	3.503	764	766	772	rVB	330	195	0.01%	0.002%
20	3.532	772	775	779	rBV2	237	193	0.01%	0.002%
21	3.558	781	783	786	rBV2	160	87	0.01%	0.001%
22	3.587	786	792	794	rBV2	643	569	0.03%	0.005%
23	3.671	815	818	821	rVB2	293	161	0.01%	0.001%
24	3.690	821	824	825	rBV2	241	131	0.01%	0.001%
25	3.741	837	840	843	rBV	333	214	0.01%	0.002%
26	3.786	844	854	895	rBV	107867	313968	19.18%	2.758%
27	4.246	982	997	1028	rBV	264471	726658	44.39%	6.383%
28	4.638	1117	1119	1120	rBV	275	101	0.01%	0.001%
29	4.696	1133	1137	1141	rBV3	318	233	0.01%	0.002%
30	4.828	1175	1178	1179	rBV	379	189	0.01%	0.002%
31	4.857	1185	1187	1189	rBV2	265	127	0.01%	0.001%
32	4.899	1198	1200	1201	rBV	328	150	0.01%	0.001%
33	4.953	1201	1217	1251	rBV2	620466	1636872	100.00%	14.378%
34	5.436	1364	1367	1370	rBV3	387	364	0.02%	0.003%
35	5.490	1381	1384	1386	rBV2	344	208	0.01%	0.002%
36	5.532	1386	1397	1434	rBV	372966	798231	48.77%	7.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035277.D
 Acq On : 18 Apr 2024 12:50
 Operator : SY/MD
 Sample : P2144-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.834	1482	1491	1492	rBV6	5618	7018	0.43%	0.062%
38	5.924	1517	1519	1522	rBV2	358	150	0.01%	0.001%
39	5.986	1524	1538	1573	rBV	366190	761471	46.52%	6.689%
40	6.217	1608	1610	1614	rBV3	461	224	0.01%	0.002%
41	6.249	1618	1620	1622	rBV2	371	209	0.01%	0.002%
42	6.355	1651	1653	1657	rVB2	519	332	0.02%	0.003%
43	6.442	1665	1680	1697	rBV2	6764	15995	0.98%	0.140%
44	6.526	1703	1706	1709	rBV3	215	150	0.01%	0.001%
45	6.568	1715	1719	1720	rBV2	228	162	0.01%	0.001%
46	6.577	1720	1722	1724	rBV2	188	104	0.01%	0.001%
47	6.606	1729	1731	1734	rBV2	310	211	0.01%	0.002%
48	6.635	1739	1740	1741	rBV2	341	80	0.00%	0.001%
49	6.645	1741	1743	1745	rBV2	300	160	0.01%	0.001%
50	6.654	1745	1746	1747	rBV	321	68	0.00%	0.001%
51	6.725	1765	1768	1770	rBV2	357	256	0.02%	0.002%
52	6.799	1788	1791	1795	rBV	219	139	0.01%	0.001%
53	6.844	1802	1805	1808	rBV2	331	258	0.02%	0.002%
54	6.912	1814	1826	1852	rBV	170797	333480	20.37%	2.929%
55	7.240	1917	1928	1955	rBV	679155	1222254	74.67%	10.736%
56	7.551	2016	2025	2055	rBV	116661	221808	13.55%	1.948%
57	7.809	2103	2105	2107	rBV	408	249	0.02%	0.002%
58	7.876	2117	2126	2141	rVB3	4466	7983	0.49%	0.070%
59	7.944	2144	2147	2149	rBV2	257	126	0.01%	0.001%
60	7.989	2158	2161	2163	rBV2	488	235	0.01%	0.002%
61	8.024	2163	2172	2213	rBV	319313	675107	41.24%	5.930%
62	8.465	2306	2309	2310	rBV	522	262	0.02%	0.002%
63	8.606	2350	2353	2357	rBV4	434	327	0.02%	0.003%
64	8.635	2360	2362	2364	rBV	329	160	0.01%	0.001%
65	8.690	2377	2379	2382	rVB	499	268	0.02%	0.002%
66	8.731	2390	2392	2396	rBV3	374	303	0.02%	0.003%
67	8.783	2396	2408	2437	rBV	583594	969782	59.25%	8.518%
68	9.030	2483	2485	2487	rBV2	454	189	0.01%	0.002%
69	9.075	2495	2499	2500	rBV3	406	299	0.02%	0.003%
70	9.156	2522	2524	2526	rVB3	323	127	0.01%	0.001%
71	9.198	2535	2537	2540	rBV2	401	244	0.01%	0.002%
72	9.256	2552	2555	2558	rBV2	465	432	0.03%	0.004%
73	9.320	2572	2575	2579	rVB2	314	261	0.02%	0.002%
74	9.365	2587	2589	2590	rBV2	193	74	0.00%	0.001%
75	9.413	2602	2604	2606	rBV2	268	133	0.01%	0.001%
76	9.484	2620	2626	2627	rBV2	536	409	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035277.D
 Acq On : 18 Apr 2024 12:50
 Operator : SY/MD
 Sample : P2144-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E07Z4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.542	2642	2644	2645	rBV2	370	122	0.01%	0.001%
78	9.596	2658	2661	2667	rBV3	331	350	0.02%	0.003%
79	9.632	2667	2672	2676	rVB3	516	462	0.03%	0.004%
80	9.654	2677	2679	2680	rBV3	194	73	0.00%	0.001%
81	9.722	2697	2700	2704	rBV2	270	188	0.01%	0.002%
82	9.770	2713	2715	2718	rBV3	370	217	0.01%	0.002%
83	9.854	2739	2741	2743	rBV	334	179	0.01%	0.002%
84	9.911	2757	2759	2765	rVB2	514	297	0.02%	0.003%
85	9.995	2782	2785	2787	rBV	245	165	0.01%	0.001%
86	10.069	2805	2808	2809	rBV	305	161	0.01%	0.001%
87	10.149	2821	2833	2863	rBV	499263	793745	48.49%	6.972%
88	10.378	2902	2904	2911	rBV2	793	637	0.04%	0.006%
89	10.477	2932	2935	2937	rBV2	336	213	0.01%	0.002%
90	10.542	2954	2955	2958	rBV2	334	236	0.01%	0.002%
91	10.783	3028	3030	3035	rBV3	539	458	0.03%	0.004%
92	10.927	3073	3075	3077	rBV2	290	151	0.01%	0.001%
93	11.130	3133	3138	3140	rBV4	632	654	0.04%	0.006%
94	11.182	3144	3154	3183	rBV	513601	828684	50.63%	7.279%
95	11.558	3258	3271	3294	rBV	649020	1033499	63.14%	9.078%
96	11.892	3370	3375	3380	rBV4	1292	1723	0.11%	0.015%
97	12.153	3453	3456	3460	rVB4	607	522	0.03%	0.005%
98	12.175	3460	3463	3464	rBV2	460	282	0.02%	0.002%
99	12.718	3630	3632	3635	rBV	332	172	0.01%	0.002%
100	12.734	3635	3637	3638	rBV	364	178	0.01%	0.002%

Sum of corrected areas: 11384496




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035277.D
Acq On : 18 Apr 2024 12:50
Operator : SY/MD
Sample : P2144-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07Z4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

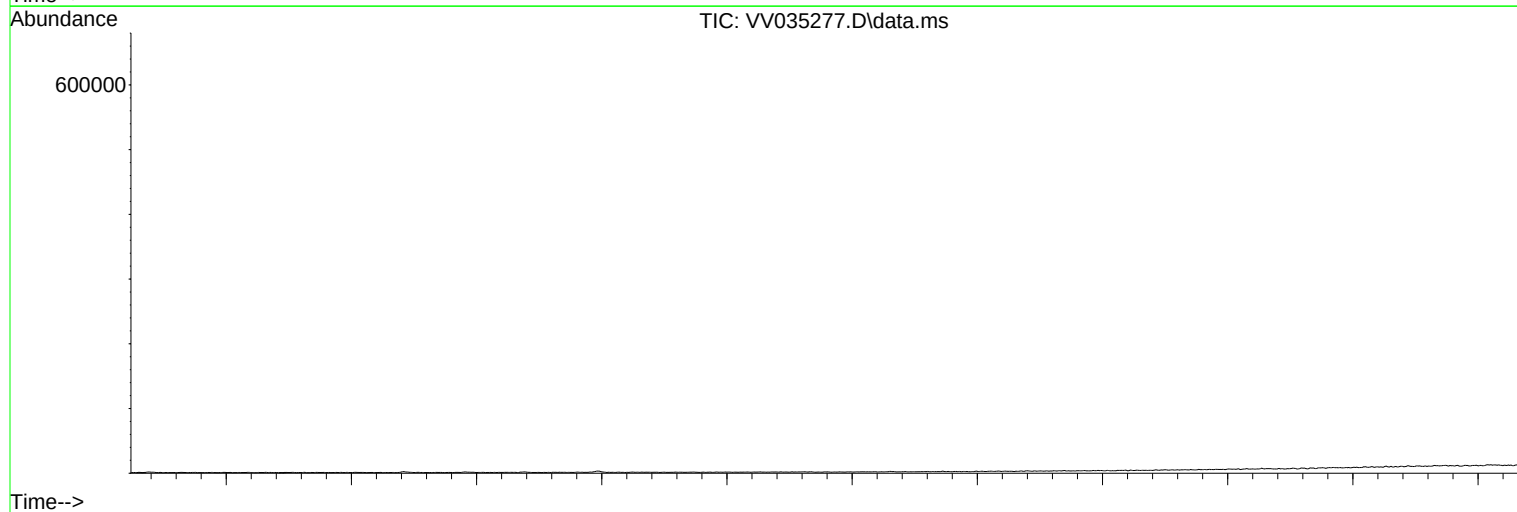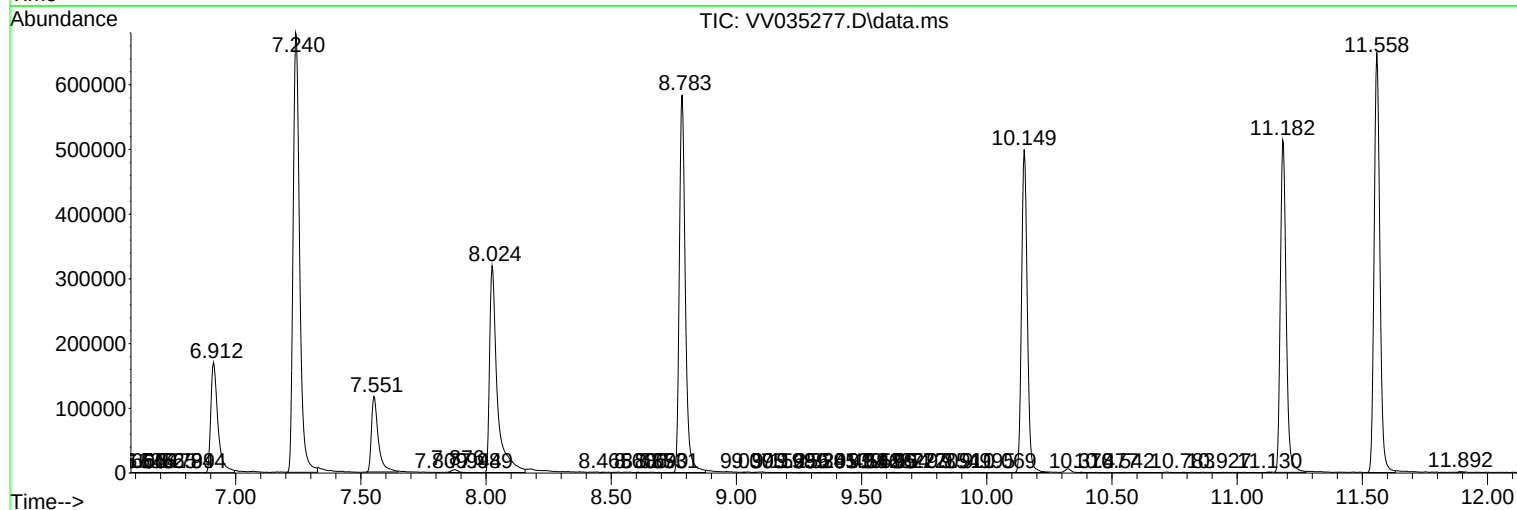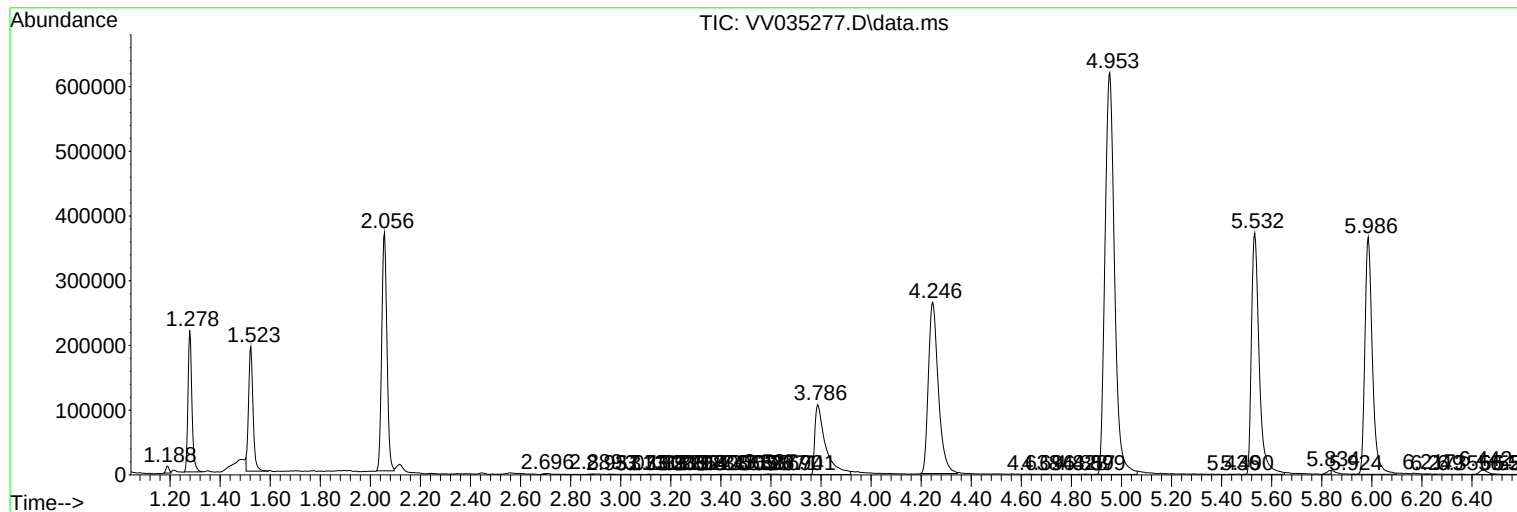

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035277.D
Acq On : 18 Apr 2024 12:50
Operator : SY/MD
Sample : P2144-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07Z4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035277.D
Acq On : 18 Apr 2024 12:50
Operator : SY/MD
Sample : P2144-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E07Z4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------