

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035278.D
 Acq On : 18 Apr 2024 13:14
 Operator : SY/MD
 Sample : P2144-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	221491	238080	14.45%	2.082%
2	1.523	145	150	169	rVB	218421	257276	15.62%	2.250%
3	2.056	307	316	330	rBV	364063	524466	31.83%	4.586%
4	2.240	368	373	382	rBV	14020	12894	0.78%	0.113%
5	2.442	429	436	447	rVB3	4217	7144	0.43%	0.062%
6	2.700	512	516	517	rBV2	790	536	0.03%	0.005%
7	2.761	530	535	538	rBV	248	191	0.01%	0.002%
8	2.777	538	540	543	rVB	364	151	0.01%	0.001%
9	2.934	586	589	590	rBV	394	176	0.01%	0.002%
10	3.079	632	634	635	rBV	176	56	0.00%	0.000%
11	3.217	675	677	682	rVB2	338	191	0.01%	0.002%
12	3.240	682	684	685	rBV2	139	66	0.00%	0.001%
13	3.278	690	696	698	rBV3	359	418	0.03%	0.004%
14	3.304	702	704	709	rVB3	377	162	0.01%	0.001%
15	3.365	721	723	725	rBV2	230	149	0.01%	0.001%
16	3.458	748	752	756	rBV3	331	303	0.02%	0.003%
17	3.487	759	761	764	rBV3	301	203	0.01%	0.002%
18	3.535	775	776	778	rVB	140	31	0.00%	0.000%
19	3.552	778	781	786	rVB3	263	257	0.02%	0.002%
20	3.577	786	789	794	rBV2	264	173	0.01%	0.002%
21	3.606	794	798	801	rBV2	261	235	0.01%	0.002%
22	3.626	801	804	805	rBV	207	92	0.01%	0.001%
23	3.658	811	814	816	rBV	75	56	0.00%	0.000%
24	3.671	816	818	820	rBV2	247	126	0.01%	0.001%
25	3.716	829	832	836	rBV	120	98	0.01%	0.001%
26	3.738	836	839	841	rVB2	172	97	0.01%	0.001%
27	3.757	841	845	846	rBV3	285	180	0.01%	0.002%
28	3.789	846	855	886	rBV	112551	318668	19.34%	2.786%
29	4.246	982	997	1035	rBV	256546	660584	40.10%	5.776%
30	4.670	1126	1129	1135	rVB2	564	455	0.03%	0.004%
31	4.716	1139	1143	1146	rBV3	365	307	0.02%	0.003%
32	4.735	1147	1149	1152	rBV3	357	214	0.01%	0.002%
33	4.754	1152	1155	1165	rVB4	605	660	0.04%	0.006%
34	4.799	1165	1169	1170	rBV	341	211	0.01%	0.002%
35	4.883	1193	1195	1198	rBV2	228	111	0.01%	0.001%
36	4.953	1201	1217	1253	rBV2	624276	1647499	100.00%	14.405%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035278.D
 Acq On : 18 Apr 2024 13:14
 Operator : SY/MD
 Sample : P2144-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.449	1369	1371	1374	rBV2	177	117	0.01%	0.001%
38	5.465	1374	1376	1378	rBV2	251	127	0.01%	0.001%
39	5.532	1386	1397	1441	rBV	385434	822954	49.95%	7.196%
40	5.838	1483	1492	1505	rBV4	4878	10270	0.62%	0.090%
41	5.941	1518	1524	1525	rBV	577	466	0.03%	0.004%
42	5.986	1525	1538	1567	rVV	363111	755095	45.83%	6.602%
43	6.265	1623	1625	1627	rBV	191	67	0.00%	0.001%
44	6.301	1632	1636	1638	rBV3	543	299	0.02%	0.003%
45	6.394	1664	1665	1666	rVB3	259	50	0.00%	0.000%
46	6.426	1672	1675	1679	rBV	629	429	0.03%	0.004%
47	6.449	1679	1682	1683	rBV2	404	208	0.01%	0.002%
48	6.490	1691	1695	1699	rBV	386	332	0.02%	0.003%
49	6.593	1725	1727	1729	rVB	373	117	0.01%	0.001%
50	6.609	1729	1732	1733	rBV	208	120	0.01%	0.001%
51	6.616	1733	1734	1737	rVB	375	181	0.01%	0.002%
52	6.638	1737	1741	1745	rBV3	502	443	0.03%	0.004%
53	6.751	1771	1776	1779	rBV4	401	356	0.02%	0.003%
54	6.809	1790	1794	1795	rBV	192	150	0.01%	0.001%
55	6.831	1799	1801	1803	rVB	348	101	0.01%	0.001%
56	6.867	1810	1812	1816	rBV2	401	337	0.02%	0.003%
57	6.912	1816	1826	1852	rBV	168026	325864	19.78%	2.849%
58	7.240	1918	1928	1964	rBV	677628	1222208	74.19%	10.687%
59	7.551	2016	2025	2058	rBV	116198	223252	13.55%	1.952%
60	7.908	2134	2136	2141	rVB4	752	478	0.03%	0.004%
61	7.969	2153	2155	2158	rBV3	407	222	0.01%	0.002%
62	8.024	2163	2172	2216	rBV	343559	716947	43.52%	6.269%
63	8.558	2335	2338	2340	rBV2	413	241	0.01%	0.002%
64	8.638	2362	2363	2366	rBV3	494	144	0.01%	0.001%
65	8.783	2397	2408	2437	rBV	594445	1001335	60.78%	8.755%
66	9.140	2517	2519	2521	rBV	211	118	0.01%	0.001%
67	9.288	2563	2565	2567	rBV	213	114	0.01%	0.001%
68	9.407	2596	2602	2606	rBV2	262	270	0.02%	0.002%
69	9.764	2710	2713	2715	rBV	344	203	0.01%	0.002%
70	9.821	2728	2731	2735	rBV2	254	227	0.01%	0.002%
71	9.873	2744	2747	2749	rBV	446	282	0.02%	0.002%
72	10.008	2784	2789	2792	rBV3	462	383	0.02%	0.003%
73	10.149	2821	2833	2857	rBV	506631	809009	49.11%	7.074%
74	10.320	2880	2886	2887	rBV2	781	677	0.04%	0.006%
75	10.416	2914	2916	2919	rBV3	355	240	0.01%	0.002%
76	10.567	2961	2963	2966	rBV2	211	143	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035278.D
 Acq On : 18 Apr 2024 13:14
 Operator : SY/MD
 Sample : P2144-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.718	3006	3010	3014	rVB3	538	458	0.03%	0.004%
78	10.741	3014	3017	3021	rBV2	271	242	0.01%	0.002%
79	10.760	3021	3023	3027	rVB2	314	150	0.01%	0.001%
80	10.792	3027	3033	3037	rBV2	569	588	0.04%	0.005%
81	11.021	3098	3104	3106	rBV2	221	230	0.01%	0.002%
82	11.111	3130	3132	3135	rVB2	393	209	0.01%	0.002%
83	11.130	3135	3138	3143	rBV2	1043	841	0.05%	0.007%
84	11.181	3143	3154	3177	rBV	526728	840372	51.01%	7.348%
85	11.503	3250	3254	3257	rBV3	577	483	0.03%	0.004%
86	11.558	3260	3271	3295	rBV	656741	1026090	62.28%	8.972%
87	12.982	3712	3714	3715	rBV	427	138	0.01%	0.001%

Sum of corrected areas: 11436893




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035278.D
Acq On : 18 Apr 2024 13:14
Operator : SY/MD
Sample : P2144-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

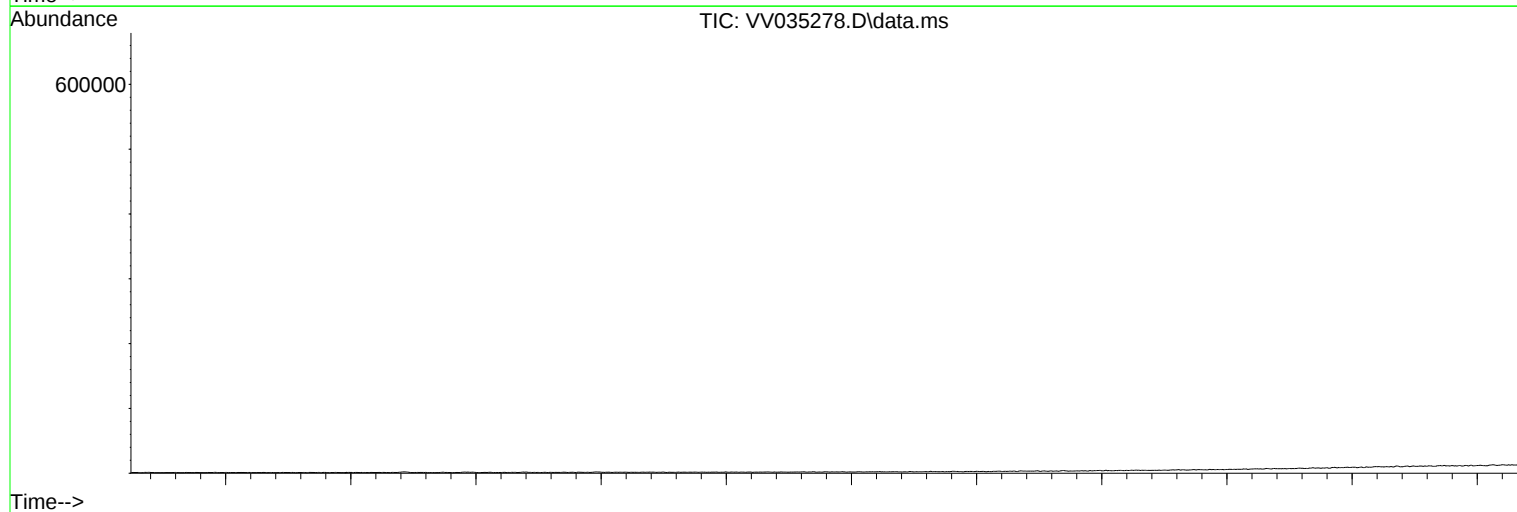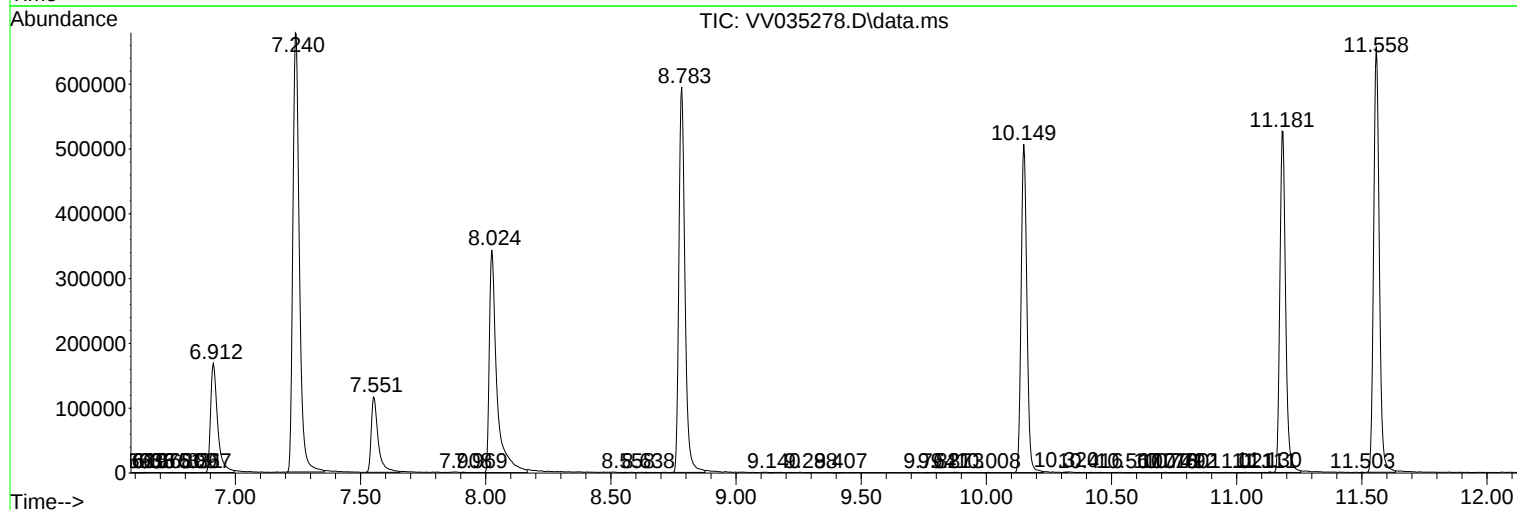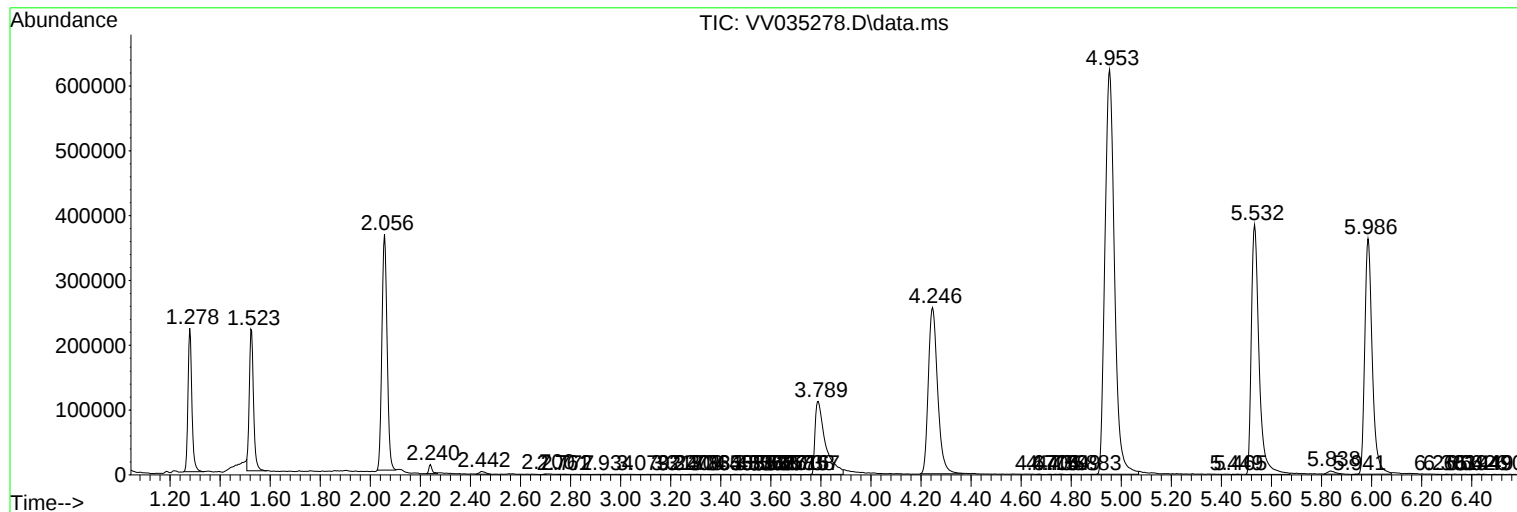

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035278.D
Acq On : 18 Apr 2024 13:14
Operator : SY/MD
Sample : P2144-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035278.D
Acq On : 18 Apr 2024 13:14
Operator : SY/MD
Sample : P2144-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------