

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035279.D
 Acq On : 18 Apr 2024 13:38
 Operator : SY/MD
 Sample : P2158-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	227968	245211	14.47%	2.104%
2	1.526	145	151	164	rVB	193581	234622	13.84%	2.013%
3	2.056	307	316	332	rBV	380387	544566	32.13%	4.672%
4	2.828	554	556	558	rBV2	292	135	0.01%	0.001%
5	2.989	602	606	607	rBV	345	235	0.01%	0.002%
6	3.066	627	630	632	rBV	300	213	0.01%	0.002%
7	3.092	637	638	641	rBV	195	84	0.00%	0.001%
8	3.153	655	657	659	rVB2	227	62	0.00%	0.001%
9	3.166	659	661	662	rBV	207	109	0.01%	0.001%
10	3.333	709	713	714	rBV	171	139	0.01%	0.001%
11	3.375	723	726	728	rBV2	273	185	0.01%	0.002%
12	3.455	747	751	754	rBV	298	199	0.01%	0.002%
13	3.516	767	770	771	rBV2	97	62	0.00%	0.001%
14	3.526	771	773	775	rVB	312	115	0.01%	0.001%
15	3.539	775	777	778	rBV	128	57	0.00%	0.000%
16	3.558	780	783	787	rBV2	157	110	0.01%	0.001%
17	3.580	787	790	793	rVB2	163	91	0.01%	0.001%
18	3.600	793	796	798	rBV2	207	145	0.01%	0.001%
19	3.625	802	804	807	rBV	169	75	0.00%	0.001%
20	3.641	807	809	811	rVB	147	47	0.00%	0.000%
21	3.661	811	815	816	rBV	180	120	0.01%	0.001%
22	3.706	824	829	831	rBV2	144	111	0.01%	0.001%
23	3.738	836	839	844	rVB3	324	314	0.02%	0.003%
24	3.786	845	854	899	rBV	115817	351924	20.76%	3.019%
25	4.246	981	997	1027	rBV	266994	688576	40.63%	5.908%
26	4.741	1142	1151	1152	rBV3	760	1034	0.06%	0.009%
27	4.953	1201	1217	1256	rBV2	643760	1694931	100.00%	14.542%
28	5.387	1349	1352	1357	rBV4	512	425	0.03%	0.004%
29	5.442	1367	1369	1372	rBV3	401	241	0.01%	0.002%
30	5.477	1378	1380	1384	rVB2	313	179	0.01%	0.002%
31	5.532	1386	1397	1428	rBV	389589	817837	48.25%	7.017%
32	5.918	1515	1517	1518	rBV	223	90	0.01%	0.001%
33	5.985	1525	1538	1573	rBV	375885	779479	45.99%	6.688%
34	6.345	1647	1650	1655	rVB4	544	472	0.03%	0.004%
35	6.378	1656	1660	1663	rBV3	405	264	0.02%	0.002%
36	6.436	1676	1678	1679	rBV3	198	76	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035279.D
 Acq On : 18 Apr 2024 13:38
 Operator : SY/MD
 Sample : P2158-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.461	1682	1686	1692	rVB5	596	633	0.04%	0.005%
38	6.603	1728	1730	1732	rBV	297	126	0.01%	0.001%
39	6.632	1737	1739	1741	rBV	210	119	0.01%	0.001%
40	6.760	1776	1779	1780	rBV	178	114	0.01%	0.001%
41	6.770	1780	1782	1784	rBV3	344	174	0.01%	0.001%
42	6.805	1792	1793	1795	rBV3	210	66	0.00%	0.001%
43	6.818	1795	1797	1800	rVB	331	157	0.01%	0.001%
44	6.831	1800	1801	1802	rBV	242	83	0.00%	0.001%
45	6.911	1815	1826	1852	rBV	174187	337390	19.91%	2.895%
46	7.239	1918	1928	1957	rBV	706636	1262285	74.47%	10.830%
47	7.551	2016	2025	2054	rBV	119782	226701	13.38%	1.945%
48	7.915	2130	2138	2146	rVB6	2661	4455	0.26%	0.038%
49	7.947	2146	2148	2154	rVB4	379	220	0.01%	0.002%
50	8.024	2163	2172	2214	rBV	347206	718636	42.40%	6.166%
51	8.516	2321	2325	2327	rBV3	743	509	0.03%	0.004%
52	8.783	2396	2408	2439	rBV	596230	999024	58.94%	8.571%
53	9.059	2492	2494	2498	rVB3	688	389	0.02%	0.003%
54	9.210	2540	2541	2542	rBV3	279	102	0.01%	0.001%
55	9.271	2559	2560	2563	rBV2	135	79	0.00%	0.001%
56	9.365	2587	2589	2593	rVB3	325	225	0.01%	0.002%
57	9.387	2594	2596	2597	rBV	153	44	0.00%	0.000%
58	9.416	2602	2605	2607	rBV2	325	274	0.02%	0.002%
59	9.474	2621	2623	2624	rBV2	222	94	0.01%	0.001%
60	9.538	2641	2643	2646	rBV	204	111	0.01%	0.001%
61	9.606	2662	2664	2665	rBV	387	166	0.01%	0.001%
62	9.750	2704	2709	2712	rBV4	451	382	0.02%	0.003%
63	9.770	2713	2715	2717	rVB	302	104	0.01%	0.001%
64	9.802	2722	2725	2726	rBV2	305	147	0.01%	0.001%
65	9.869	2744	2746	2749	rVB3	444	201	0.01%	0.002%
66	9.882	2749	2750	2753	rVB3	326	131	0.01%	0.001%
67	9.943	2765	2769	2776	rBV2	316	281	0.02%	0.002%
68	9.972	2776	2778	2779	rBV	372	136	0.01%	0.001%
69	10.149	2822	2833	2855	rBV	524611	828817	48.90%	7.111%
70	10.522	2947	2949	2951	rBV	399	233	0.01%	0.002%
71	10.840	3044	3048	3050	rBV	325	220	0.01%	0.002%
72	10.931	3074	3076	3079	rVB2	284	109	0.01%	0.001%
73	11.123	3132	3136	3139	rBV2	977	963	0.06%	0.008%
74	11.185	3144	3155	3181	rBV	533147	844378	49.82%	7.245%
75	11.451	3235	3238	3240	rBV2	449	304	0.02%	0.003%
76	11.558	3260	3271	3300	rBV	663406	1060215	62.55%	9.096%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035279.D
Acq On : 18 Apr 2024 13:38
Operator : SY/MD
Sample : P2158-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

77	12.133	3446	3450	3453	rBV3	421	357	0.02%	0.003%
78	12.435	3541	3544	3546	rBV2	415	260	0.02%	0.002%
79	12.914	3691	3693	3695	rBV	313	180	0.01%	0.002%
80	13.210	3777	3785	3793	rBV8	2003	2946	0.17%	0.025%
81	13.628	3913	3915	3918	rBV2	408	197	0.01%	0.002%
82	13.911	4001	4003	4004	rBV2	379	135	0.01%	0.001%

Sum of corrected areas: 11655407




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035279.D
Acq On : 18 Apr 2024 13:38
Operator : SY/MD
Sample : P2158-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

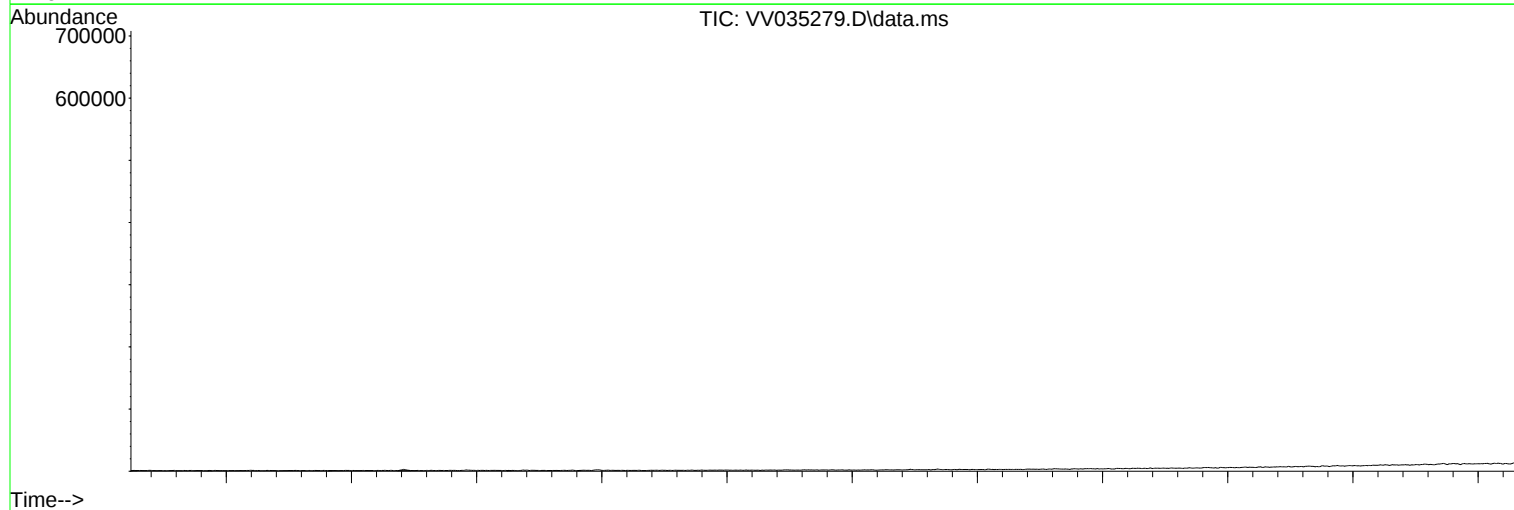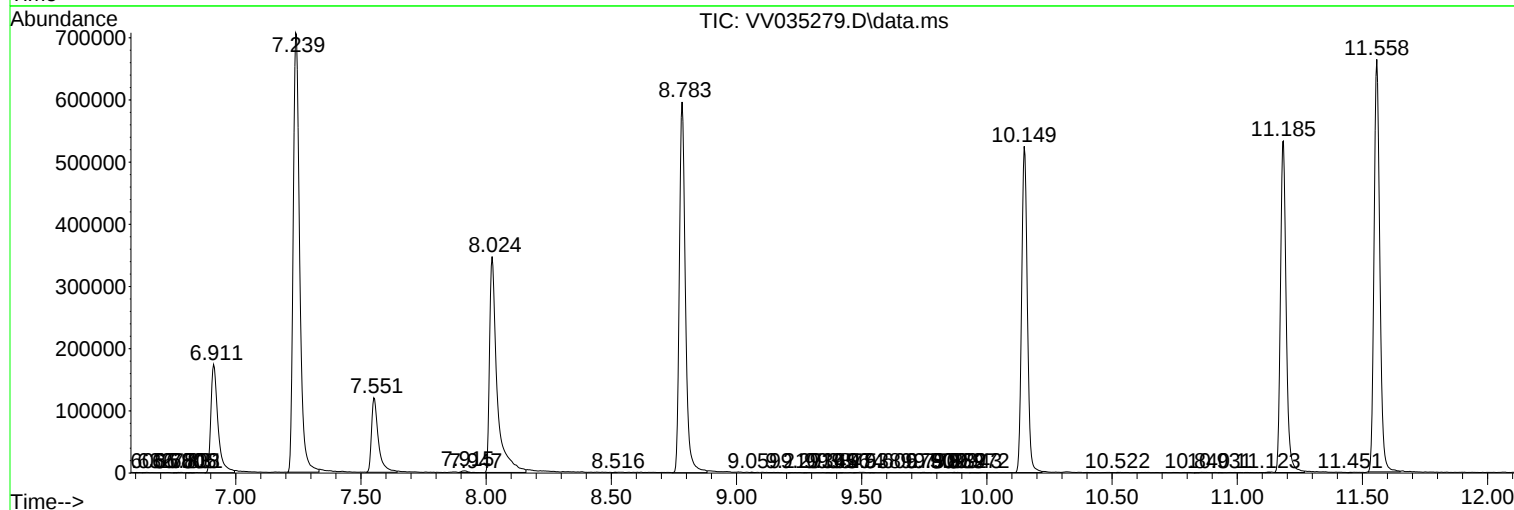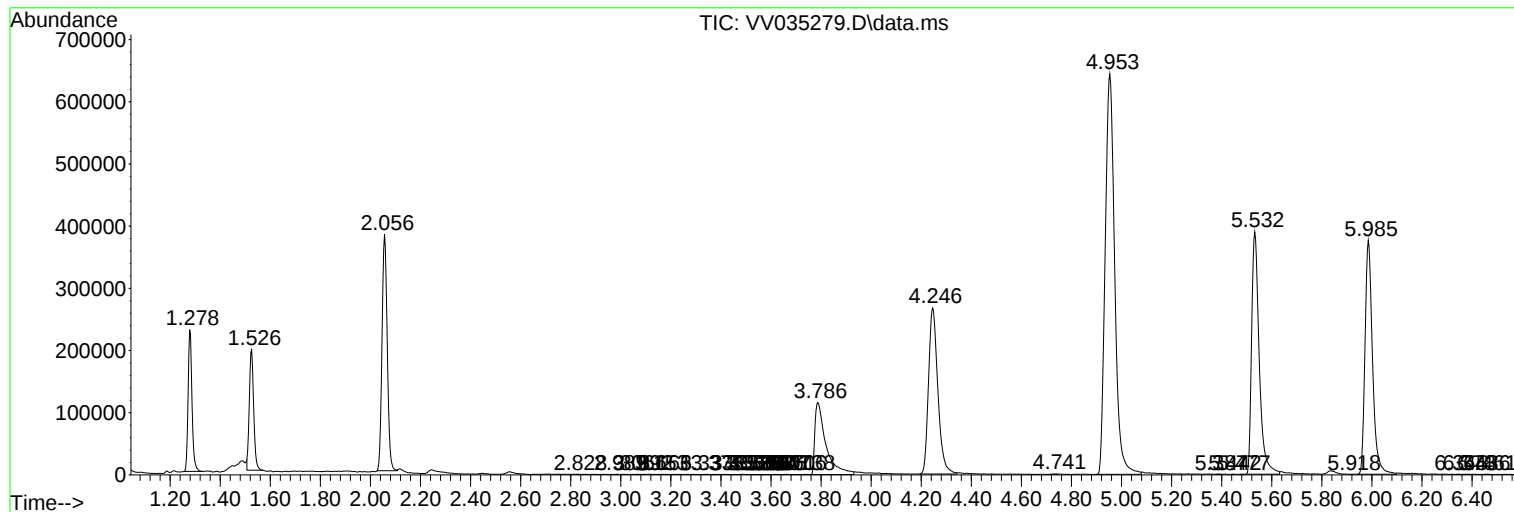

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035279.D
Acq On : 18 Apr 2024 13:38
Operator : SY/MD
Sample : P2158-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035279.D
Acq On : 18 Apr 2024 13:38
Operator : SY/MD
Sample : P2158-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------