

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035281.D
 Acq On : 18 Apr 2024 14:26
 Operator : SY/MD
 Sample : P2158-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	49	rBV2	3467	3397	0.04%	0.012%
2	1.214	50	54	60	rBV4	3515	4921	0.06%	0.017%
3	1.278	67	74	92	rBV	236150	253700	3.23%	0.862%
4	1.526	144	151	167	rVB	198125	247135	3.15%	0.839%
5	2.056	306	316	329	rBV	373009	542880	6.92%	1.844%
6	2.243	367	374	375	rBV6	2894	3126	0.04%	0.011%
7	2.449	430	438	450	rVB7	2831	4946	0.06%	0.017%
8	2.558	461	472	485	rBV3	3554	8494	0.11%	0.029%
9	2.632	493	495	498	rBV	366	274	0.00%	0.001%
10	2.706	513	518	521	rVV4	727	729	0.01%	0.002%
11	3.053	622	626	629	rBV3	337	300	0.00%	0.001%
12	3.121	634	647	651	rBV3	1431	2417	0.03%	0.008%
13	3.156	654	658	661	rVB4	583	511	0.01%	0.002%
14	3.220	674	678	683	rVB3	404	420	0.01%	0.001%
15	3.285	691	698	702	rBV4	455	504	0.01%	0.002%
16	3.661	807	815	818	rBV5	952	1322	0.02%	0.004%
17	3.786	846	854	896	rBV	113437	338418	4.31%	1.150%
18	4.246	981	997	1030	rBV	250644	658094	8.39%	2.235%
19	4.481	1064	1070	1072	rBV5	656	548	0.01%	0.002%
20	4.519	1078	1082	1084	rBV2	514	344	0.00%	0.001%
21	4.580	1097	1101	1106	rBV5	688	644	0.01%	0.002%
22	4.728	1141	1147	1151	rBV5	2311	3019	0.04%	0.010%
23	4.953	1201	1217	1224	rBV2	641178	1541150	19.65%	5.235%
24	5.005	1225	1233	1273	rVB	1623777	3598322	45.88%	12.223%
25	5.532	1386	1397	1431	rBV	408126	855210	10.90%	2.905%
26	5.834	1482	1491	1492	rBV4	3438	3639	0.05%	0.012%
27	5.928	1514	1520	1523	rBV4	391	356	0.00%	0.001%
28	5.985	1524	1538	1569	rBV	358699	751465	9.58%	2.553%
29	6.265	1623	1625	1627	rBV	439	277	0.00%	0.001%
30	6.281	1627	1630	1632	rVV4	467	335	0.00%	0.001%
31	6.375	1658	1659	1665	rVB3	598	310	0.00%	0.001%
32	6.403	1665	1668	1672	rBV4	427	305	0.00%	0.001%
33	6.465	1682	1687	1691	rBV5	399	362	0.00%	0.001%
34	6.606	1726	1731	1733	rBV3	383	344	0.00%	0.001%
35	6.632	1733	1739	1741	rBV4	348	335	0.00%	0.001%
36	6.664	1746	1749	1756	rVB5	1048	896	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035281.D
 Acq On : 18 Apr 2024 14:26
 Operator : SY/MD
 Sample : P2158-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.702	1756	1761	1763	rBV2	422	338	0.00%	0.001%
38	6.728	1767	1769	1772	rVB3	501	270	0.00%	0.001%
39	6.911	1812	1826	1862	rBV	169848	338797	4.32%	1.151%
40	7.239	1917	1928	1969	rBV	687237	1238114	15.79%	4.206%
41	7.555	2015	2026	2054	rBV	115128	226418	2.89%	0.769%
42	7.789	2096	2099	2100	rBV2	561	298	0.00%	0.001%
43	7.866	2118	2123	2131	rBV4	823	1128	0.01%	0.004%
44	7.905	2131	2135	2136	rBV3	1267	636	0.01%	0.002%
45	7.973	2154	2156	2160	rVB4	563	337	0.00%	0.001%
46	8.024	2160	2172	2217	rBV	347195	702982	8.96%	2.388%
47	8.458	2305	2307	2310	rBV3	425	290	0.00%	0.001%
48	8.526	2324	2328	2330	rBV4	417	371	0.00%	0.001%
49	8.577	2342	2344	2348	rVV3	400	296	0.00%	0.001%
50	8.809	2395	2416	2467	rBV2	4238967	7843451	100.00%	26.642%
51	9.172	2526	2529	2531	rBV3	387	267	0.00%	0.001%
52	9.188	2531	2534	2537	rBV3	649	606	0.01%	0.002%
53	9.657	2676	2680	2683	rBV3	719	521	0.01%	0.002%
54	9.677	2683	2686	2690	rVV3	335	327	0.00%	0.001%
55	9.886	2748	2751	2756	rVB3	670	589	0.01%	0.002%
56	9.915	2756	2760	2765	rVB6	344	311	0.00%	0.001%
57	10.008	2783	2789	2791	rVB2	484	382	0.00%	0.001%
58	10.062	2802	2806	2807	rBV	454	292	0.00%	0.001%
59	10.149	2821	2833	2861	rBV	516793	804158	10.25%	2.732%
60	10.291	2874	2877	2879	rBV	487	274	0.00%	0.001%
61	10.313	2879	2884	2885	rBV3	1830	1231	0.02%	0.004%
62	10.358	2895	2898	2903	rBV2	409	364	0.00%	0.001%
63	10.490	2931	2939	2943	rBV3	465	588	0.01%	0.002%
64	10.773	3024	3027	3033	rVB4	575	454	0.01%	0.002%
65	10.821	3038	3042	3049	rVB2	360	348	0.00%	0.001%
66	10.866	3053	3056	3060	rVB3	602	474	0.01%	0.002%
67	10.985	3089	3093	3100	rBV3	273	345	0.00%	0.001%
68	11.017	3100	3103	3106	rBV3	366	279	0.00%	0.001%
69	11.117	3123	3134	3145	rBV	188677	295529	3.77%	1.004%
70	11.204	3145	3161	3190	rVB2	1828572	3708344	47.28%	12.596%
71	11.509	3251	3256	3258	rBV5	3109	2768	0.04%	0.009%
72	11.574	3260	3276	3302	rVV2	1986788	3945520	50.30%	13.402%
73	11.847	3359	3361	3364	rBV3	468	296	0.00%	0.001%
74	11.905	3376	3379	3380	rBV2	578	308	0.00%	0.001%
75	11.918	3381	3383	3386	rVV3	507	266	0.00%	0.001%
76	11.953	3391	3394	3397	rBV2	765	398	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035281.D
 Acq On : 18 Apr 2024 14:26
 Operator : SY/MD
 Sample : P2158-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.982	3397	3403	3404	rBV4	421	374	0.00%	0.001%
78	12.030	3415	3418	3421	rBV2	445	328	0.00%	0.001%
79	12.111	3440	3443	3447	rBV3	465	420	0.01%	0.001%
80	12.136	3448	3451	3454	rVV3	525	309	0.00%	0.001%
81	12.342	3507	3515	3526	rVV5	4830	8680	0.11%	0.029%
82	12.522	3563	3571	3581	rVB7	1603	3082	0.04%	0.010%
83	12.586	3583	3591	3602	rBV4	11291	20217	0.26%	0.069%
84	12.686	3617	3622	3632	rVB6	3259	5237	0.07%	0.018%
85	12.818	3660	3663	3668	rBV	504	574	0.01%	0.002%
86	12.940	3697	3701	3703	rBV	345	315	0.00%	0.001%
87	13.066	3737	3740	3745	rVB3	599	577	0.01%	0.002%
88	13.197	3769	3781	3804	rBV	698426	1086997	13.86%	3.692%
89	13.451	3856	3860	3867	rVB2	2131	2323	0.03%	0.008%
90	13.676	3919	3930	3947	rBV	158351	254299	3.24%	0.864%
91	13.818	3970	3974	3975	rBV2	655	505	0.01%	0.002%
92	13.982	4019	4025	4031	rBV5	1692	2521	0.03%	0.009%
93	14.104	4057	4063	4080	rVB5	2109	4647	0.06%	0.016%
94	14.342	4135	4137	4142	rVB4	447	338	0.00%	0.001%
95	14.413	4156	4159	4162	rBV3	514	420	0.01%	0.001%
96	14.474	4174	4178	4181	rBV4	507	432	0.01%	0.001%
97	14.757	4252	4266	4277	rBV2	20885	38996	0.50%	0.132%
98	14.840	4289	4292	4296	rBV4	724	504	0.01%	0.002%
99	14.860	4296	4298	4300	rBV2	575	338	0.00%	0.001%
100	15.332	4436	4445	4456	rBV2	36862	58777	0.75%	0.200%

Sum of corrected areas: 29439624




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035281.D
Acq On : 18 Apr 2024 14:26
Operator : SY/MD
Sample : P2158-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

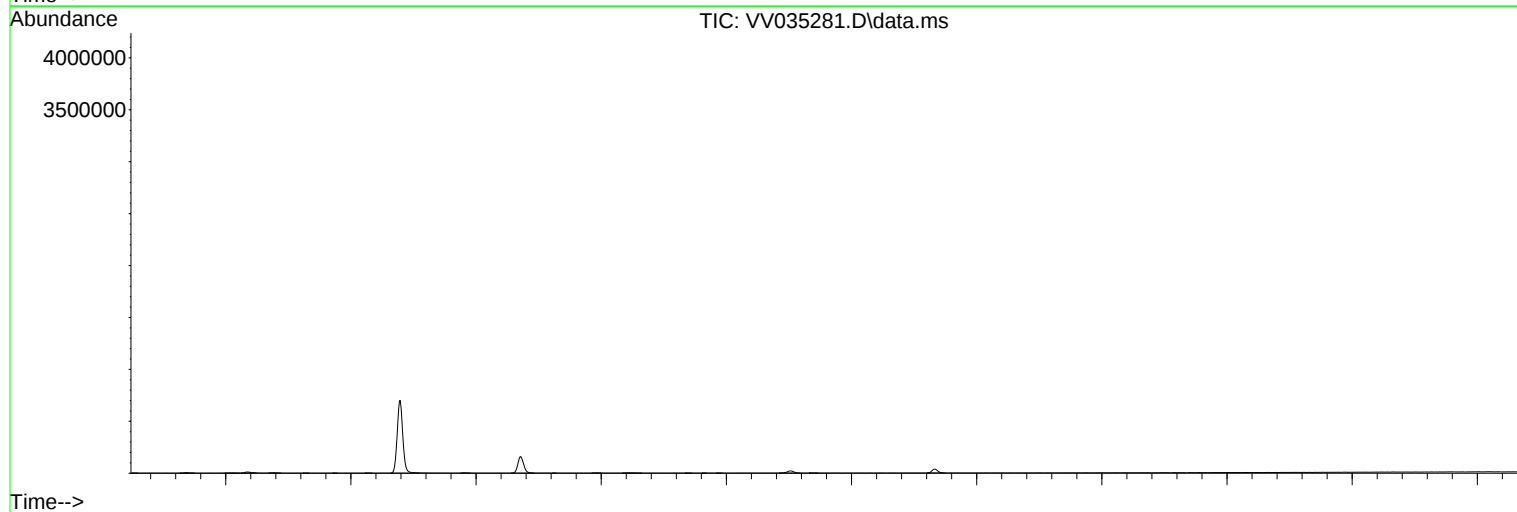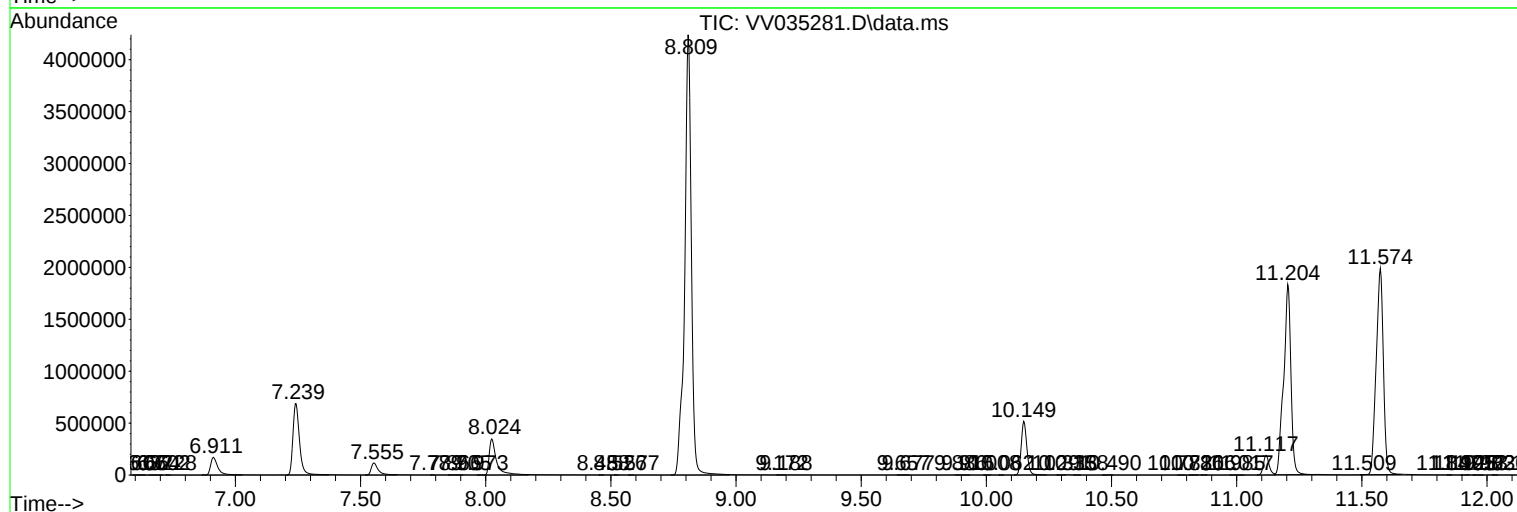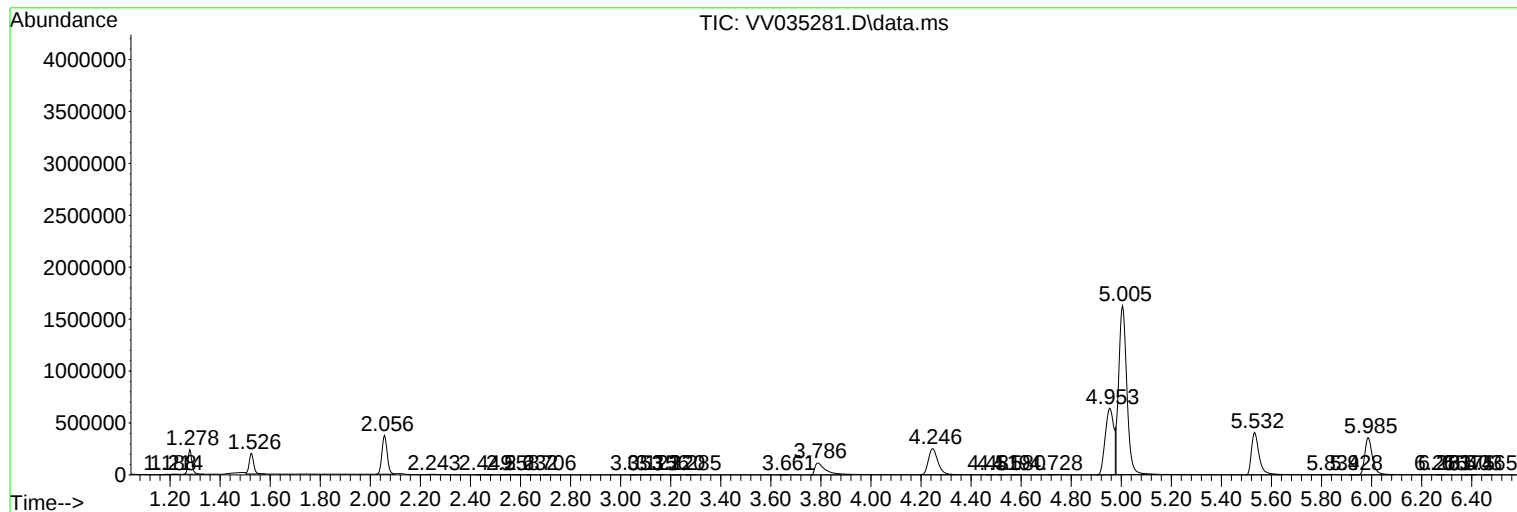

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035281.D
Acq On : 18 Apr 2024 14:26
Operator : SY/MD
Sample : P2158-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035281.D
Acq On : 18 Apr 2024 14:26
Operator : SY/MD
Sample : P2158-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc