

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035293.D
 Acq On : 18 Apr 2024 19:14
 Operator : SY/MD
 Sample : VIBLK278
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK278

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	210985	228935	13.73%	1.882%
2	1.526	145	151	164	rVB	189340	233605	14.01%	1.920%
3	2.056	307	316	336	rVB	363732	523807	31.42%	4.306%
4	2.744	529	530	532	rVB	172	46	0.00%	0.000%
5	3.002	607	610	613	rBV	395	299	0.02%	0.002%
6	3.105	639	642	644	rBV2	280	199	0.01%	0.002%
7	3.182	664	666	668	rBV	286	172	0.01%	0.001%
8	3.246	683	686	688	rBV	331	163	0.01%	0.001%
9	3.278	693	696	697	rBV2	244	146	0.01%	0.001%
10	3.442	745	747	751	rVB2	265	141	0.01%	0.001%
11	3.519	769	771	773	rBV2	204	129	0.01%	0.001%
12	3.597	793	795	797	rBV2	125	81	0.00%	0.001%
13	3.658	812	814	817	rVB2	328	158	0.01%	0.001%
14	3.748	840	842	846	rVB2	356	164	0.01%	0.001%
15	3.786	846	854	908	rBV	118708	359262	21.55%	2.953%
16	4.246	982	997	1025	rBV	258725	665296	39.90%	5.469%
17	4.722	1143	1145	1146	rBV	245	121	0.01%	0.001%
18	4.728	1146	1147	1148	rBV2	476	178	0.01%	0.001%
19	4.828	1174	1178	1181	rBV3	427	423	0.03%	0.003%
20	4.953	1200	1217	1252	rBV2	633812	1667241	100.00%	13.706%
21	5.465	1373	1376	1378	rBV3	396	228	0.01%	0.002%
22	5.532	1387	1397	1435	rBV	384666	811201	48.66%	6.669%
23	5.838	1482	1492	1512	rVB8	5357	13298	0.80%	0.109%
24	5.934	1515	1522	1524	rBV3	396	432	0.03%	0.004%
25	5.985	1525	1538	1581	rBV	365527	766968	46.00%	6.305%
26	6.317	1639	1641	1642	rBV2	198	83	0.00%	0.001%
27	6.358	1648	1654	1657	rBV4	371	458	0.03%	0.004%
28	6.403	1663	1668	1670	rBV3	468	415	0.02%	0.003%
29	6.494	1695	1696	1698	rVB	403	106	0.01%	0.001%
30	6.513	1700	1702	1704	rBV2	273	171	0.01%	0.001%
31	6.555	1712	1715	1717	rBV2	198	89	0.01%	0.001%
32	6.584	1722	1724	1725	rBV	163	64	0.00%	0.001%
33	6.593	1725	1727	1728	rBV	262	91	0.01%	0.001%
34	6.667	1748	1750	1751	rBV2	216	116	0.01%	0.001%
35	6.699	1758	1760	1761	rBV	485	180	0.01%	0.001%
36	6.754	1774	1777	1781	rBV2	515	410	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
 Data File : VV035293.D
 Acq On : 18 Apr 2024 19:14
 Operator : SY/MD
 Sample : VIBLK278
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK278

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.844	1800	1805	1808	rBV3	457	451	0.03%	0.004%
38	6.870	1811	1813	1815	rVB2	195	79	0.00%	0.001%
39	6.912	1815	1826	1858	rBV	173663	342624	20.55%	2.817%
40	7.243	1918	1929	1956	rBV	691797	1231229	73.85%	10.122%
41	7.555	2017	2026	2059	rBV	120571	227121	13.62%	1.867%
42	7.783	2096	2097	2098	rBV	466	149	0.01%	0.001%
43	7.857	2117	2120	2122	rBV4	693	415	0.02%	0.003%
44	7.947	2146	2148	2150	rVB	295	126	0.01%	0.001%
45	7.982	2156	2159	2161	rBV2	251	174	0.01%	0.001%
46	8.024	2163	2172	2212	rBV	361756	742358	44.53%	6.103%
47	8.648	2364	2366	2369	rVB3	310	136	0.01%	0.001%
48	8.683	2372	2377	2379	rBV2	329	278	0.02%	0.002%
49	8.783	2398	2408	2441	rBV2	600700	1142424	68.52%	9.392%
50	9.313	2569	2573	2574	rBV	354	202	0.01%	0.002%
51	9.600	2659	2662	2665	rBV2	278	219	0.01%	0.002%
52	9.673	2680	2685	2687	rBV3	426	335	0.02%	0.003%
53	9.706	2692	2695	2700	rVV3	314	390	0.02%	0.003%
54	9.735	2703	2704	2705	rBV3	216	50	0.00%	0.000%
55	9.773	2714	2716	2719	rBV2	174	78	0.00%	0.001%
56	9.796	2719	2723	2725	rBV2	381	246	0.01%	0.002%
57	9.837	2732	2736	2737	rBV2	300	155	0.01%	0.001%
58	9.873	2742	2747	2750	rBV4	702	831	0.05%	0.007%
59	9.963	2770	2775	2778	rBV3	513	403	0.02%	0.003%
60	9.982	2779	2781	2783	rBV	151	61	0.00%	0.001%
61	10.088	2812	2814	2815	rBV	241	103	0.01%	0.001%
62	10.149	2820	2833	2860	rBV	524660	831364	49.86%	6.835%
63	10.387	2906	2907	2909	rVB	238	66	0.00%	0.001%
64	10.416	2911	2916	2917	rBV2	282	268	0.02%	0.002%
65	10.554	2954	2959	2962	rBV2	375	316	0.02%	0.003%
66	10.599	2969	2973	2977	rVB3	266	253	0.02%	0.002%
67	10.722	3006	3011	3016	rBV3	505	560	0.03%	0.005%
68	10.831	3041	3045	3049	rVB2	610	474	0.03%	0.004%
69	10.857	3049	3053	3054	rBV	436	279	0.02%	0.002%
70	10.915	3070	3071	3072	rBV	266	93	0.01%	0.001%
71	10.969	3086	3088	3090	rBV	296	185	0.01%	0.002%
72	11.056	3112	3115	3117	rBV2	227	129	0.01%	0.001%
73	11.075	3117	3121	3124	rBV	239	221	0.01%	0.002%
74	11.127	3129	3137	3144	rBV2	7178	11757	0.71%	0.097%
75	11.185	3145	3155	3188	rVB	541985	946046	56.74%	7.777%
76	11.558	3259	3271	3296	rBV2	685562	1255263	75.29%	10.319%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035293.D
Acq On : 18 Apr 2024 19:14
Operator : SY/MD
Sample : VIBLK278
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK278

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

77	12.040	3419	3421	3422	rBV2	286	125	0.01%	0.001%
78	12.165	3457	3460	3461	rBV	570	323	0.02%	0.003%
79	12.625	3599	3603	3604	rBV	356	258	0.02%	0.002%
80	12.744	3638	3640	3643	rBV2	264	169	0.01%	0.001%
81	12.959	3704	3707	3709	rBV	373	229	0.01%	0.002%
82	13.201	3771	3782	3804	rBV	71838	121351	7.28%	0.998%
83	13.683	3923	3932	3948	rBV2	17347	28900	1.73%	0.238%

Sum of corrected areas: 12164142




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035293.D
Acq On : 18 Apr 2024 19:14
Operator : SY/MD
Sample : VIBLK278
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

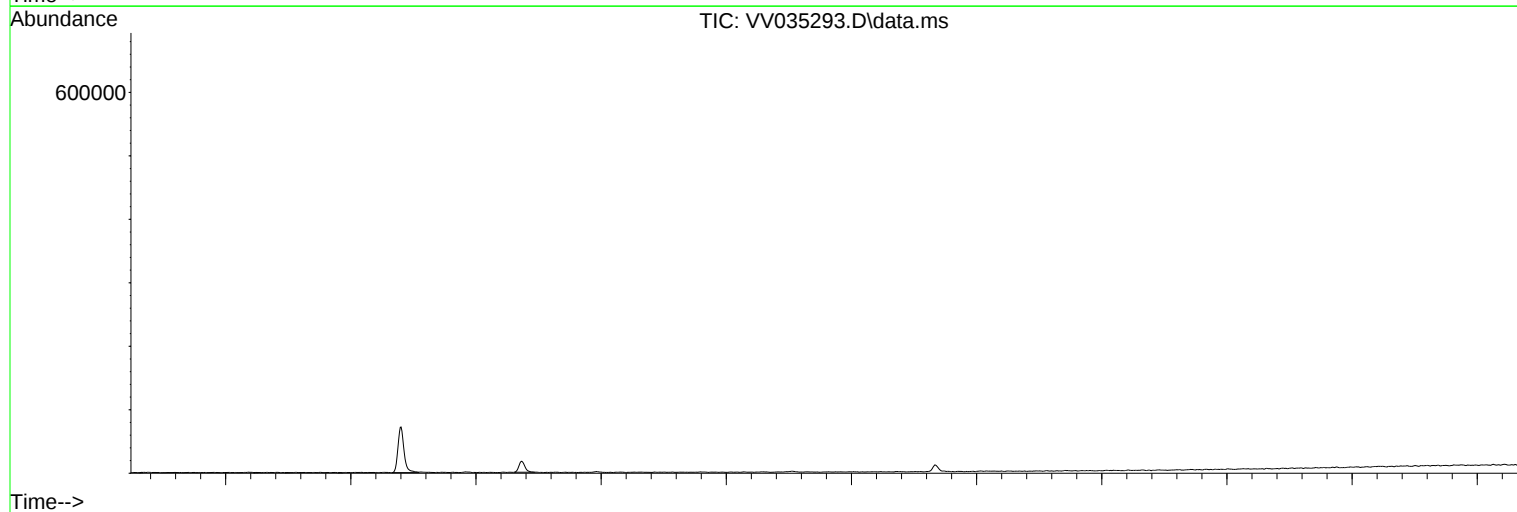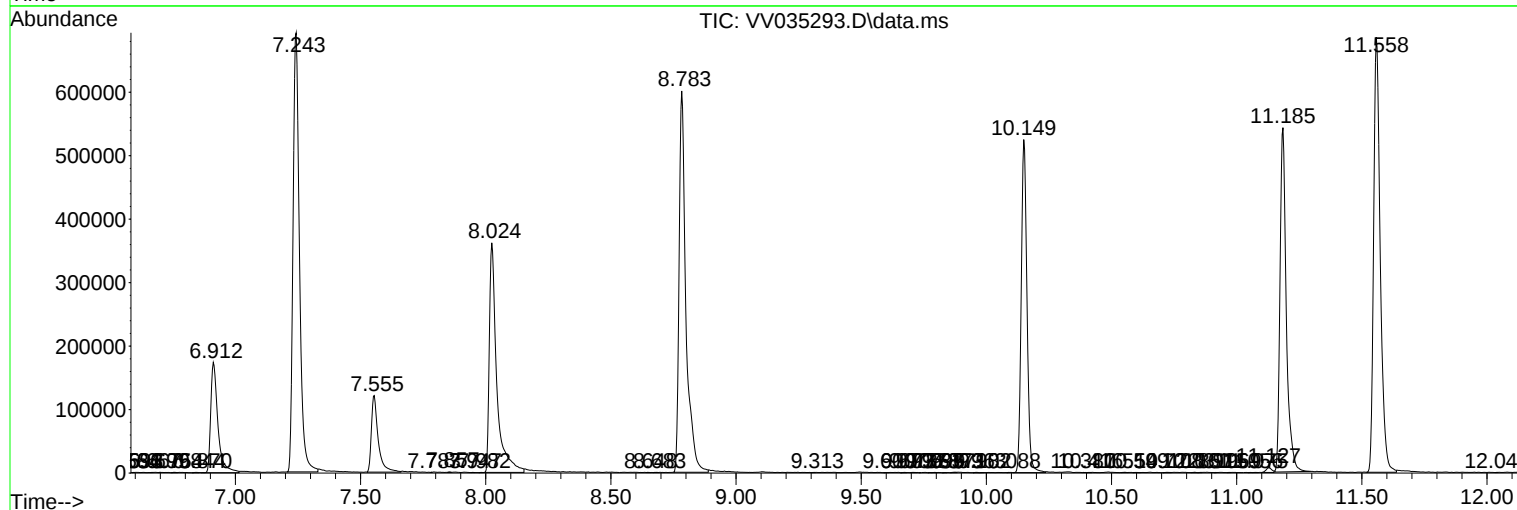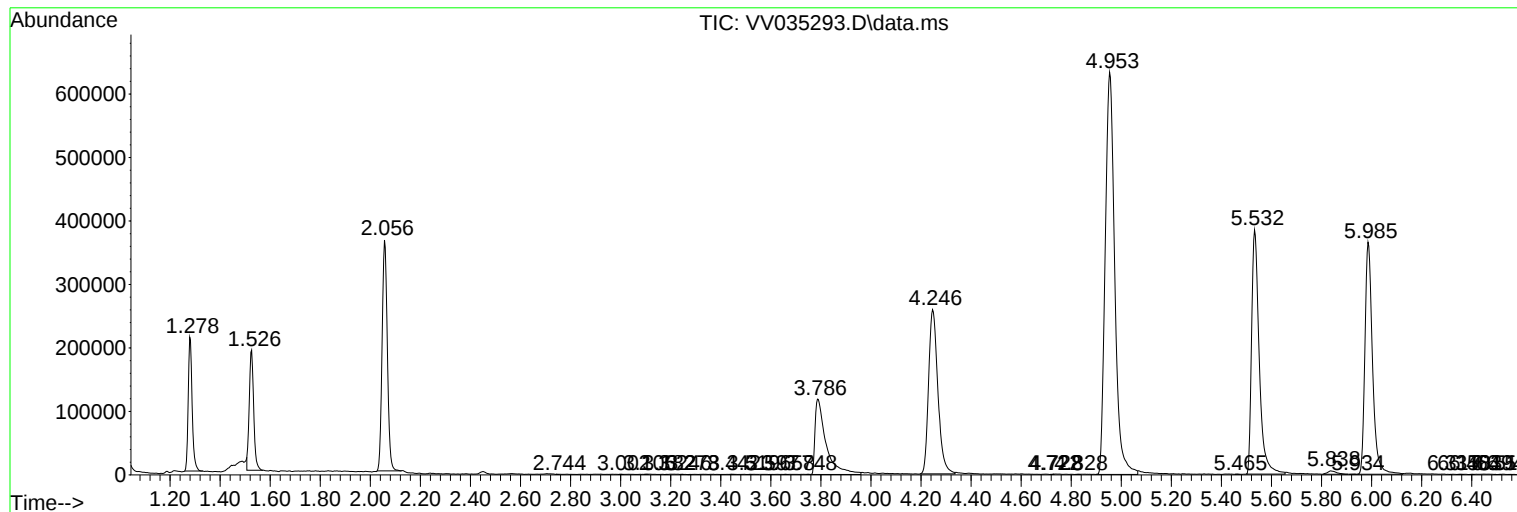

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035293.D
Acq On : 18 Apr 2024 19:14
Operator : SY/MD
Sample : VIBLK278
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035293.D
Acq On : 18 Apr 2024 19:14
Operator : SY/MD
Sample : VIBLK278
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------