
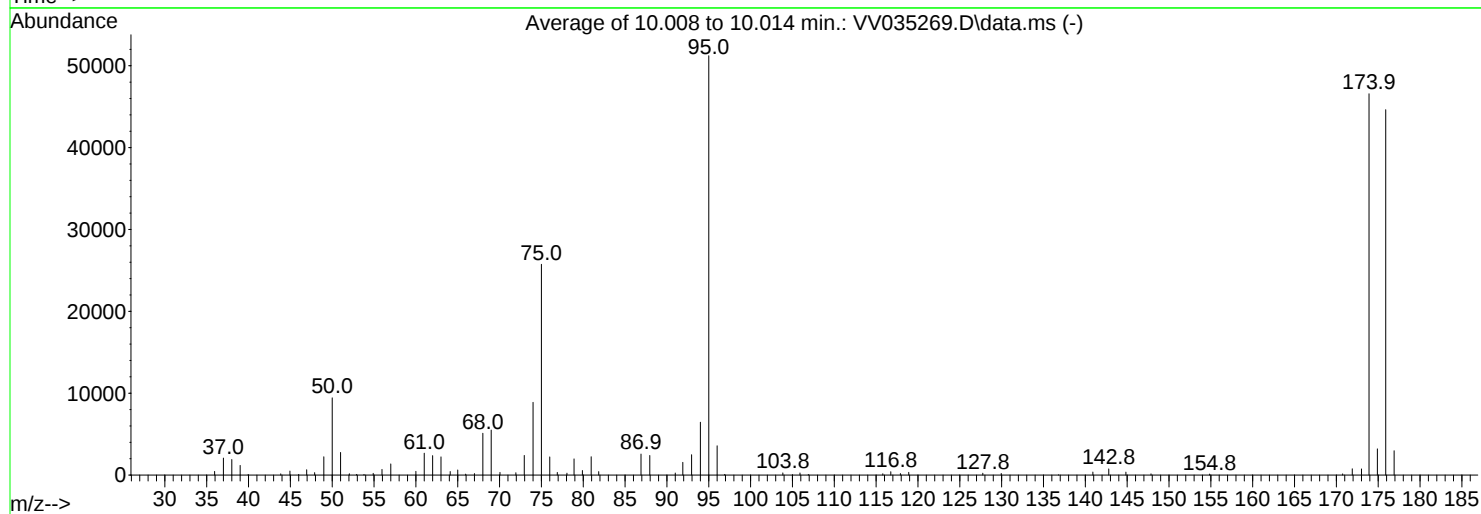


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041824\
Data File : VV035269.D
Acq On : 18 Apr 2024 08:34
Operator : SY/MD
Sample : BFB286
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB286

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Tue Apr 23 00:28:07 2024

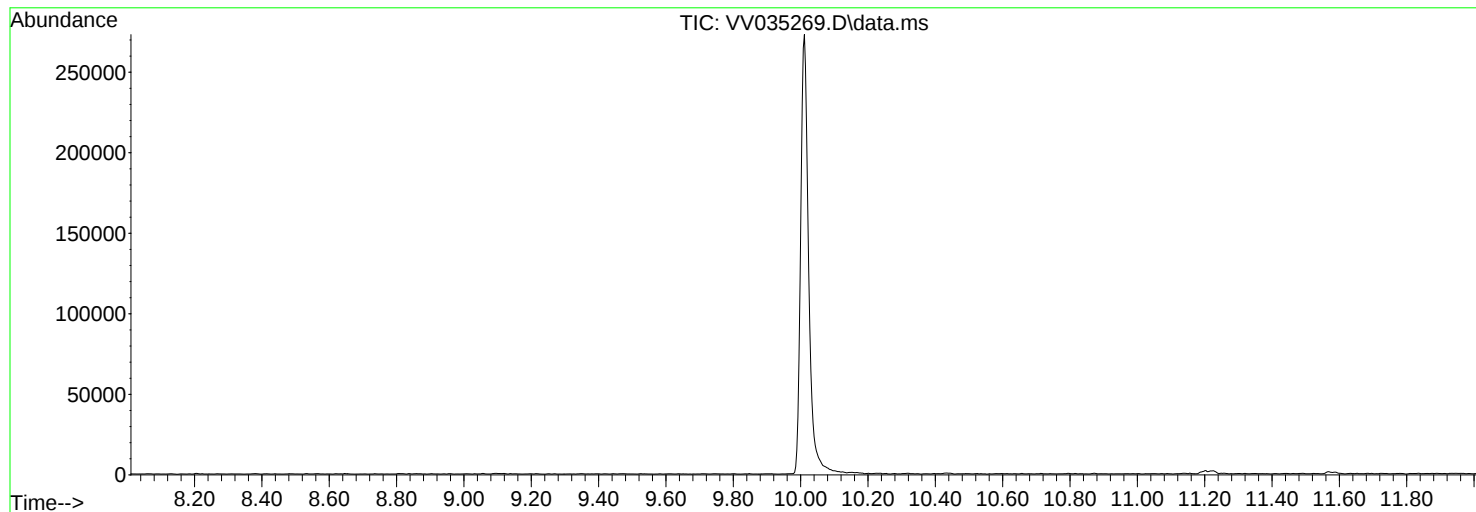

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	9436	PASS
75	95	30	80	50.3	25749	PASS
95	95	100	100	100.0	51224	PASS
96	95	5	9	7.0	3575	PASS
173	174	0.00	2	1.6	749	PASS
174	95	50	120	90.9	46579	PASS
175	174	5	9	6.9	3203	PASS
176	174	95	105	95.8	44635	PASS
177	176	5	10	6.7	2973	PASS

m/z	Abundance
39.90	264.0
43.80	504.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
35.90	429.0
37.00	2130.0
38.00	1851.0
39.00	1118.0
40.00	268.0
43.90	738.0
44.90	433.0
46.90	736.0
47.90	307.0
49.00	2286.0
50.00	9903.0
51.00	2759.0
52.00	188.0
52.90	127.0
54.90	197.0
56.00	674.0
57.00	1405.0
60.00	472.0
61.00	2635.0
62.00	2359.0
63.00	2197.0
64.10	456.0
65.00	637.0
65.90	111.0
67.00	189.0
68.00	5428.0
69.00	5798.0
70.10	344.0
72.00	294.0
73.00	2380.0
74.00	9007.0
75.00	26240.0
76.00	2222.0
76.90	344.0
78.10	228.0
78.90	2056.0
79.90	532.0
80.90	2264.0
81.90	419.0
86.90	2616.0
87.90	2330.0
91.00	222.0
91.90	1561.0
93.00	2582.0
94.00	6638.0
95.00	51968.0
96.00	3541.0
103.80	243.0
105.00	108.0
105.90	245.0
106.90	129.0
115.80	162.0
116.70	414.0
117.90	233.0
118.90	353.0
127.70	182.0
129.90	152.0
141.00	378.0
142.80	725.0
144.80	377.0
147.90	146.0
154.90	135.0
170.80	175.0
171.90	671.0
173.00	731.0
173.90	45808.0
174.90	3138.0
175.90	43928.0
176.90	2914.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
36.00	461.0
37.00	2153.0
38.00	1949.0
39.00	1241.0
40.10	351.0
44.00	687.0
45.00	518.0
46.00	125.0
46.90	632.0
47.90	287.0
49.00	2301.0
50.00	9804.0
51.00	2862.0
52.10	159.0
52.90	100.0
53.80	117.0
54.90	214.0
55.90	703.0
57.00	1410.0
60.00	480.0
61.00	2769.0
62.00	2420.0
63.00	2287.0
64.10	461.0
65.00	654.0
66.00	125.0
67.00	196.0
68.00	5245.0
69.00	5641.0
70.10	339.0
71.90	300.0
73.00	2484.0
74.00	9205.0
75.00	26648.0
76.00	2283.0
76.90	336.0
78.10	237.0
78.90	2069.0
79.90	556.0
80.90	2329.0
81.80	438.0
86.90	2695.0
88.00	2462.0
91.00	268.0
91.90	1570.0
93.00	2531.0
94.00	6676.0
95.00	52984.0
96.00	3731.0
96.90	112.0
103.80	269.0
105.90	268.0
106.90	109.0
115.80	168.0
116.70	418.0
117.90	200.0
118.90	349.0
127.80	240.0
130.00	211.0
136.80	117.0
140.90	360.0
142.80	778.0
144.90	361.0
147.90	158.0
154.90	126.0
170.80	147.0
171.90	785.0
173.00	773.0
173.90	48048.0
174.90	3261.0
175.90	46480.0
176.90	3115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286

m/z	Abundance
36.00	447.0
37.00	1946.0
38.00	1895.0
39.00	1181.0
40.00	346.0
44.00	540.0
45.00	526.0
46.00	128.0
47.00	581.0
47.90	305.0
49.00	2114.0
50.00	8602.0
51.00	2667.0
52.10	144.0
53.80	127.0
54.90	220.0
55.90	696.0
57.00	1265.0
60.00	428.0
61.00	2620.0
62.00	2337.0
63.00	2191.0
64.10	390.0
65.00	574.0
66.00	113.0
67.00	169.0
68.00	4655.0
69.00	5065.0
70.00	300.0
71.90	274.0
72.90	2333.0
74.00	8450.0
75.00	24360.0
76.00	2140.0
76.90	284.0
78.00	238.0
78.90	1802.0
79.90	580.0
81.00	2137.0
81.80	414.0
86.90	2398.0
88.00	2388.0
91.00	263.0
91.90	1527.0
92.90	2345.0
94.00	6061.0
95.00	48720.0
96.00	3452.0
96.90	133.0
103.90	284.0
105.90	268.0
115.80	157.0
116.80	400.0
117.80	136.0
118.90	296.0
127.80	269.0
129.90	242.0
140.80	376.0
142.80	745.0
144.90	357.0
147.80	151.0
154.80	104.0
170.70	111.0
171.90	848.0
173.00	743.0
173.90	45880.0
174.90	3210.0
175.90	43496.0
176.90	2890.0

Instrument :
MSVOA_V
ClientSampleId :
BFB286