




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025630.D
Acq On : 19 Apr 2022 13:58
Operator : SY/MD
Sample : N2471-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFG3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/20/2022
Supervised By :Mahesh Dadoda 04/20/2022

Quant Time: Apr 20 02:52:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 20 02:46:45 2022
Response via : Initial Calibration

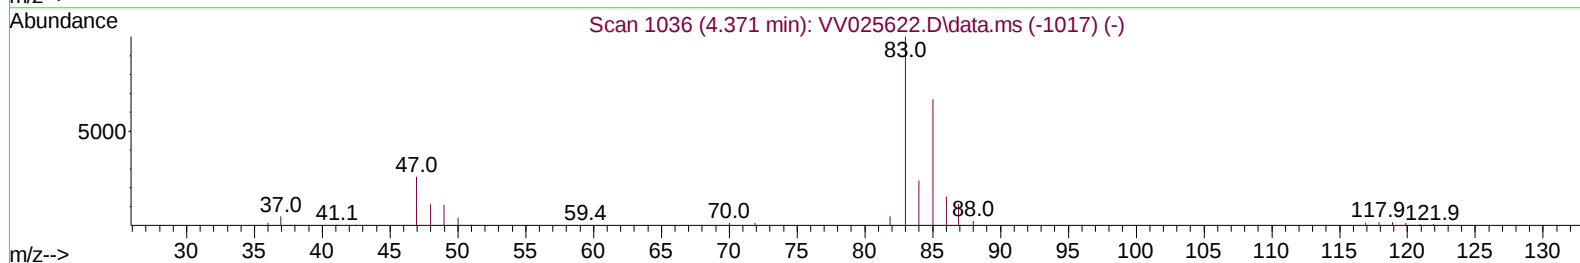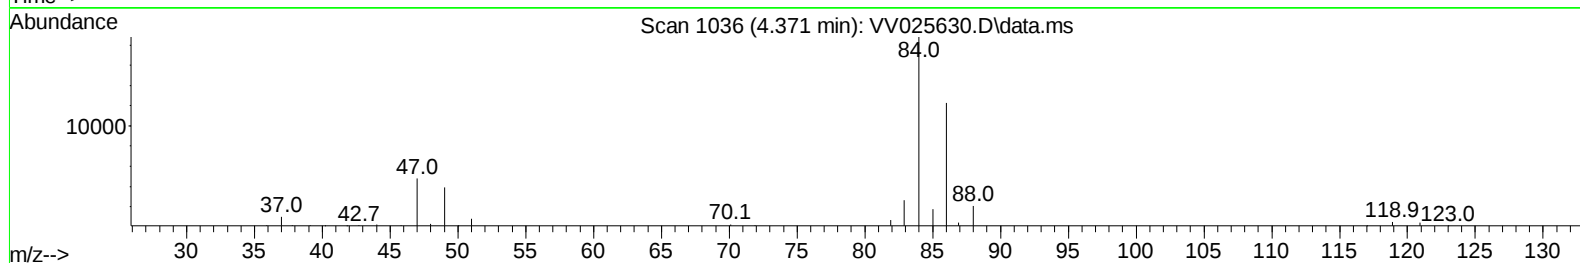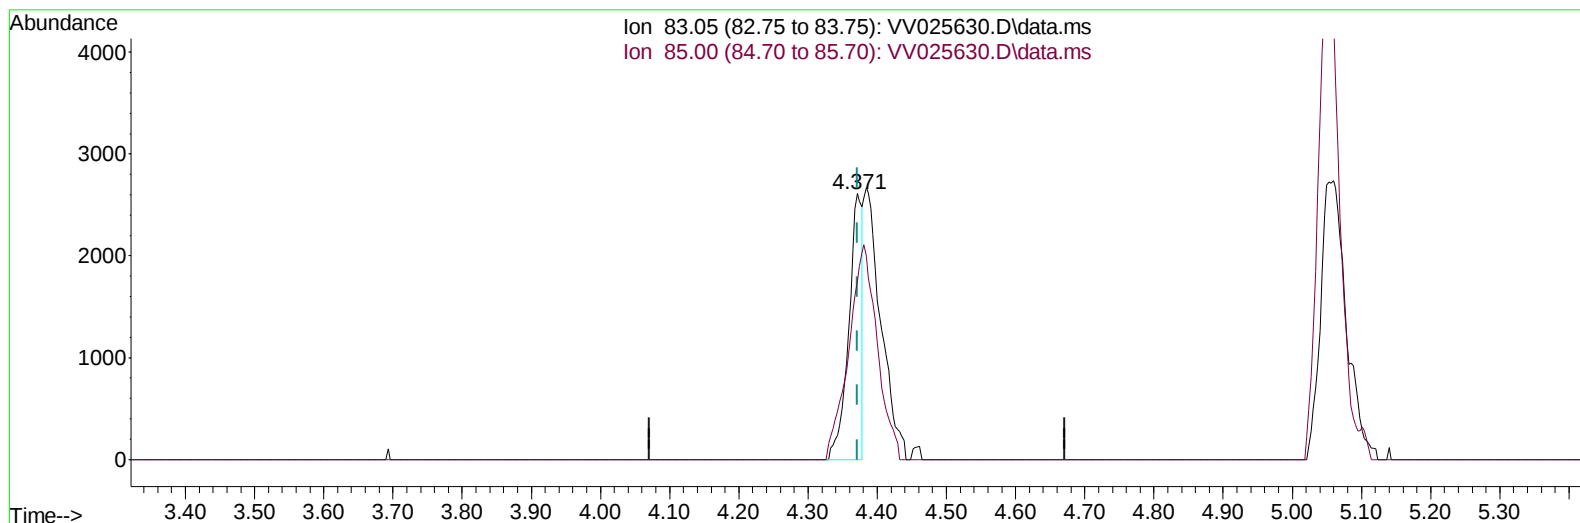

TIC: VV025630.D\data.ms

(25) Chloroform (T)

4.371min (-0.000) 0.20 ug/L

response 3498

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	62.10	67.06
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
 Data File : VV025630.D
 Acq On : 19 Apr 2022 13:58
 Operator : SY/MD
 Sample : N2471-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFG3

Manual IntegrationsAPPROVED

Quant Time: Apr 20 02:52:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 20 02:46:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/20/2022
 Supervised By :Mahesh Dadoda 04/20/2022

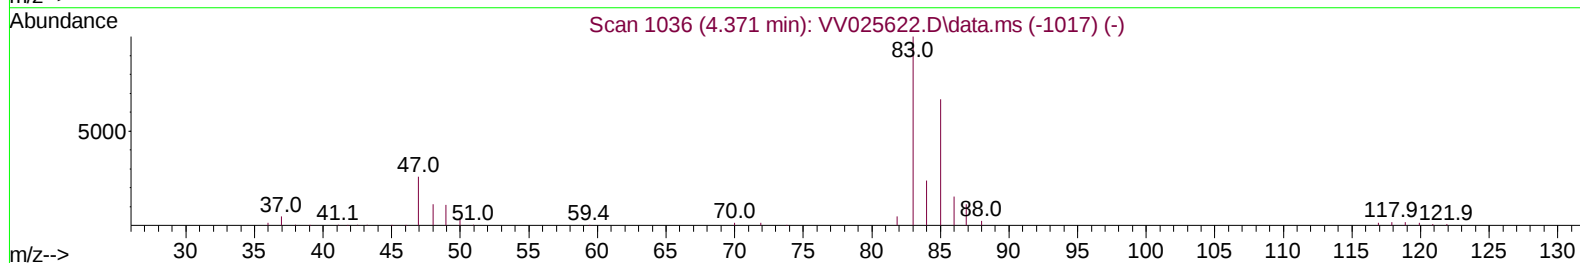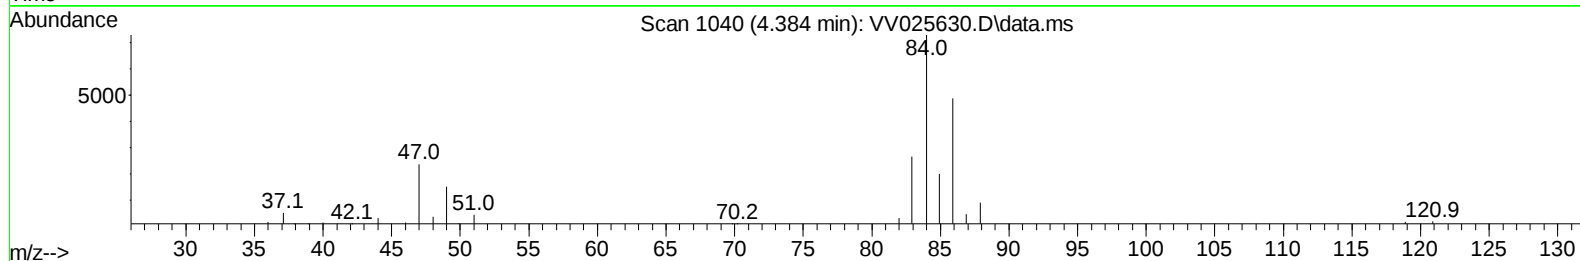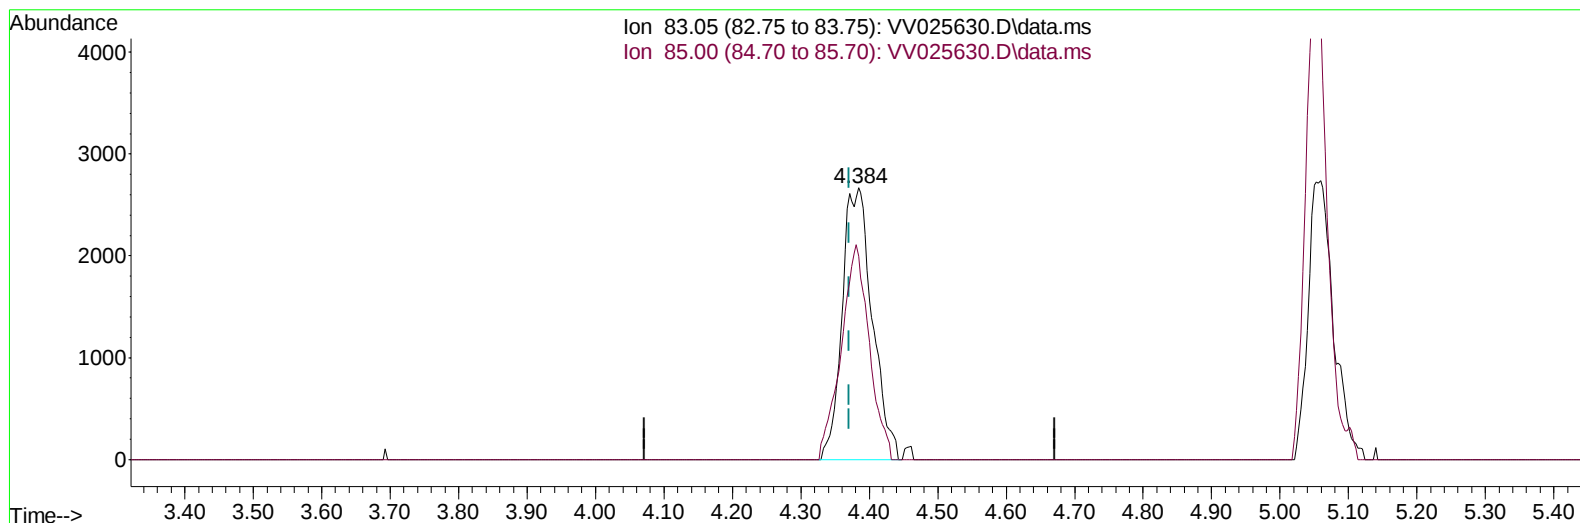

TIC: VV025630.D\data.ms

(25) Chloroform (T)

4.384min (+ 0.013) 0.46 ug/L m

response 8131

Ion	Exp%	Act%
83.05	100.00	100.00
85.00	62.10	74.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
 Data File : VV025630.D
 Acq On : 19 Apr 2022 13:58
 Operator : SY/MD
 Sample : N2471-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFG3

Manual IntegrationsAPPROVED

Quant Time: Apr 20 02:52:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 20 02:46:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/20/2022
 Supervised By :Mahesh Dadoda 04/20/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		136598	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		140031	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		64552	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.310	65		51633	4.066	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.400%	
7) Chloroethane-d5	1.574	69		49444	3.660	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.200%	
11) 1,1-Dichloroethene-d2	2.114	63		80822	3.177	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.600%	
20) 2-Butanone-d5	3.899	46		66841	43.269	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.540%	
24) Chloroform-d	4.352	84		84093	4.382	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%	
26) 1,2-Dichloroethane-d4	5.037	65		38883	4.702	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%	
32) Benzene-d6	5.053	84		165438	4.083	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.600%	
36) 1,2-Dichloropropane-d6	6.072	67		50906	4.505	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.200%	
41) Toluene-d8	7.316	98		138157	3.674	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.400%	
43) trans-1,3-Dichloroprop...	7.625	79		13997	3.685	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.800%	
46) 2-Hexanone-d5	8.088	63		48457	36.353	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.700%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84		28222	3.953	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152		48387	4.471	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.400%	
Target Compounds							
13) Acetone	2.188	43		4464	4.257	ug/L	86
25) Chloroform	4.384	83		8131m	0.458	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025630.D
Acq On : 19 Apr 2022 13:58
Operator : SY/MD
Sample : N2471-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFG3

Manual IntegrationsAPPROVED

Quant Time: Apr 20 02:52:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 20 02:46:45 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/20/2022
Supervised By :Mahesh Dadoda 04/20/2022

