

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041922\
 Data File : VW025628.D
 Acq On : 19 Apr 2022 12:33
 Operator : SY/MD
 Sample : N2384-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 20 02:51:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 20 02:46:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	189647	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	192788	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	87985	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.311	65	71933	4.080	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.600%
7) Chloroethane-d5	1.571	69	72120	3.845	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.800%
11) 1,1-Dichloroethene-d2	2.111	63	111994	3.171	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%
20) 2-Butanone-d5	3.886	46	96536	45.011	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.020%
24) Chloroform-d	4.346	84	115994	4.354	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.000%
26) 1,2-Dichloroethane-d4	5.027	65	53681	4.676	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%
32) Benzene-d6	5.047	84	231967	4.159	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.200%
36) 1,2-Dichloropropane-d6	6.066	67	69229	4.450	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.000%
41) Toluene-d8	7.313	98	200779	3.879	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.600%
43) trans-1,3-Dichloroprop...	7.622	79	20917	4.000	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%
46) 2-Hexanone-d5	8.085	63	71449	38.934	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.860%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	40214	4.092	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	65189	4.419	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.400%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	3175	0.199	ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025628.D
Acq On : 19 Apr 2022 12:33
Operator : SY/MD
Sample : N2384-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Apr 20 02:51:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 20 02:46:45 2022
Response via : Initial Calibration

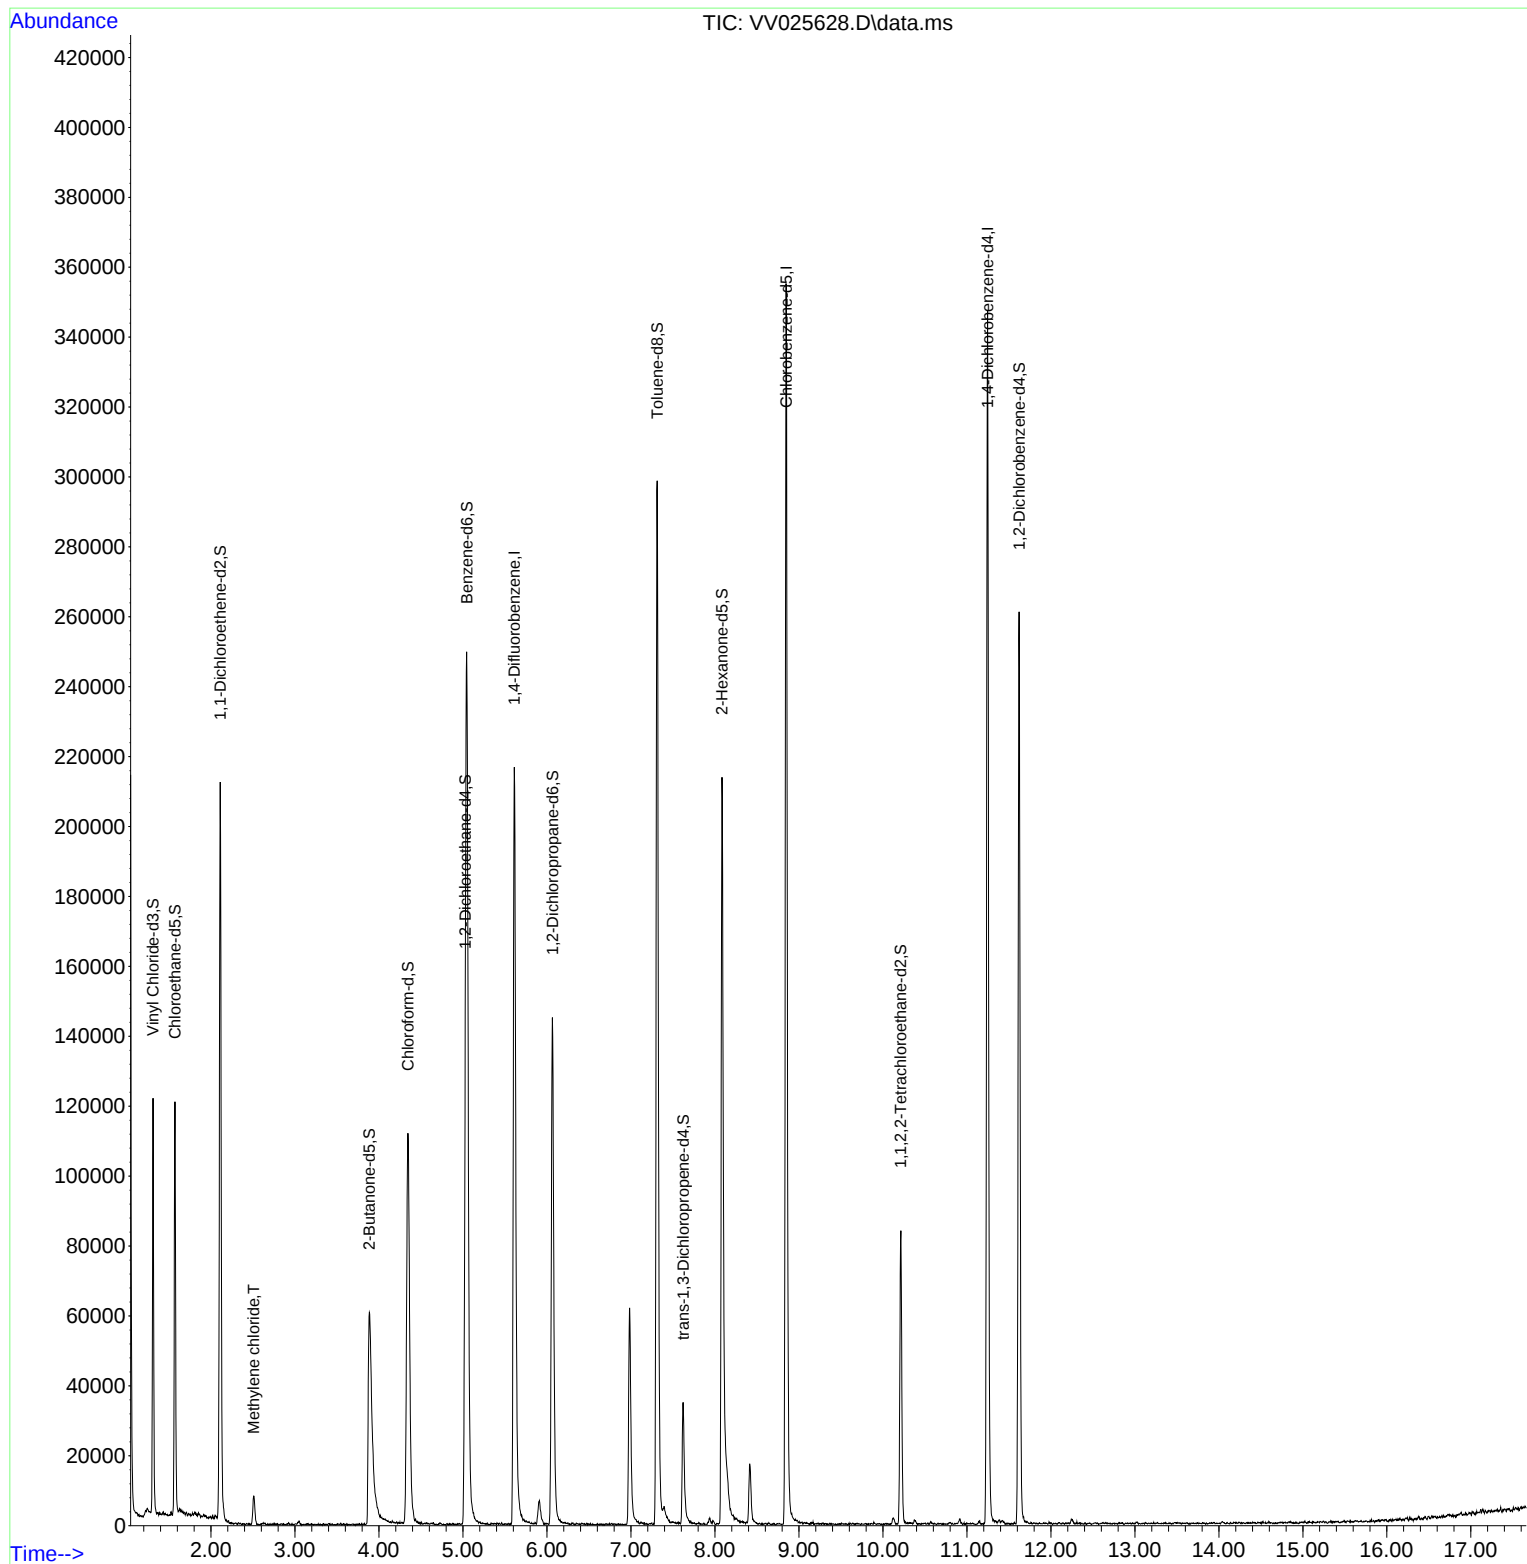

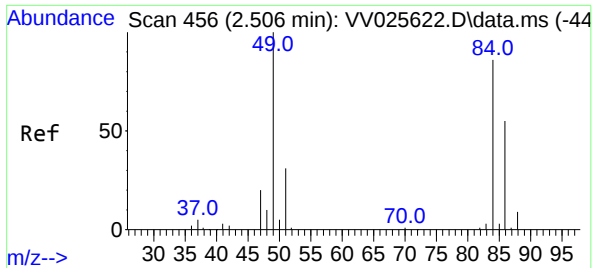

#16
Methylene chloride
Concen: 0.199 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025628.D
Acq: 19 Apr 2022 12:33

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

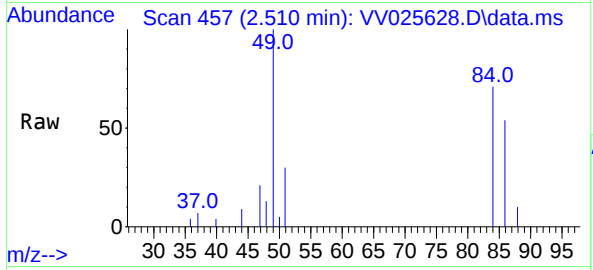

Tgt Ion: 84 Resp: 3175
Ion Ratio Lower Upper
84 100
86 76.0 45.9 85.3
49 140.7 76.6 142.3

