

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
 Data File : VV025625.D
 Acq On : 19 Apr 2022 10:58
 Operator : SY/MD
 Sample : N2384-13DL 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Q4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	93	rVB	90156	92558	19.03%	2.109%
2	1.571	157	165	176	rBV	86549	97843	20.12%	2.229%
3	2.111	322	333	351	rVB	172891	252101	51.84%	5.744%
4	3.915	878	894	939	rBV3	35075	163810	33.69%	3.732%
5	4.352	1011	1030	1054	rBV2	88692	221958	45.65%	5.057%
6	5.050	1231	1247	1276	rBV3	194390	486266	100.00%	11.079%
7	5.619	1411	1424	1448	rBV2	167244	345022	70.95%	7.861%
8	5.915	1505	1516	1526	rBV8	5090	9577	1.97%	0.218%
9	6.072	1551	1565	1587	rBV	110761	232696	47.85%	5.302%
10	6.989	1840	1850	1869	rBV	46060	89345	18.37%	2.036%
11	7.317	1939	1952	1973	rBV	223874	403239	82.93%	9.187%
12	7.625	2039	2048	2073	rBV2	25632	49366	10.15%	1.125%
13	7.976	2142	2157	2179	rBV	187125	315789	64.94%	7.195%
14	8.091	2181	2193	2225	rBV	156173	328055	67.46%	7.474%
15	8.419	2284	2295	2305	rBV3	10971	17758	3.65%	0.405%
16	8.850	2419	2429	2450	rBV	276369	446745	91.87%	10.178%
17	10.214	2843	2853	2870	rBV	67565	106300	21.86%	2.422%
18	11.246	3161	3174	3194	rBV	266345	413024	84.94%	9.410%
19	11.622	3281	3291	3309	rBV	200482	317697	65.33%	7.238%




Sum of corrected areas: 4389149

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025625.D
Acq On : 19 Apr 2022 10:58
Operator : SY/MD
Sample : N2384-13DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

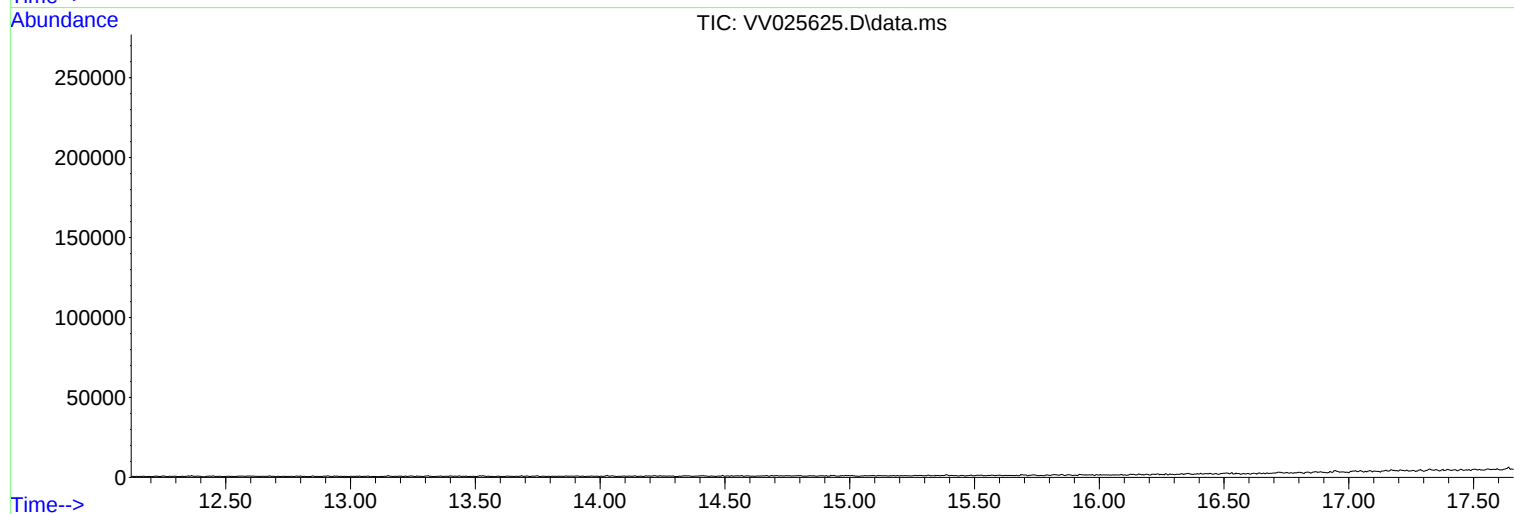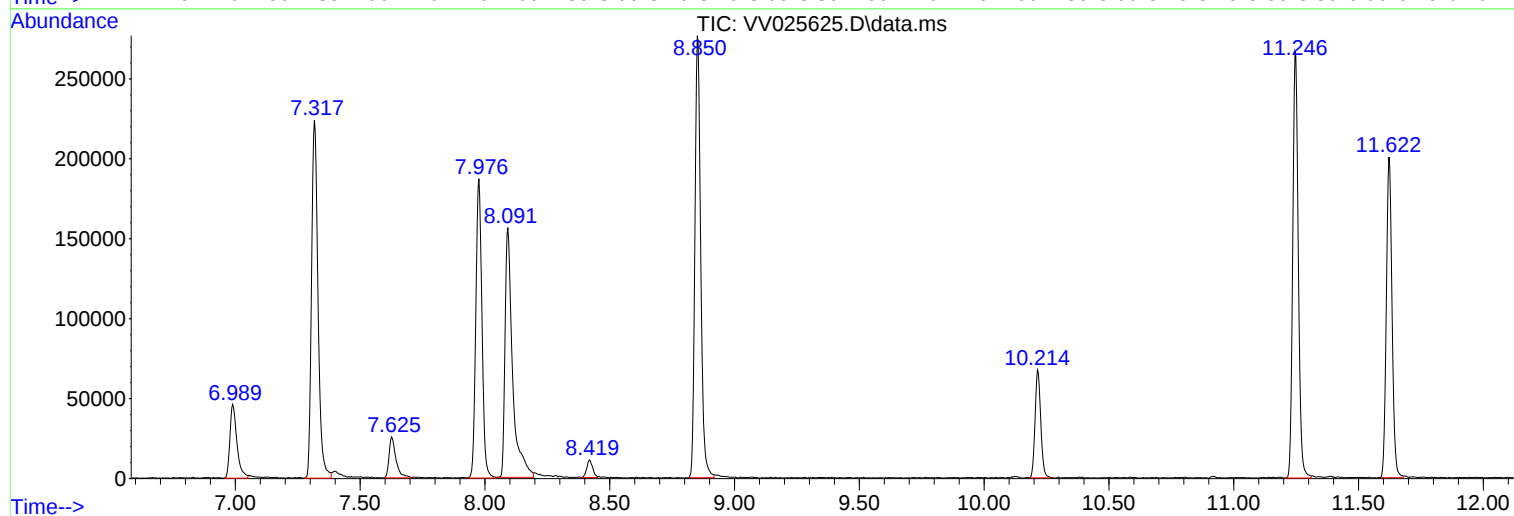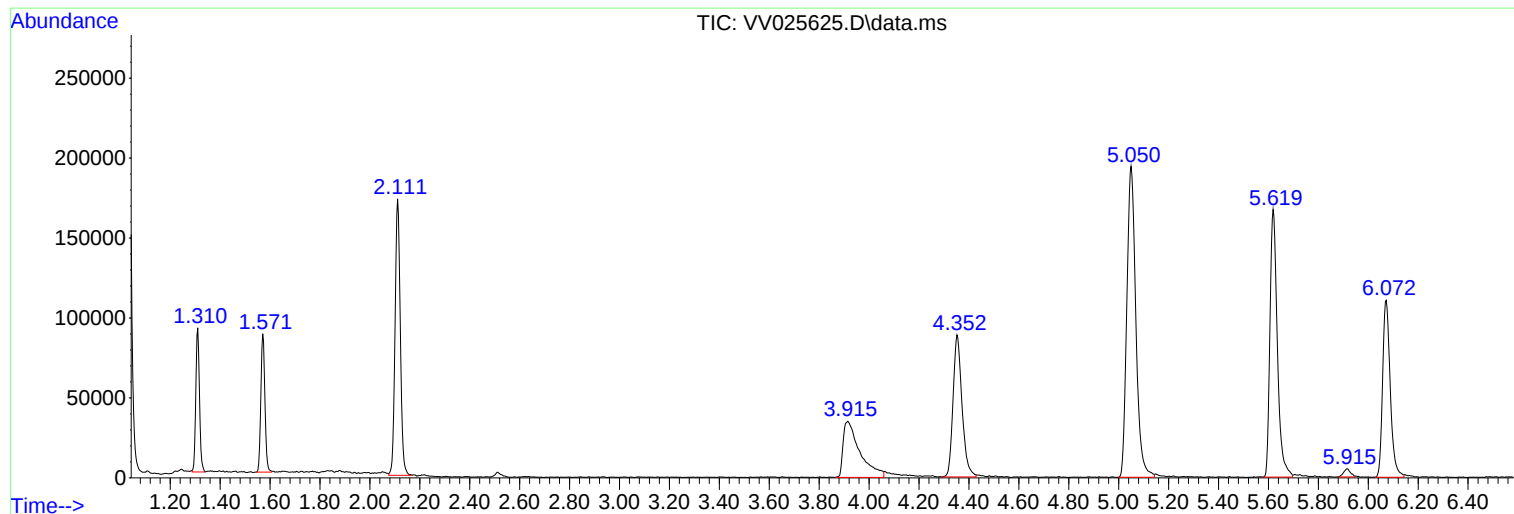

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025625.D
Acq On : 19 Apr 2022 10:58
Operator : SY/MD
Sample : N2384-13DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025625.D
Acq On : 19 Apr 2022 10:58
Operator : SY/MD
Sample : N2384-13DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc