

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
 Data File : VV025626.D
 Acq On : 19 Apr 2022 11:21
 Operator : SY/MD
 Sample : N2384-10DL 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Q1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	77	84	102	rVB	89880	95440	20.04%	2.163%
2	1.574	158	166	175	rBV	81821	91798	19.28%	2.080%
3	2.111	322	333	355	rVB	159256	240714	50.55%	5.456%
4	2.516	447	459	469	rBV5	2828	4782	1.00%	0.108%
5	3.915	876	894	930	rBV3	53490	202428	42.51%	4.588%
6	4.355	1015	1031	1055	rBV2	85531	216994	45.57%	4.918%
7	5.050	1232	1247	1275	rBV2	190668	476207	100.00%	10.793%
8	5.619	1413	1424	1453	rBV	159056	330454	69.39%	7.489%
9	5.921	1506	1518	1541	rVB5	19256	45247	9.50%	1.025%
10	6.072	1552	1565	1592	rBV	112117	228902	48.07%	5.188%
11	6.989	1839	1850	1871	rBV2	45126	87780	18.43%	1.989%
12	7.317	1940	1952	1973	rBV	221429	387869	81.45%	8.791%
13	7.625	2039	2048	2063	rBV2	25584	46835	9.84%	1.061%
14	7.976	2145	2157	2175	rBV	209489	351422	73.80%	7.965%
15	8.092	2183	2193	2231	rBV	160022	332066	69.73%	7.526%
16	8.420	2283	2295	2313	rVB3	14805	26339	5.53%	0.597%
17	8.850	2418	2429	2456	rBV	265401	433412	91.01%	9.823%
18	10.217	2842	2854	2866	rBV	65867	105830	22.22%	2.399%
19	11.249	3164	3175	3194	rBV	255856	393967	82.73%	8.929%
20	11.622	3280	3291	3312	rBV	198783	313827	65.90%	7.113%




Sum of corrected areas: 4412313

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025626.D
Acq On : 19 Apr 2022 11:21
Operator : SY/MD
Sample : N2384-10DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

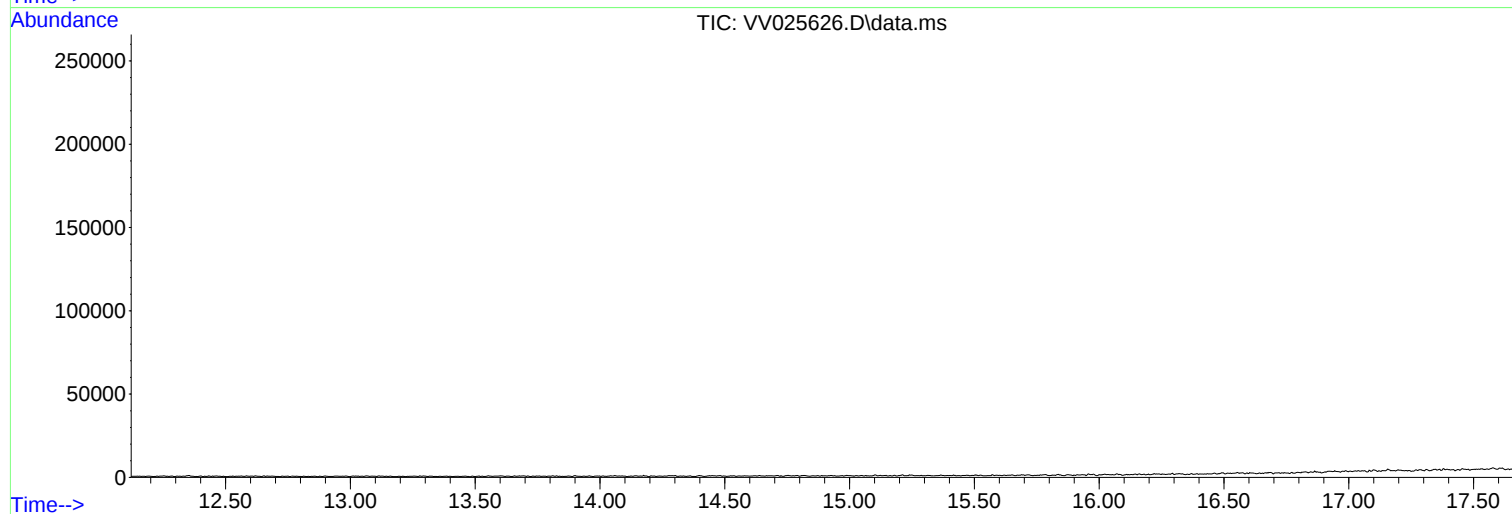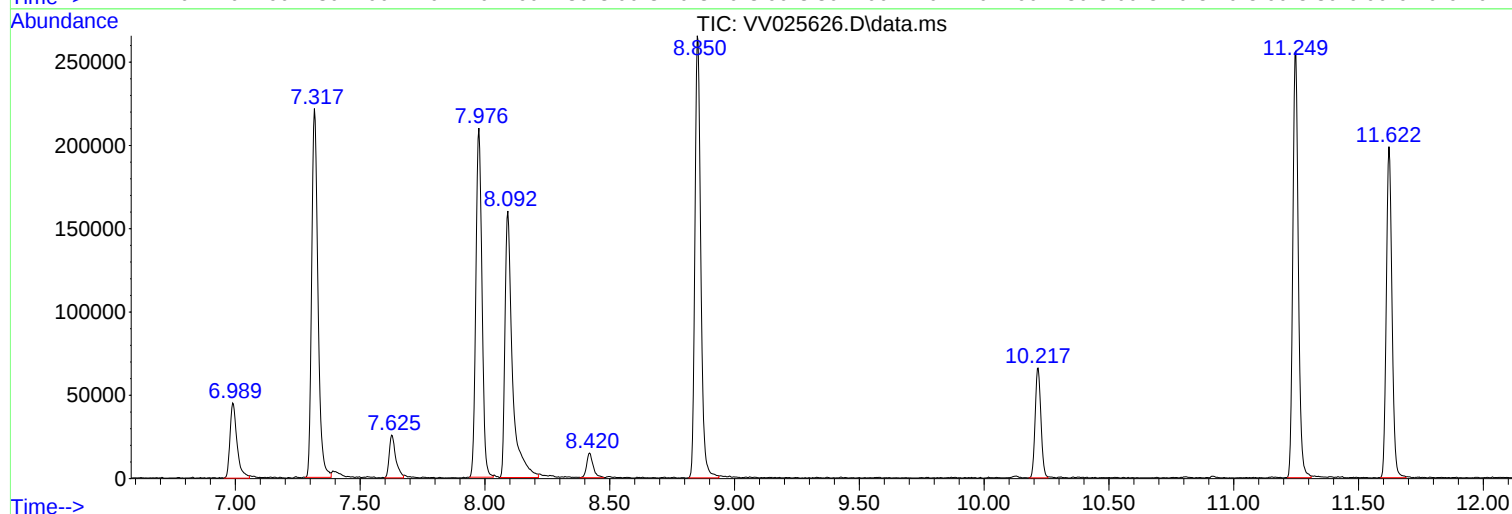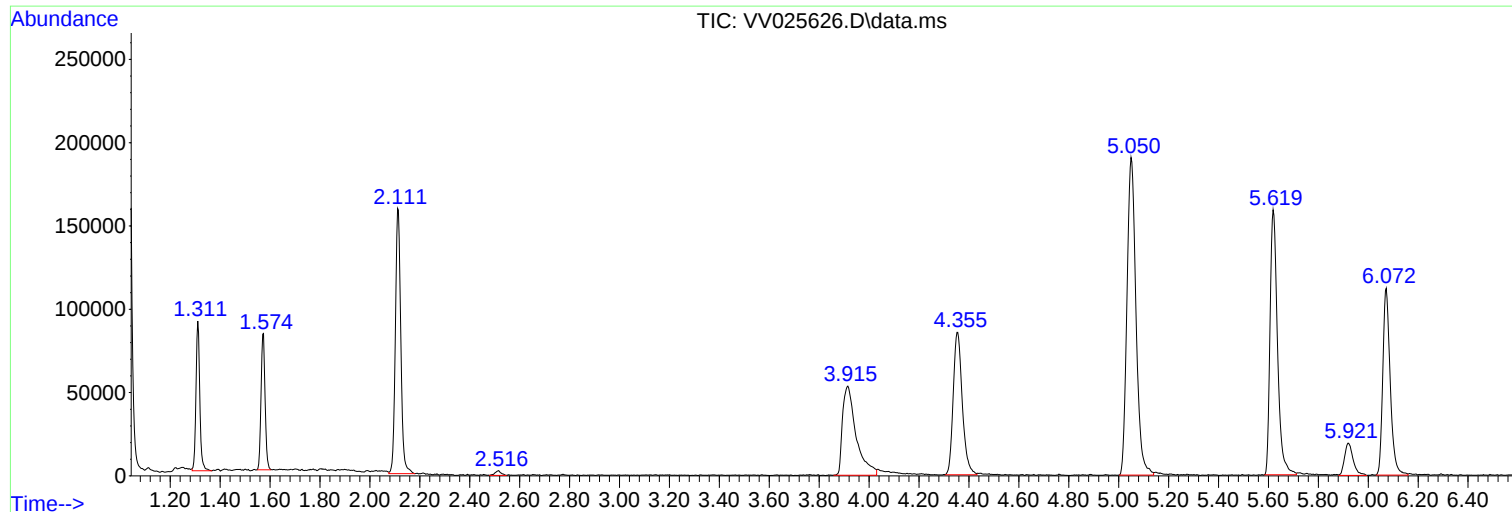

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025626.D
Acq On : 19 Apr 2022 11:21
Operator : SY/MD
Sample : N2384-10DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025626.D
Acq On : 19 Apr 2022 11:21
Operator : SY/MD
Sample : N2384-10DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc