

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
 Data File : VV025632.D
 Acq On : 19 Apr 2022 16:24
 Operator : SY/MD
 Sample : N2384-07DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6P8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	100	rVB	108157	111038	18.21%	2.160%
2	1.571	157	165	182	rBV	106667	124372	20.39%	2.419%
3	2.111	322	333	351	rVB	192830	283295	46.45%	5.510%
4	2.513	446	458	472	rBV	21323	36626	6.01%	0.712%
5	3.899	873	889	927	rBV2	57681	202170	33.15%	3.932%
6	4.352	1008	1030	1060	rBV	109882	282123	46.26%	5.487%
7	5.050	1231	1247	1282	rBV2	244254	609899	100.00%	11.862%
8	5.619	1412	1424	1453	rBV	213480	441416	72.38%	8.585%
9	5.915	1506	1516	1531	rBV8	6074	13597	2.23%	0.264%
10	6.072	1552	1565	1592	rBV	141343	294908	48.35%	5.736%
11	6.989	1838	1850	1873	rBV2	59557	114208	18.73%	2.221%
12	7.317	1937	1952	1973	rBV	283540	502495	82.39%	9.773%
13	7.625	2038	2048	2073	rBV2	33023	61939	10.16%	1.205%
14	7.982	2151	2159	2168	rVB9	3676	6210	1.02%	0.121%
15	8.088	2182	2192	2221	rBV	210448	423508	69.44%	8.237%
16	8.850	2418	2429	2459	rBV	345841	565677	92.75%	11.002%
17	10.214	2842	2853	2868	rBV	83900	133679	21.92%	2.600%
18	10.381	2897	2905	2918	rVB3	4496	8118	1.33%	0.158%
19	11.246	3163	3174	3192	rBV	338699	519064	85.11%	10.096%
20	11.622	3280	3291	3319	rBV	260123	407196	66.76%	7.920%




Sum of corrected areas: 5141538

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025632.D
Acq On : 19 Apr 2022 16:24
Operator : SY/MD
Sample : N2384-07DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6P8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

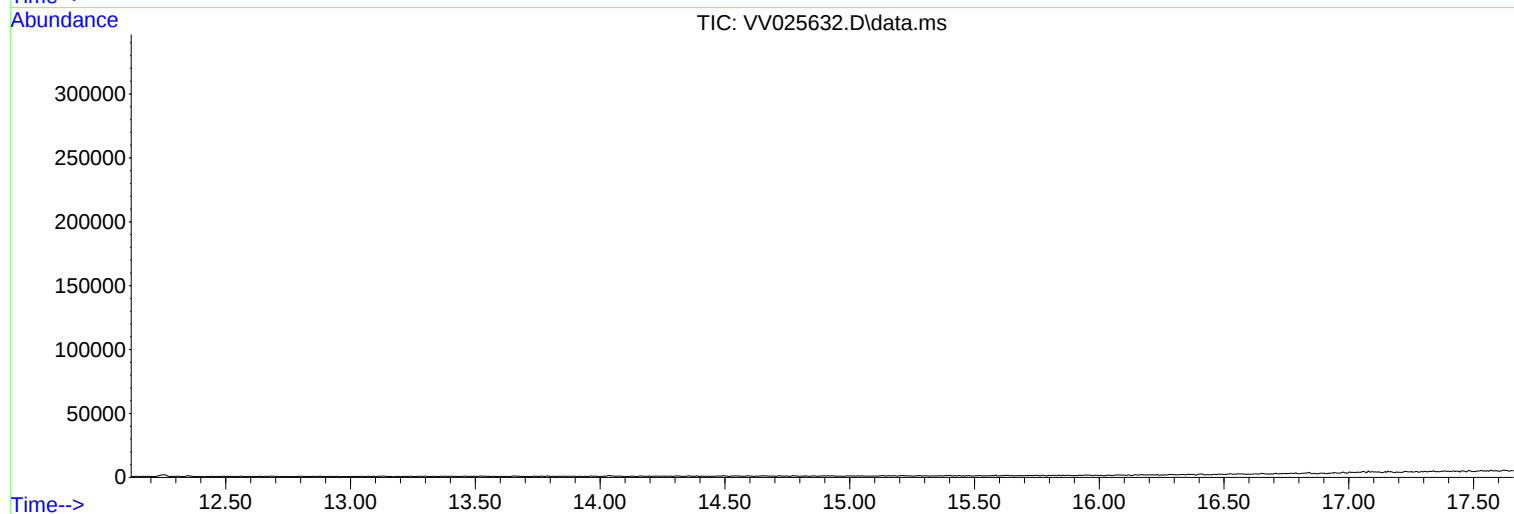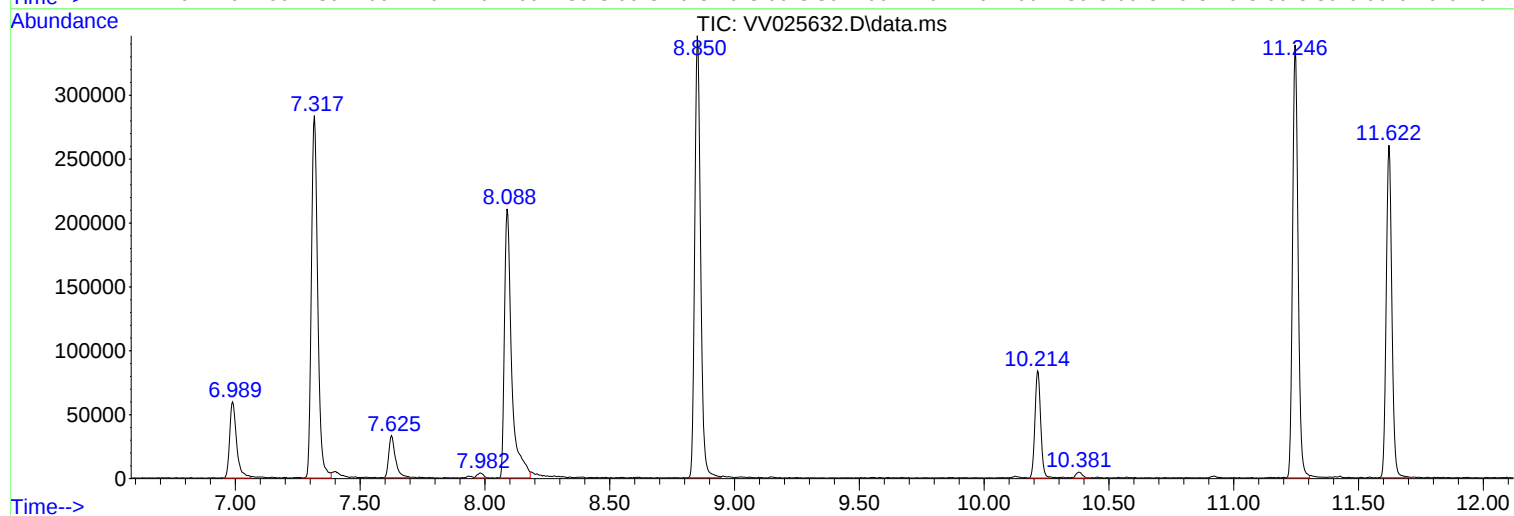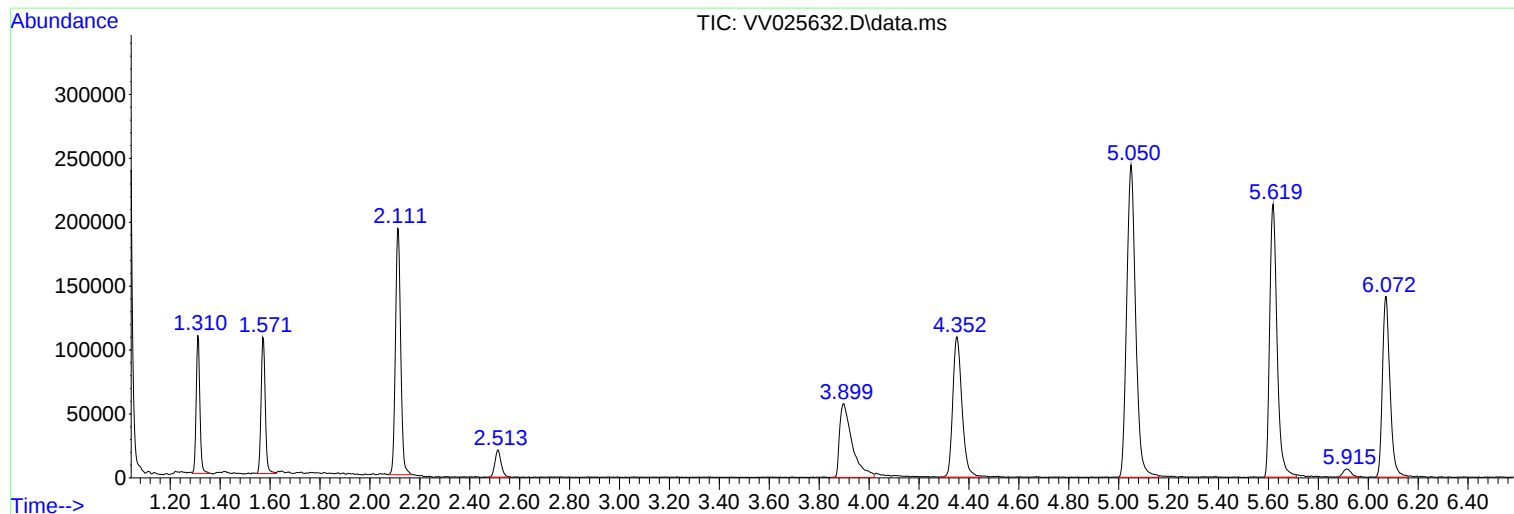

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025632.D
Acq On : 19 Apr 2022 16:24
Operator : SY/MD
Sample : N2384-07DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6P8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025632.D
Acq On : 19 Apr 2022 16:24
Operator : SY/MD
Sample : N2384-07DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6P8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------