

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
 Data File : VV025633.D
 Acq On : 19 Apr 2022 16:47
 Operator : SY/MD
 Sample : N2384-20DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6S0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	18	22	31	rVB	6016	6160	1.12%	0.120%
2	1.311	76	84	98	rVB	102243	104092	18.86%	2.023%
3	1.571	157	165	175	rBV	98837	113089	20.50%	2.198%
4	2.111	321	333	348	rVB	178753	258201	46.79%	5.019%
5	2.513	447	458	469	rBV2	7948	13549	2.46%	0.263%
6	3.899	873	889	924	rBV3	53153	184646	33.46%	3.589%
7	4.352	1012	1030	1055	rBV	99813	251587	45.60%	4.890%
8	5.050	1230	1247	1280	rBV2	220002	551776	100.00%	10.725%
9	5.619	1411	1424	1447	rBV	195777	402741	72.99%	7.828%
10	5.915	1502	1516	1534	rBV7	7915	19072	3.46%	0.371%
11	6.069	1548	1564	1592	rBV2	128882	268978	48.75%	5.228%
12	6.989	1839	1850	1875	rBV	52752	102429	18.56%	1.991%
13	7.317	1939	1952	1972	rBV	260296	459581	83.29%	8.933%
14	7.625	2038	2048	2069	rBV	29535	55381	10.04%	1.076%
15	7.976	2137	2157	2176	rBV	263895	446128	80.85%	8.671%
16	8.088	2183	2192	2230	rBV	195361	393076	71.24%	7.640%
17	8.850	2416	2429	2456	rBV	322235	531058	96.25%	10.322%
18	10.214	2843	2853	2866	rBV	77639	124945	22.64%	2.429%
19	11.246	3164	3174	3193	rBV	312752	484602	87.83%	9.419%
20	11.622	3280	3291	3313	rBV	236776	373688	67.72%	7.263%




Sum of corrected areas: 5144779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025633.D
Acq On : 19 Apr 2022 16:47
Operator : SY/MD
Sample : N2384-20DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6S0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

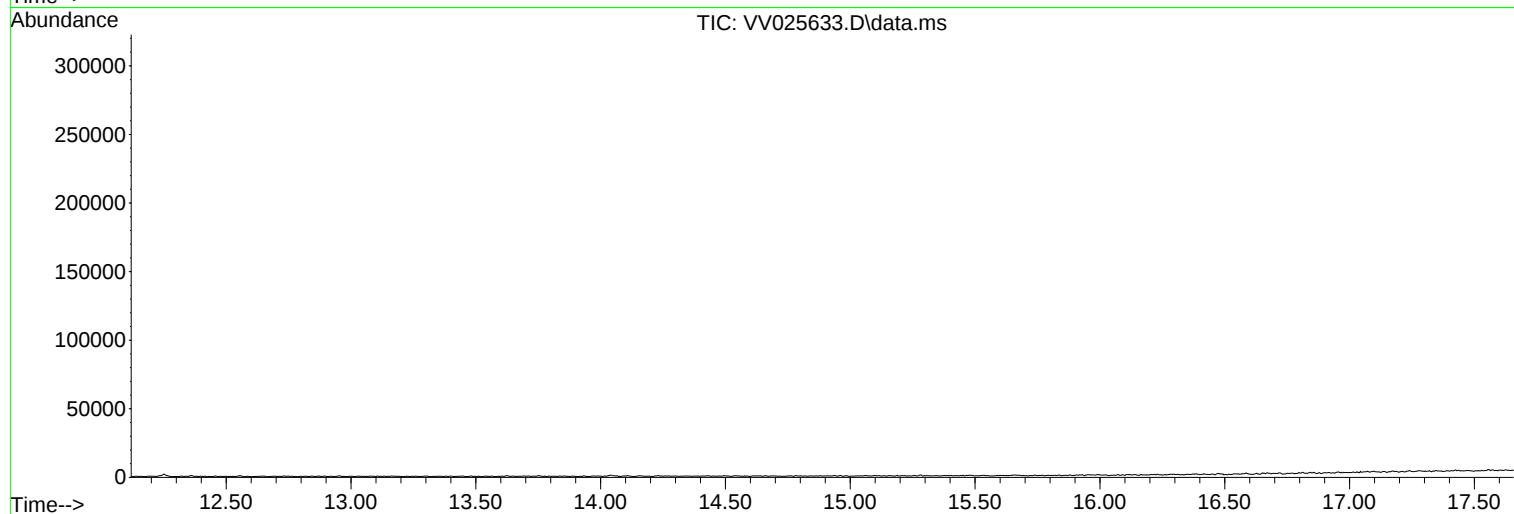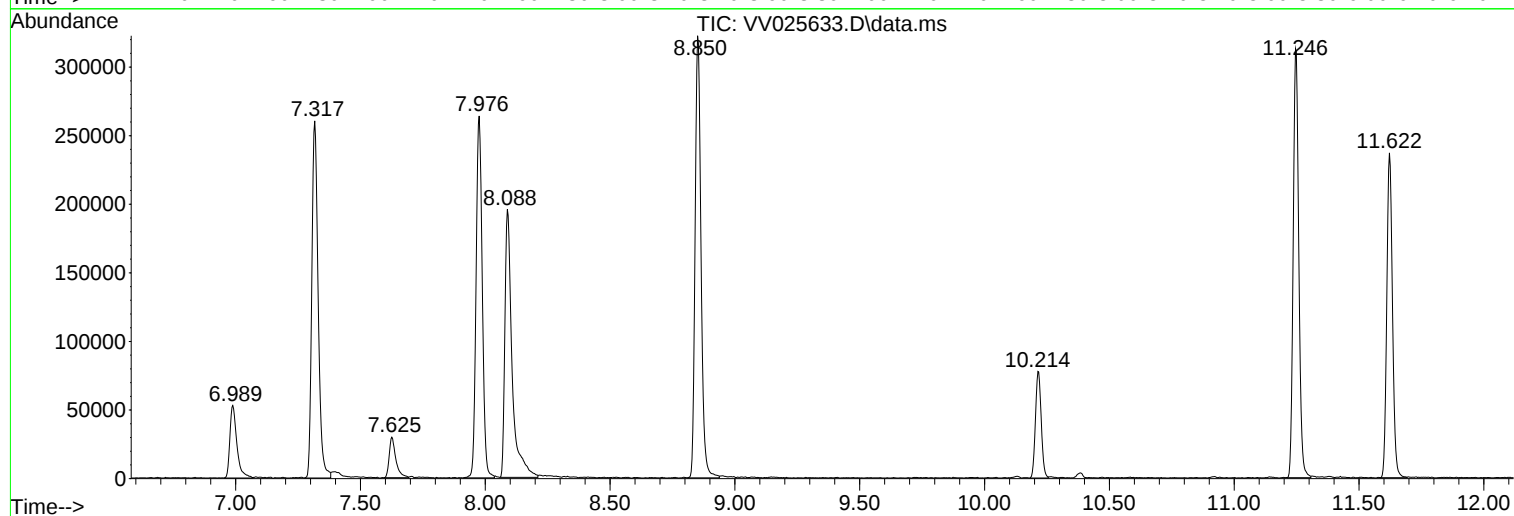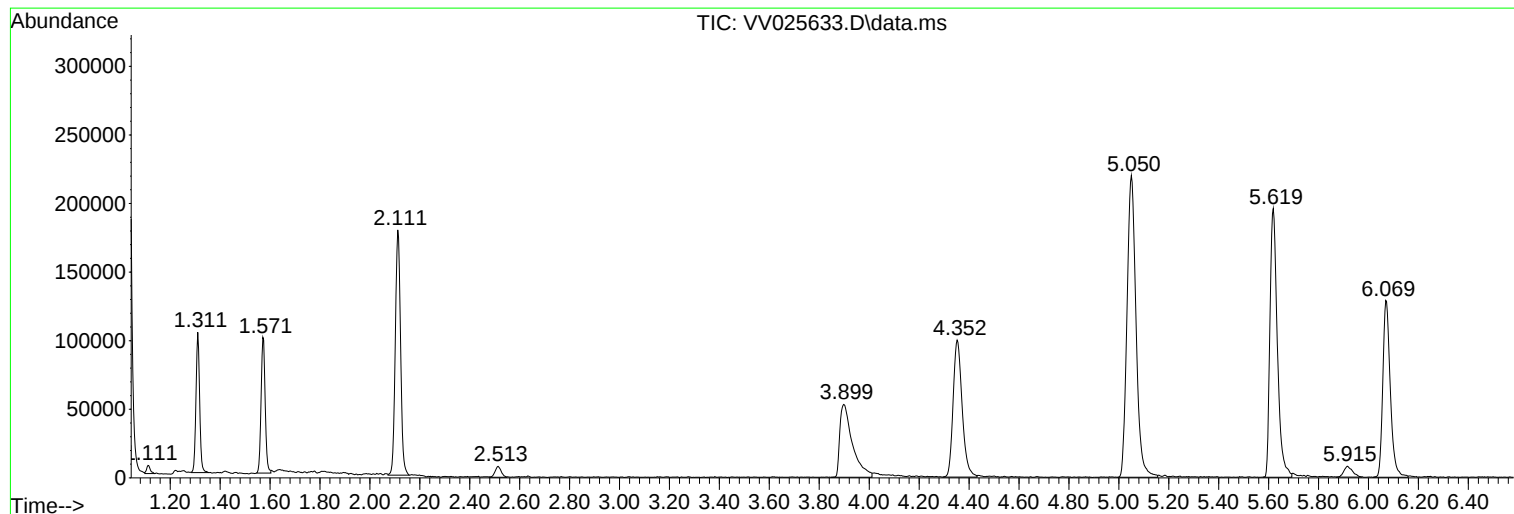

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025633.D
Acq On : 19 Apr 2022 16:47
Operator : SY/MD
Sample : N2384-20DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6S0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041922\
Data File : VV025633.D
Acq On : 19 Apr 2022 16:47
Operator : SY/MD
Sample : N2384-20DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6S0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc