

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041924\
 Data File : VW035301.D
 Acq On : 19 Apr 2024 12:36
 Operator : SY/MD
 Sample : P2157-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R91

Quant Time: Apr 19 22:30:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 19 22:28:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	428706	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	421300	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	178201	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	125757	30.374	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	60.740%		
7) Chloroethane-d5	1.532	69	112032	31.154	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	62.300%#		
11) 1,1-Dichloroethene-d2	2.060	65	55680	30.680	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	61.360%		
21) 2-Butanone-d5	3.789	46	193215	78.687	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	78.690%		
24) Chloroform-d	4.249	84	263774	37.893	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.780%		
26) 1,2-Dichloroethane-d4	4.941	65	170041	38.475	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	76.940%		
32) Benzene-d6	4.957	84	510603	36.081	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	72.160%		
36) 1,2-Dichloropropane-d6	5.985	67	171025	38.058	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	76.120%		
41) Toluene-d8	7.243	98	430387	33.770	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	67.540%#		
43) trans-1,3-Dichloroprop...	7.555	79	63083	28.875	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	57.760%#		
47) 2-Hexanone-d5	8.024	63	107045	63.003	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	63.000%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	244790	39.556	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	79.120%		
66) 1,2-Dichlorobenzene-d4	11.558	152	166282	41.560	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.120%		
Target Compounds					Qvalue	
13) Acetone	2.121	43	12615	5.596	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035301.D
Acq On : 19 Apr 2024 12:36
Operator : SY/MD
Sample : P2157-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R91

Quant Time: Apr 19 22:30:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 19 22:28:16 2024
Response via : Initial Calibration

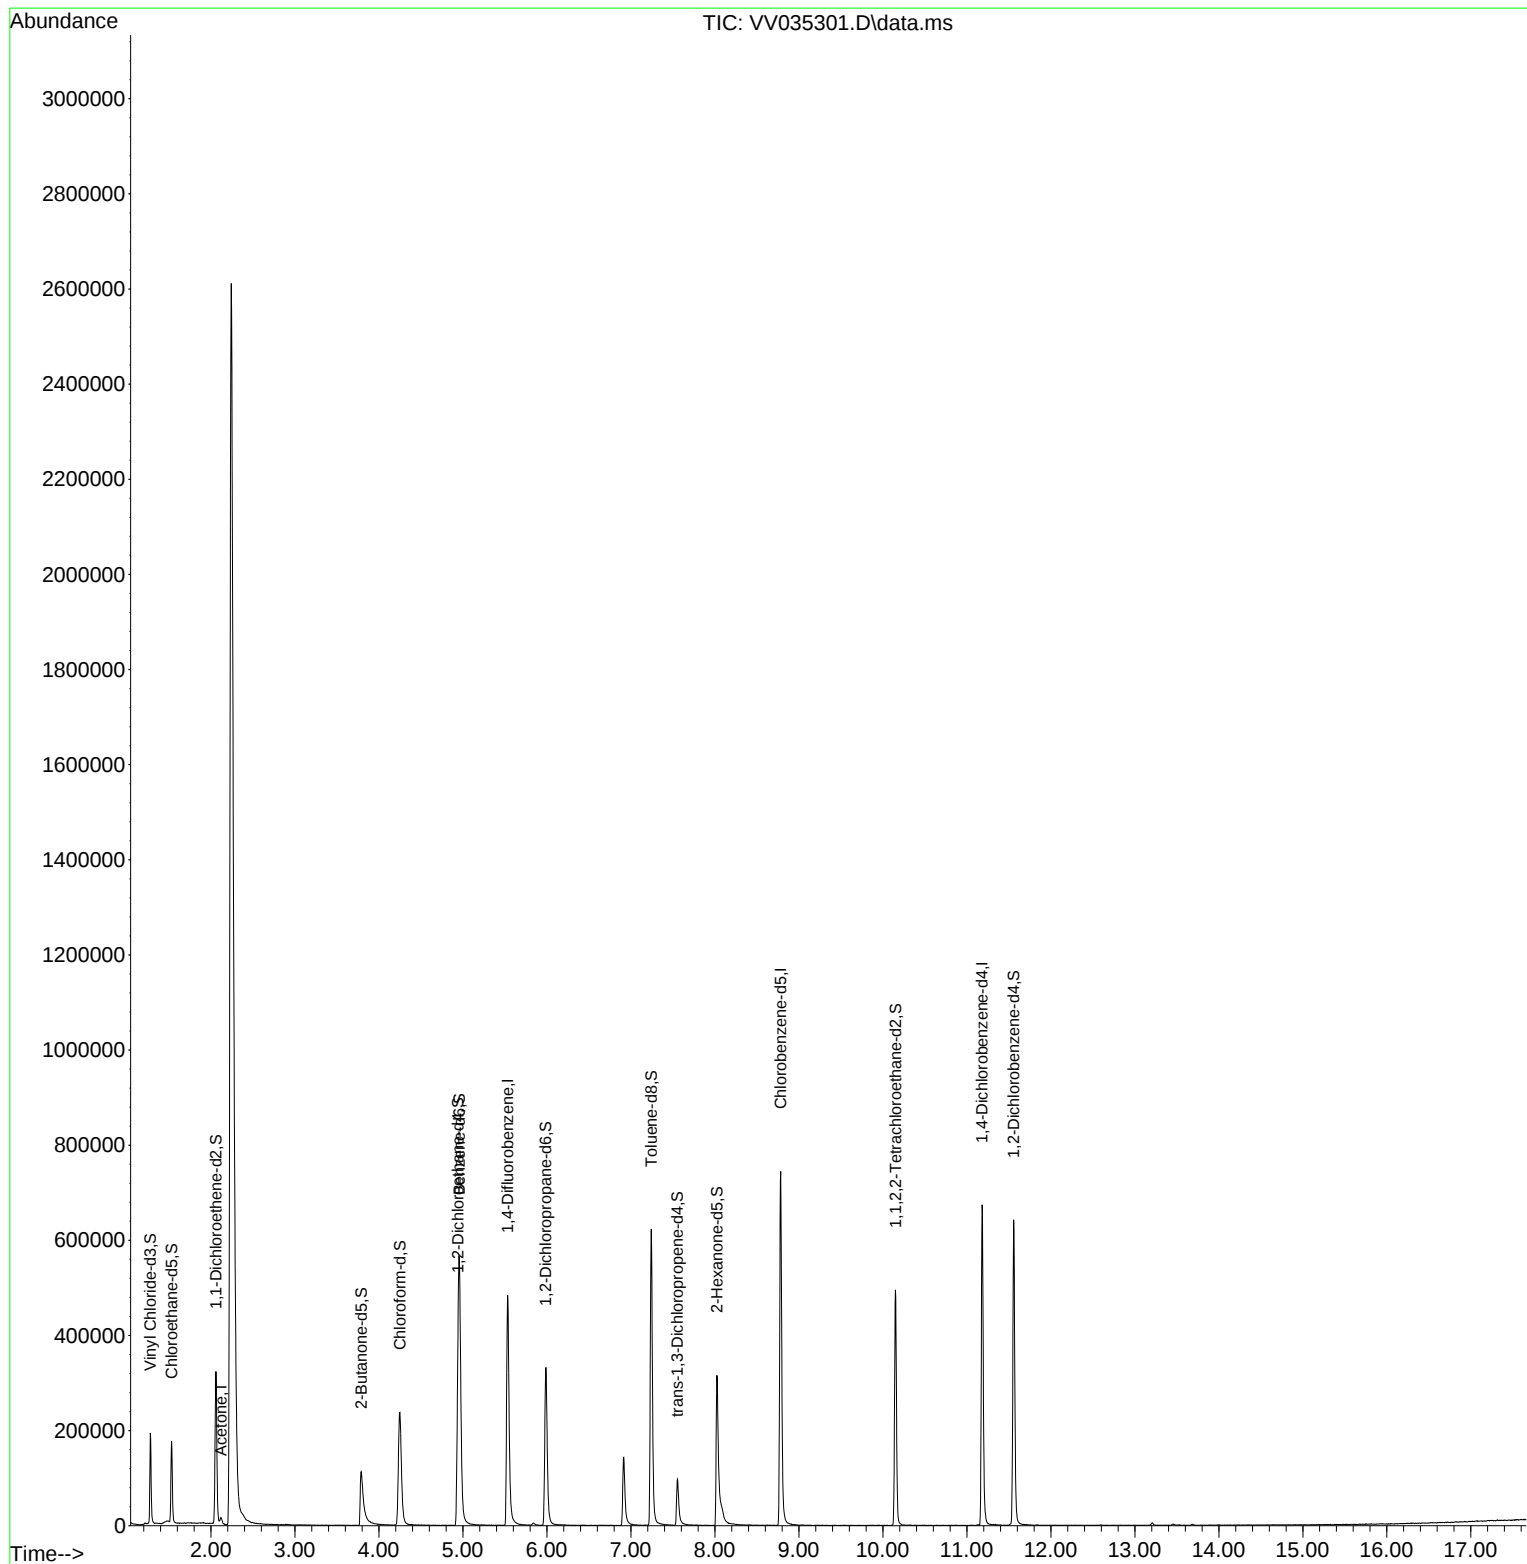

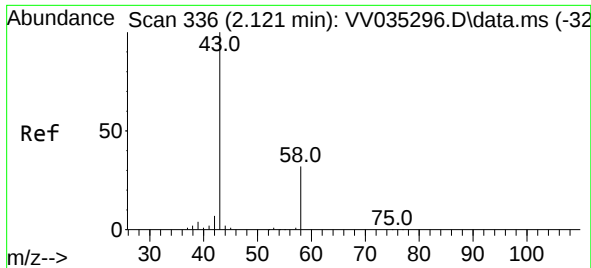

#13

Acetone

Concen: 5.596 ug/L

RT: 2.121 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV035301.D

Acq: 19 Apr 2024 12:36

Instrument :

MSVOA_V

ClientSampleId :

MC0R91

Tgt Ion: 43 Resp: 12615

Ion Ratio Lower Upper

43 100

58 34.3 0.0 66.0

