

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035297.D
 Acq On : 19 Apr 2024 10:56
 Operator : SY/MD
 Sample : VV0419WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035297.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	49	rBV	3936	3406	0.19%	0.026%
2	1.217	51	55	61	rVV2	3468	3893	0.22%	0.030%
3	1.278	67	74	91	rVB	222887	242081	13.66%	1.854%
4	1.526	144	151	171	rVB	212007	261106	14.73%	2.000%
5	2.056	306	316	332	rBV	374397	545132	30.76%	4.175%
6	2.445	428	437	448	rVB8	2422	4365	0.25%	0.033%
7	2.545	465	468	470	rBV3	483	344	0.02%	0.003%
8	2.696	509	515	516	rBV3	1657	1373	0.08%	0.011%
9	2.828	552	556	563	rVB2	318	308	0.02%	0.002%
10	2.937	585	590	591	rBV	407	365	0.02%	0.003%
11	2.976	599	602	605	rVB2	389	267	0.02%	0.002%
12	3.246	683	686	691	rVB	363	306	0.02%	0.002%
13	3.593	792	794	798	rBV2	364	284	0.02%	0.002%
14	3.789	846	855	901	rBV	127357	377489	21.30%	2.891%
15	4.162	966	971	973	rBV4	587	531	0.03%	0.004%
16	4.246	979	997	1035	rBV	280047	724500	40.87%	5.549%
17	4.477	1067	1069	1072	rBV3	448	256	0.01%	0.002%
18	4.609	1108	1110	1113	rVB2	550	353	0.02%	0.003%
19	4.760	1156	1157	1161	rVB2	505	261	0.01%	0.002%
20	4.828	1176	1178	1182	rBV	404	270	0.02%	0.002%
21	4.953	1200	1217	1258	rBV2	663509	1772489	100.00%	13.576%
22	5.239	1303	1306	1314	rVB5	855	926	0.05%	0.007%
23	5.275	1314	1317	1321	rVV5	605	514	0.03%	0.004%
24	5.326	1329	1333	1337	rVV5	423	459	0.03%	0.004%
25	5.349	1337	1340	1342	rVV4	606	442	0.02%	0.003%
26	5.375	1345	1348	1353	rVB3	814	540	0.03%	0.004%
27	5.426	1361	1364	1367	rBV3	503	403	0.02%	0.003%
28	5.532	1386	1397	1429	rBV	492136	1023578	57.75%	7.840%
29	5.838	1481	1492	1508	rBV7	7221	16936	0.96%	0.130%
30	5.985	1522	1538	1570	rBV	387703	820406	46.29%	6.284%
31	6.272	1623	1627	1632	rVB4	453	490	0.03%	0.004%
32	6.336	1644	1647	1650	rVB3	407	273	0.02%	0.002%
33	6.442	1675	1680	1682	rBV4	371	331	0.02%	0.003%
34	6.458	1682	1685	1690	rVB3	652	621	0.04%	0.005%
35	6.609	1725	1732	1734	rBV3	336	273	0.02%	0.002%
36	6.690	1753	1757	1759	rBV3	447	317	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035297.D
 Acq On : 19 Apr 2024 10:56
 Operator : SY/MD
 Sample : VV0419WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.702	1759	1761	1766	rVB3	542	425	0.02%	0.003%
38	6.764	1776	1780	1784	rVB3	347	300	0.02%	0.002%
39	6.911	1816	1826	1862	rBV	186182	370759	20.92%	2.840%
40	7.072	1873	1876	1883	rVB3	991	947	0.05%	0.007%
41	7.130	1892	1894	1896	rBV2	477	286	0.02%	0.002%
42	7.175	1905	1908	1910	rBV3	379	254	0.01%	0.002%
43	7.239	1917	1928	1971	rBV	728068	1312004	74.02%	10.049%
44	7.464	1996	1998	2003	rVB4	521	301	0.02%	0.002%
45	7.551	2016	2025	2047	rBV	129779	245991	13.88%	1.884%
46	7.844	2114	2116	2119	rBV2	394	282	0.02%	0.002%
47	7.911	2132	2137	2138	rBV3	1187	923	0.05%	0.007%
48	8.024	2163	2172	2216	rBV	381320	812171	45.82%	6.221%
49	8.358	2274	2276	2279	rBV3	500	302	0.02%	0.002%
50	8.522	2325	2327	2331	rVB3	517	328	0.02%	0.003%
51	8.689	2376	2379	2384	rVB4	322	340	0.02%	0.003%
52	8.722	2384	2389	2390	rBV2	415	300	0.02%	0.002%
53	8.783	2397	2408	2449	rBV	742637	1257835	70.96%	9.634%
54	8.960	2457	2463	2465	rBV6	1354	1546	0.09%	0.012%
55	9.095	2501	2505	2509	rVV5	983	955	0.05%	0.007%
56	9.162	2522	2526	2532	rBV4	594	575	0.03%	0.004%
57	9.435	2605	2611	2614	rBV3	415	414	0.02%	0.003%
58	9.493	2622	2629	2634	rBV2	1623	2122	0.12%	0.016%
59	9.873	2742	2747	2749	rBV2	880	867	0.05%	0.007%
60	10.017	2789	2792	2796	rVB2	480	263	0.01%	0.002%
61	10.149	2820	2833	2864	rBV	573080	909712	51.32%	6.968%
62	10.259	2865	2867	2872	rVB4	589	537	0.03%	0.004%
63	10.416	2912	2916	2918	rBV2	471	276	0.02%	0.002%
64	10.461	2925	2930	2931	rBV	381	272	0.02%	0.002%
65	10.477	2931	2935	2938	rBV3	912	827	0.05%	0.006%
66	10.545	2954	2956	2961	rVB2	537	346	0.02%	0.003%
67	10.599	2969	2973	2977	rBV2	476	440	0.02%	0.003%
68	10.821	3036	3042	3043	rBV	339	291	0.02%	0.002%
69	10.860	3048	3054	3067	rVB4	1353	2162	0.12%	0.017%
70	11.127	3131	3137	3144	rBV6	3977	6330	0.36%	0.048%
71	11.181	3144	3154	3188	rVV	647279	1047199	59.08%	8.021%
72	11.377	3213	3215	3222	rVB3	517	449	0.03%	0.003%
73	11.406	3222	3224	3229	rVB2	436	321	0.02%	0.002%
74	11.558	3258	3271	3299	rBV	713185	1158115	65.34%	8.870%
75	11.767	3334	3336	3344	rVB4	656	532	0.03%	0.004%
76	11.869	3366	3368	3371	rBV	444	258	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035297.D
 Acq On : 19 Apr 2024 10:56
 Operator : SY/MD
 Sample : VV0419WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.156	3452	3457	3461	rBV2	363	359	0.02%	0.003%
78	12.191	3465	3468	3472	rVB4	496	396	0.02%	0.003%
79	12.249	3482	3486	3489	rVB3	450	355	0.02%	0.003%
80	12.374	3520	3525	3529	rBV5	666	739	0.04%	0.006%
81	12.442	3542	3546	3550	rBV2	305	287	0.02%	0.002%
82	12.522	3566	3571	3573	rBV3	359	300	0.02%	0.002%
83	12.590	3584	3592	3603	rBV6	3887	6475	0.37%	0.050%
84	12.670	3614	3617	3620	rBV	496	414	0.02%	0.003%
85	12.824	3663	3665	3669	rBV2	360	311	0.02%	0.002%
86	12.905	3687	3690	3694	rVB2	410	306	0.02%	0.002%
87	12.988	3712	3716	3720	rBV2	369	343	0.02%	0.003%
88	13.107	3749	3753	3756	rVB4	348	312	0.02%	0.002%
89	13.204	3773	3783	3794	rBV2	13892	21762	1.23%	0.167%
90	13.310	3810	3816	3819	rBV4	324	445	0.03%	0.003%
91	13.442	3846	3857	3872	rBV	31885	56268	3.17%	0.431%
92	13.641	3916	3919	3923	rBV2	425	415	0.02%	0.003%
93	13.683	3923	3932	3946	rVV4	11217	18767	1.06%	0.144%
94	13.895	3995	3998	4003	rBV4	512	429	0.02%	0.003%
95	14.310	4121	4127	4130	rBV4	558	654	0.04%	0.005%
96	14.400	4151	4155	4157	rBV2	648	513	0.03%	0.004%
97	14.538	4195	4198	4200	rBV3	641	458	0.03%	0.004%
98	14.619	4220	4223	4224	rBV	508	300	0.02%	0.002%
99	14.728	4255	4257	4261	rVB4	586	268	0.02%	0.002%
100	15.033	4349	4352	4354	rBV3	639	509	0.03%	0.004%




Sum of corrected areas: 13055830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035297.D
Acq On : 19 Apr 2024 10:56
Operator : SY/MD
Sample : VV0419WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

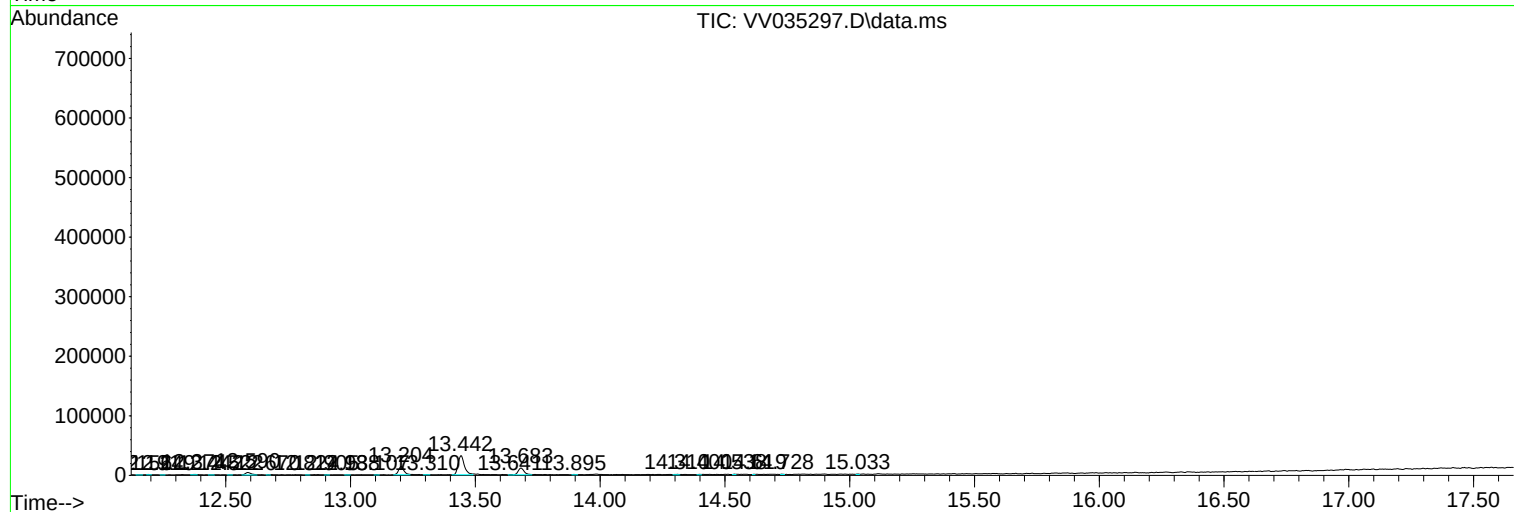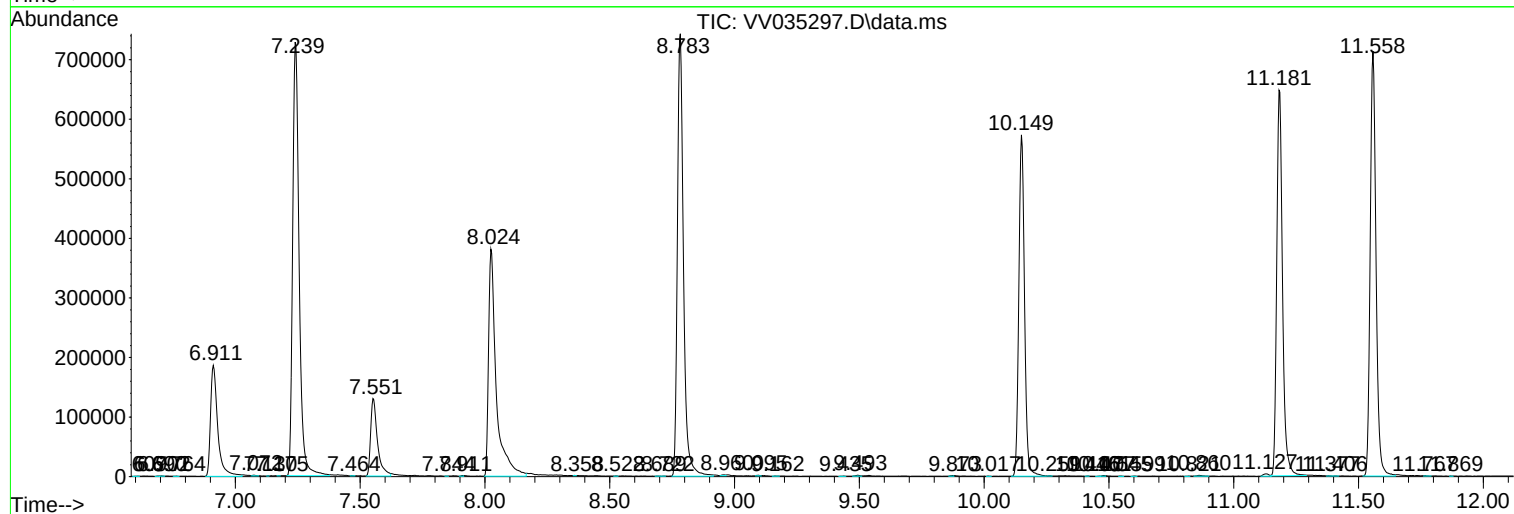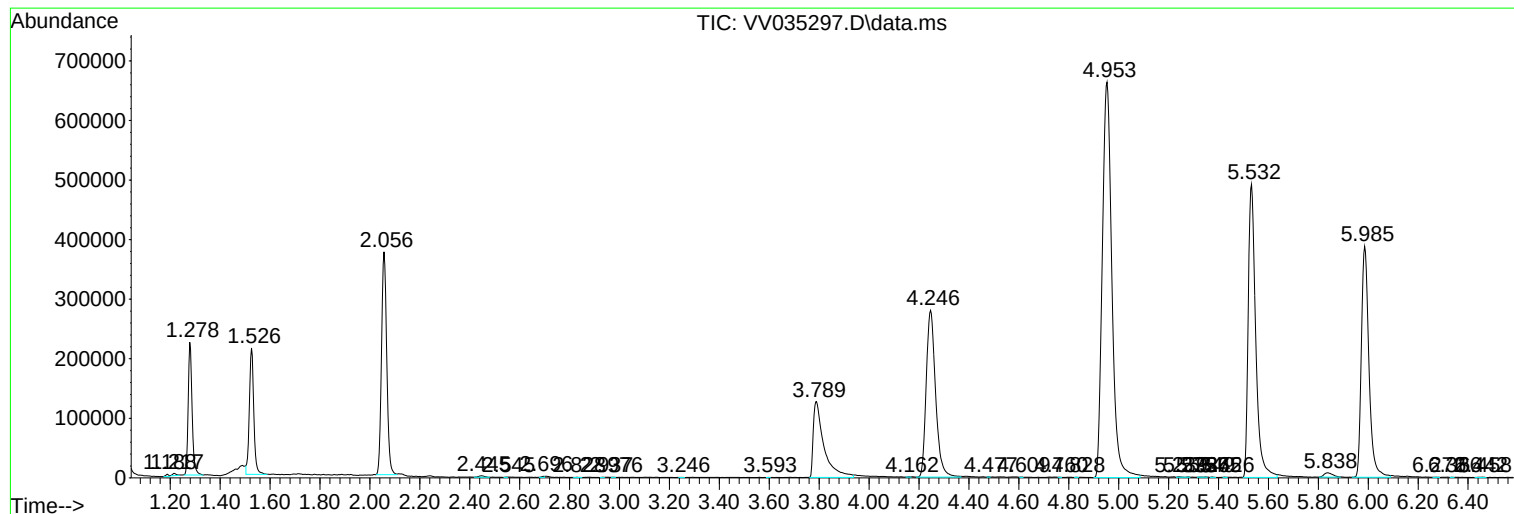

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035297.D
Acq On : 19 Apr 2024 10:56
Operator : SY/MD
Sample : VV0419WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035297.D
Acq On : 19 Apr 2024 10:56
Operator : SY/MD
Sample : VV0419WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------