

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035298.D
 Acq On : 19 Apr 2024 11:19
 Operator : SY/MD
 Sample : VV0419WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK271

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035298.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	228555	247777	14.49%	2.098%
2	1.526	145	151	167	rVB	204588	247401	14.47%	2.095%
3	2.056	307	316	333	rVB	379952	544374	31.84%	4.610%
4	2.446	428	437	449	rBV8	2410	4481	0.26%	0.038%
5	2.864	564	567	571	rBV2	417	308	0.02%	0.003%
6	2.883	571	573	576	rBV2	287	210	0.01%	0.002%
7	3.073	630	632	634	rVB	232	124	0.01%	0.001%
8	3.220	673	678	680	rBV2	315	337	0.02%	0.003%
9	3.288	697	699	705	rVB2	186	183	0.01%	0.002%
10	3.327	707	711	714	rBV3	352	316	0.02%	0.003%
11	3.410	733	737	738	rBV2	206	130	0.01%	0.001%
12	3.445	743	748	750	rBV	205	152	0.01%	0.001%
13	3.510	766	768	770	rBV2	247	128	0.01%	0.001%
14	3.536	773	776	780	rVB2	216	213	0.01%	0.002%
15	3.661	813	815	818	rBV	188	128	0.01%	0.001%
16	3.725	831	835	837	rBV	305	175	0.01%	0.001%
17	3.757	842	845	847	rBV	289	251	0.01%	0.002%
18	3.790	847	855	898	rBV	113949	341402	19.97%	2.891%
19	4.246	982	997	1032	rBV	265096	677966	39.65%	5.741%
20	4.478	1066	1069	1072	rBV4	497	371	0.02%	0.003%
21	4.728	1145	1147	1150	rBV3	287	175	0.01%	0.001%
22	4.757	1152	1156	1159	rVB4	465	382	0.02%	0.003%
23	4.773	1159	1161	1166	rBV2	368	326	0.02%	0.003%
24	4.812	1170	1173	1175	rBV2	452	278	0.02%	0.002%
25	4.953	1201	1217	1253	rBV2	650089	1709667	100.00%	14.477%
26	5.301	1323	1325	1326	rBV	355	122	0.01%	0.001%
27	5.532	1386	1397	1424	rBV	392498	825152	48.26%	6.987%
28	5.986	1525	1538	1566	rBV	373946	777160	45.46%	6.581%
29	6.269	1624	1626	1627	rBV	350	102	0.01%	0.001%
30	6.320	1640	1642	1645	rBV2	444	249	0.01%	0.002%
31	6.336	1645	1647	1649	rBV2	308	108	0.01%	0.001%
32	6.368	1653	1657	1662	rBV4	369	349	0.02%	0.003%
33	6.397	1662	1666	1671	rVB5	562	605	0.04%	0.005%
34	6.429	1674	1676	1678	rBV	245	131	0.01%	0.001%
35	6.442	1678	1680	1681	rBV	319	141	0.01%	0.001%
36	6.478	1689	1691	1692	rBV	332	128	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035298.D
 Acq On : 19 Apr 2024 11:19
 Operator : SY/MD
 Sample : VV0419WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK271

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.558	1714	1716	1719	rVB	255	103	0.01%	0.001%
38	6.596	1722	1728	1730	rBV2	271	239	0.01%	0.002%
39	6.648	1742	1744	1746	rVV2	357	159	0.01%	0.001%
40	6.664	1746	1749	1752	rVB3	298	190	0.01%	0.002%
41	6.687	1753	1756	1760	rVV2	315	213	0.01%	0.002%
42	6.825	1795	1799	1801	rBV2	354	193	0.01%	0.002%
43	6.912	1816	1826	1853	rBV	166744	328717	19.23%	2.784%
44	7.240	1918	1928	1958	rBV	716496	1280438	74.89%	10.842%
45	7.551	2016	2025	2053	rBV2	112493	218525	12.78%	1.850%
46	7.725	2077	2079	2082	rVB3	844	447	0.03%	0.004%
47	7.863	2119	2122	2124	rBV2	427	233	0.01%	0.002%
48	7.960	2150	2152	2154	rBV2	269	123	0.01%	0.001%
49	8.024	2164	2172	2215	rBV	326139	723608	42.32%	6.127%
50	8.683	2375	2377	2380	rVB2	330	140	0.01%	0.001%
51	8.722	2384	2389	2392	rVB3	532	393	0.02%	0.003%
52	8.738	2392	2394	2396	rBV	268	140	0.01%	0.001%
53	8.783	2397	2408	2448	rBV	609183	1028013	60.13%	8.705%
54	9.069	2493	2497	2498	rBV2	681	345	0.02%	0.003%
55	9.137	2516	2518	2520	rBV	280	154	0.01%	0.001%
56	9.201	2536	2538	2540	rVB2	437	180	0.01%	0.002%
57	9.262	2552	2557	2558	rBV	294	244	0.01%	0.002%
58	9.307	2567	2571	2572	rBV2	243	186	0.01%	0.002%
59	9.339	2578	2581	2582	rBV	383	153	0.01%	0.001%
60	9.358	2584	2587	2589	rVV	480	236	0.01%	0.002%
61	9.407	2600	2602	2606	rVB2	295	184	0.01%	0.002%
62	9.442	2610	2613	2614	rBV2	283	127	0.01%	0.001%
63	9.477	2619	2624	2626	rBV3	310	260	0.02%	0.002%
64	9.490	2626	2628	2629	rBV	327	113	0.01%	0.001%
65	9.532	2639	2641	2642	rBV2	493	190	0.01%	0.002%
66	9.584	2655	2657	2661	rBV	139	121	0.01%	0.001%
67	9.603	2661	2663	2665	rVV	276	128	0.01%	0.001%
68	9.622	2667	2669	2672	rVB2	332	171	0.01%	0.001%
69	9.638	2672	2674	2677	rVB	219	132	0.01%	0.001%
70	9.805	2724	2726	2728	rBV2	233	103	0.01%	0.001%
71	9.847	2735	2739	2741	rBV2	194	156	0.01%	0.001%
72	9.863	2741	2744	2746	rBV2	390	301	0.02%	0.003%
73	9.947	2768	2770	2775	rVB	479	273	0.02%	0.002%
74	9.979	2775	2780	2784	rBV3	395	433	0.03%	0.004%
75	10.008	2785	2789	2792	rVV3	276	210	0.01%	0.002%
76	10.149	2821	2833	2850	rBV	524612	825461	48.28%	6.990%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035298.D
 Acq On : 19 Apr 2024 11:19
 Operator : SY/MD
 Sample : VV0419WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK271

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.403	2910	2912	2916	rBV3	218	176	0.01%	0.001%
78	10.477	2932	2935	2937	rBV	308	213	0.01%	0.002%
79	10.522	2946	2949	2950	rBV	258	119	0.01%	0.001%
80	10.773	3024	3027	3030	rBV	352	222	0.01%	0.002%
81	10.789	3030	3032	3034	rBV	405	209	0.01%	0.002%
82	10.841	3046	3048	3049	rBV	255	126	0.01%	0.001%
83	10.934	3073	3077	3080	rBV	337	323	0.02%	0.003%
84	10.995	3090	3096	3100	rBV3	610	642	0.04%	0.005%
85	11.053	3112	3114	3116	rBV	350	167	0.01%	0.001%
86	11.130	3131	3138	3141	rBV6	2237	2529	0.15%	0.021%
87	11.185	3144	3155	3191	rVV	537458	866234	50.67%	7.335%
88	11.558	3259	3271	3293	rBV	682822	1101765	64.44%	9.330%
89	11.947	3388	3392	3396	rBV3	379	391	0.02%	0.003%
90	12.056	3422	3426	3429	rBV2	619	561	0.03%	0.005%
91	12.130	3447	3449	3450	rBV	264	112	0.01%	0.001%
92	12.275	3492	3494	3497	rBV2	309	241	0.01%	0.002%
93	12.548	3577	3579	3580	rBV2	417	233	0.01%	0.002%
94	12.709	3625	3629	3631	rBV3	354	200	0.01%	0.002%
95	12.857	3673	3675	3677	rBV3	395	169	0.01%	0.001%
96	12.937	3698	3700	3703	rBV	247	157	0.01%	0.001%
97	12.982	3712	3714	3716	rBV2	270	115	0.01%	0.001%
98	13.204	3775	3783	3804	rVB4	7332	13596	0.80%	0.115%
99	13.445	3851	3858	3873	rVB2	12138	19688	1.15%	0.167%
100	13.683	3926	3932	3946	rVB4	5354	8045	0.47%	0.068%




Sum of corrected areas: 11809470

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035298.D
Acq On : 19 Apr 2024 11:19
Operator : SY/MD
Sample : VV0419WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

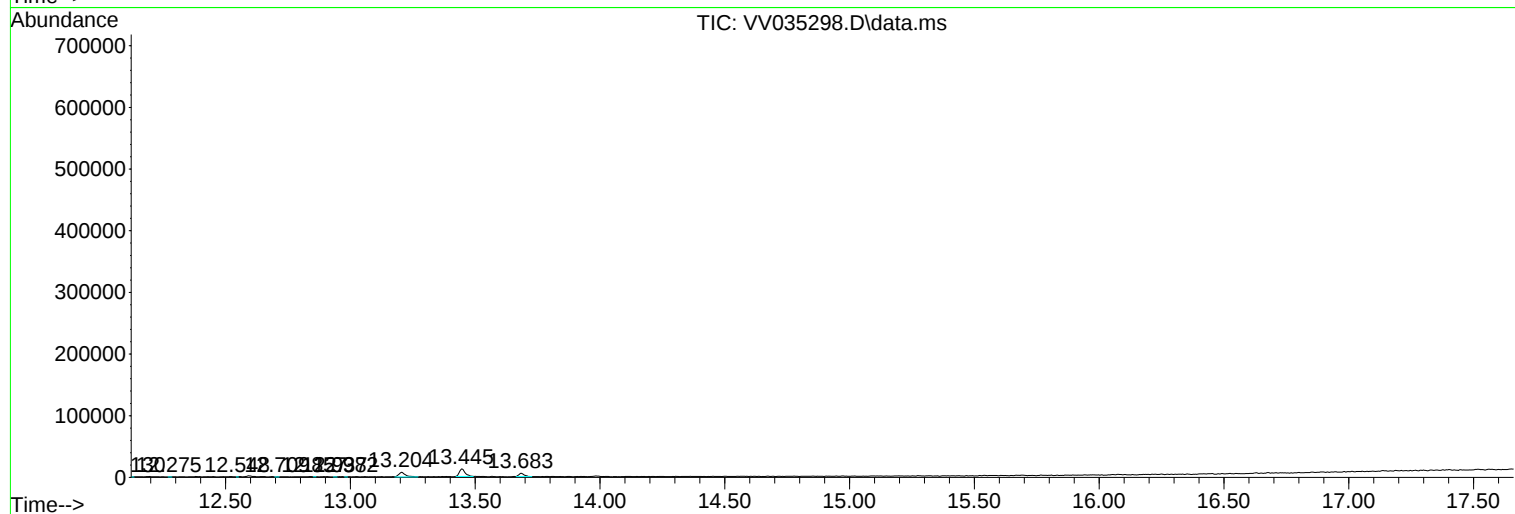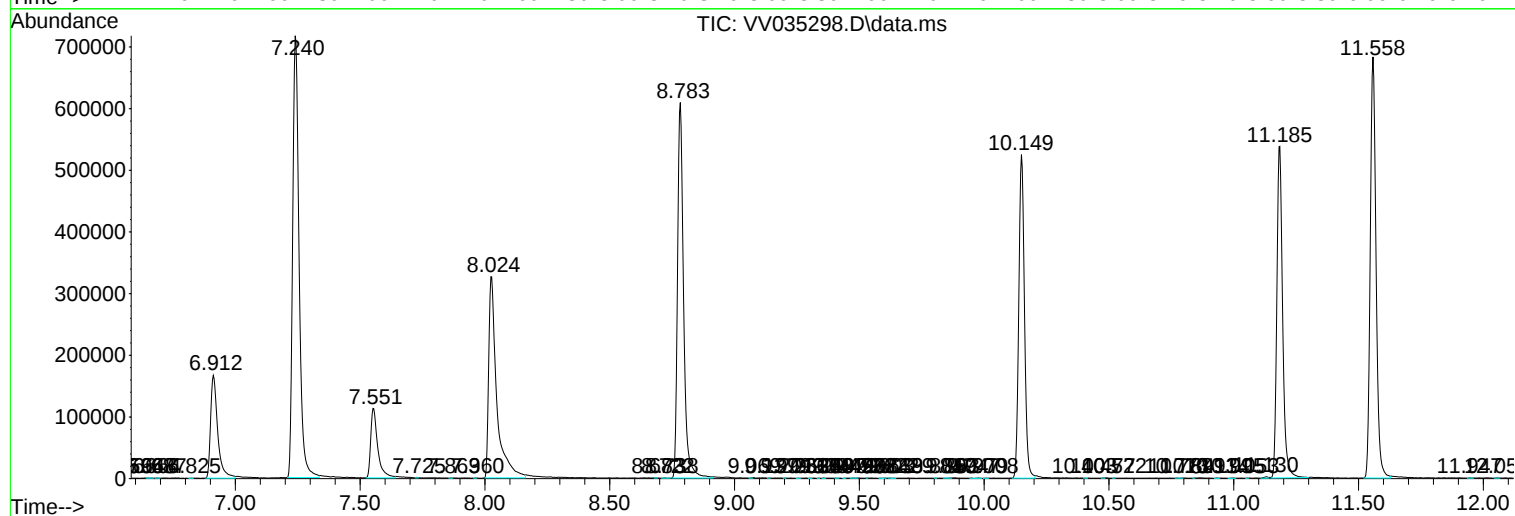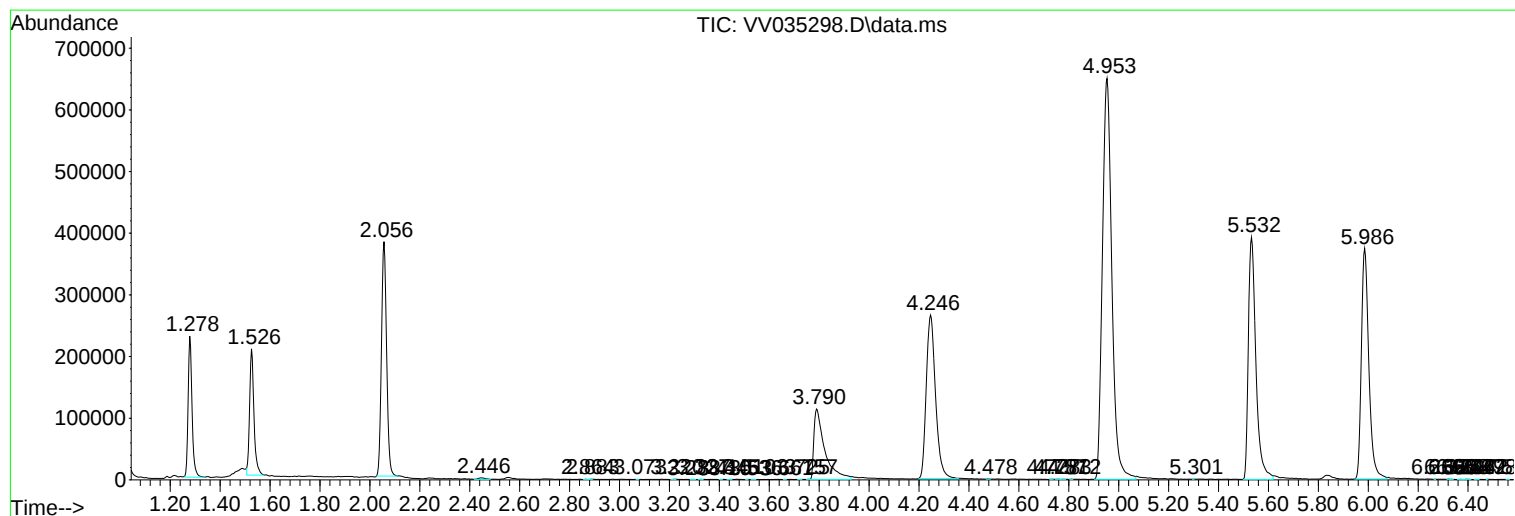

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035298.D
Acq On : 19 Apr 2024 11:19
Operator : SY/MD
Sample : VV0419WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035298.D
Acq On : 19 Apr 2024 11:19
Operator : SY/MD
Sample : VV0419WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------