

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035299.D
 Acq On : 19 Apr 2024 11:49
 Operator : SY/MD
 Sample : P2158-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	202969	222520	14.11%	2.029%
2	1.526	146	151	177	rVB	180124	231907	14.70%	2.115%
3	2.056	306	316	331	rBV	343251	498289	31.59%	4.544%
4	2.445	432	437	448	rVB5	2124	3086	0.20%	0.028%
5	2.748	528	531	533	rBV	229	167	0.01%	0.002%
6	2.793	543	545	547	rBV	253	118	0.01%	0.001%
7	2.822	550	554	556	rBV2	358	303	0.02%	0.003%
8	2.847	560	562	565	rBV2	264	141	0.01%	0.001%
9	2.944	589	592	595	rBV2	230	190	0.01%	0.002%
10	2.982	602	604	607	rBV	328	179	0.01%	0.002%
11	3.037	617	621	623	rBV2	320	182	0.01%	0.002%
12	3.053	623	626	629	rVB	280	143	0.01%	0.001%
13	3.076	631	633	635	rVB	334	144	0.01%	0.001%
14	3.098	637	640	642	rBV	393	246	0.02%	0.002%
15	3.172	661	663	666	rBV2	225	92	0.01%	0.001%
16	3.198	668	671	674	rBV	231	200	0.01%	0.002%
17	3.246	682	686	687	rBV2	285	188	0.01%	0.002%
18	3.342	713	716	717	rBV	303	149	0.01%	0.001%
19	3.407	733	736	740	rBV2	198	153	0.01%	0.001%
20	3.426	740	742	747	rVB2	219	157	0.01%	0.001%
21	3.474	756	757	759	rBV	202	100	0.01%	0.001%
22	3.526	771	773	777	rVB2	316	230	0.01%	0.002%
23	3.545	777	779	780	rBV2	184	78	0.00%	0.001%
24	3.580	788	790	795	rBV2	132	119	0.01%	0.001%
25	3.613	798	800	802	rBV	153	98	0.01%	0.001%
26	3.648	809	811	813	rVB	292	110	0.01%	0.001%
27	3.789	847	855	901	rBV	105369	329124	20.87%	3.002%
28	4.243	981	996	1032	rBV	244573	637996	40.45%	5.819%
29	4.728	1139	1147	1148	rBV3	1742	1875	0.12%	0.017%
30	4.863	1186	1189	1194	rBV3	324	309	0.02%	0.003%
31	4.950	1200	1216	1252	rBV2	592380	1577369	100.00%	14.386%
32	5.471	1375	1378	1380	rBV2	608	390	0.02%	0.004%
33	5.532	1386	1397	1428	rBV	353738	753076	47.74%	6.868%
34	5.834	1481	1491	1513	rVB2	7186	17036	1.08%	0.155%
35	5.985	1525	1538	1568	rBV	342447	727325	46.11%	6.633%
36	6.313	1638	1640	1643	rBV2	244	157	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035299.D
 Acq On : 19 Apr 2024 11:49
 Operator : SY/MD
 Sample : P2158-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.365	1654	1656	1657	rBV2	409	137	0.01%	0.001%
38	6.403	1665	1668	1673	rBV4	418	321	0.02%	0.003%
39	6.500	1696	1698	1701	rVB2	159	76	0.00%	0.001%
40	6.519	1701	1704	1709	rBV2	240	224	0.01%	0.002%
41	6.542	1709	1711	1717	rVB2	135	81	0.01%	0.001%
42	6.612	1729	1733	1738	rBV2	598	497	0.03%	0.005%
43	6.780	1781	1785	1790	rBV4	295	357	0.02%	0.003%
44	6.834	1800	1802	1806	rVB2	202	113	0.01%	0.001%
45	6.876	1811	1815	1816	rBV	164	119	0.01%	0.001%
46	6.911	1816	1826	1857	rBV	153897	305131	19.34%	2.783%
47	7.159	1898	1903	1904	rBV5	697	615	0.04%	0.006%
48	7.239	1917	1928	1958	rBV	648332	1164365	73.82%	10.619%
49	7.551	2016	2025	2053	rBV	106499	204890	12.99%	1.869%
50	7.866	2116	2123	2125	rBV2	599	549	0.03%	0.005%
51	7.911	2132	2137	2142	rVB4	1065	1264	0.08%	0.012%
52	7.989	2159	2161	2163	rBV	242	116	0.01%	0.001%
53	8.027	2164	2173	2222	rVV2	303830	699864	44.37%	6.383%
54	8.596	2348	2350	2354	rVB2	578	309	0.02%	0.003%
55	8.616	2354	2356	2358	rBV3	219	123	0.01%	0.001%
56	8.667	2370	2372	2376	rBV2	272	172	0.01%	0.002%
57	8.693	2378	2380	2382	rVB2	406	151	0.01%	0.001%
58	8.706	2382	2384	2385	rBV	262	123	0.01%	0.001%
59	8.783	2397	2408	2438	rBV	551100	936153	59.35%	8.538%
60	9.082	2499	2501	2502	rBV	308	118	0.01%	0.001%
61	9.149	2520	2522	2528	rVB2	412	309	0.02%	0.003%
62	9.185	2529	2533	2536	rBV	212	213	0.01%	0.002%
63	9.284	2562	2564	2567	rBV3	286	195	0.01%	0.002%
64	9.320	2573	2575	2578	rBV	233	144	0.01%	0.001%
65	9.345	2578	2583	2586	rBV3	506	401	0.03%	0.004%
66	9.381	2592	2594	2599	rVB	398	275	0.02%	0.003%
67	9.419	2599	2606	2608	rBV2	265	327	0.02%	0.003%
68	9.458	2615	2618	2619	rBV	149	83	0.01%	0.001%
69	9.464	2619	2620	2622	rVB	262	101	0.01%	0.001%
70	9.493	2622	2629	2631	rBV4	530	584	0.04%	0.005%
71	9.538	2641	2643	2644	rBV4	259	116	0.01%	0.001%
72	9.571	2651	2653	2656	rBV	194	113	0.01%	0.001%
73	9.632	2668	2672	2673	rBV	218	156	0.01%	0.001%
74	9.680	2683	2687	2691	rVB	372	224	0.01%	0.002%
75	9.702	2692	2694	2698	rBV2	179	71	0.00%	0.001%
76	9.763	2709	2713	2717	rBV2	403	263	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035299.D
 Acq On : 19 Apr 2024 11:49
 Operator : SY/MD
 Sample : P2158-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.969	2776	2777	2782	rBV2	147	82	0.01%	0.001%
78	10.005	2786	2788	2791	rBV	205	92	0.01%	0.001%
79	10.149	2821	2833	2860	rBV	500783	784930	49.76%	7.159%
80	10.307	2880	2882	2885	rBV	362	240	0.02%	0.002%
81	10.371	2900	2902	2906	rBV2	322	157	0.01%	0.001%
82	10.616	2974	2978	2979	rBV	384	241	0.02%	0.002%
83	10.670	2991	2995	2996	rBV	346	241	0.02%	0.002%
84	10.722	3008	3011	3014	rBV2	382	295	0.02%	0.003%
85	10.773	3024	3027	3028	rBV2	394	176	0.01%	0.002%
86	10.808	3036	3038	3041	rBV2	194	78	0.00%	0.001%
87	11.130	3132	3138	3144	rBV5	2471	3295	0.21%	0.030%
88	11.185	3144	3155	3178	rBV	489046	796360	50.49%	7.263%
89	11.429	3229	3231	3233	rVB2	655	304	0.02%	0.003%
90	11.487	3246	3249	3253	rBV2	430	376	0.02%	0.003%
91	11.558	3260	3271	3302	rBV	624935	1013015	64.22%	9.239%
92	11.837	3355	3358	3360	rBV2	424	347	0.02%	0.003%
93	12.127	3445	3448	3452	rVB2	447	328	0.02%	0.003%
94	12.590	3583	3592	3599	rBV5	3273	5260	0.33%	0.048%
95	12.625	3601	3603	3605	rBV2	447	210	0.01%	0.002%
96	13.014	3722	3724	3727	rBV	357	165	0.01%	0.002%
97	13.056	3735	3737	3740	rVB	465	205	0.01%	0.002%
98	13.204	3773	3783	3794	rBV4	8260	14475	0.92%	0.132%
99	13.448	3852	3859	3876	rVB2	6301	11556	0.73%	0.105%
100	13.683	3925	3932	3946	rVB3	5243	8910	0.56%	0.081%




Sum of corrected areas: 10964727

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035299.D
Acq On : 19 Apr 2024 11:49
Operator : SY/MD
Sample : P2158-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

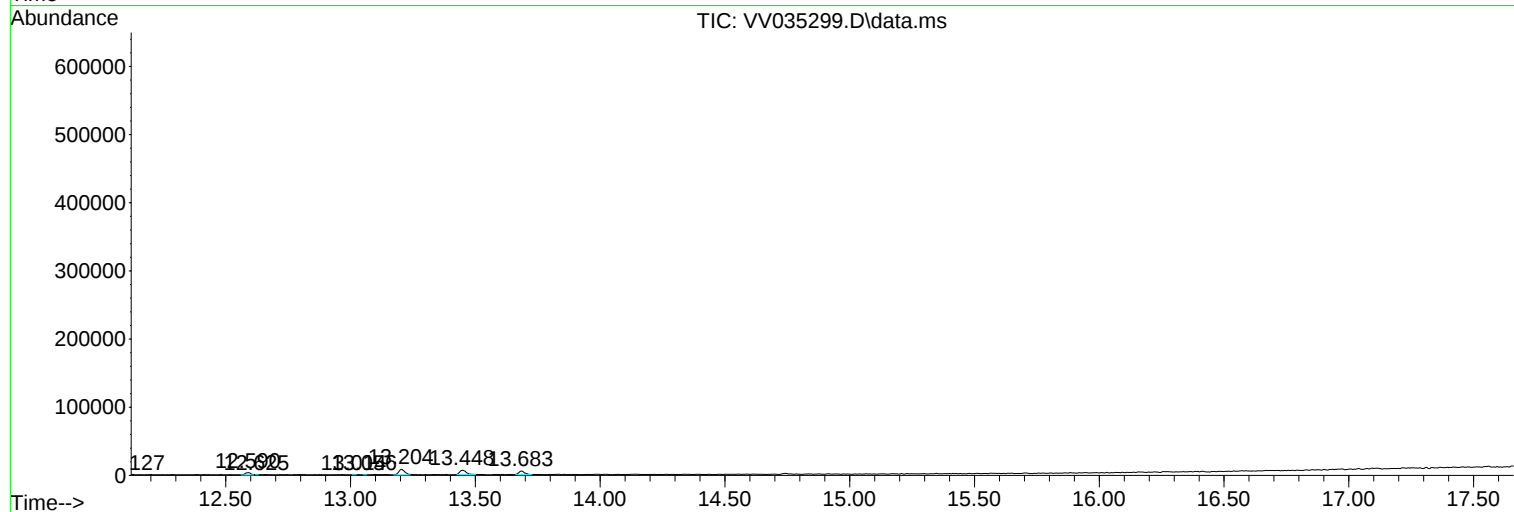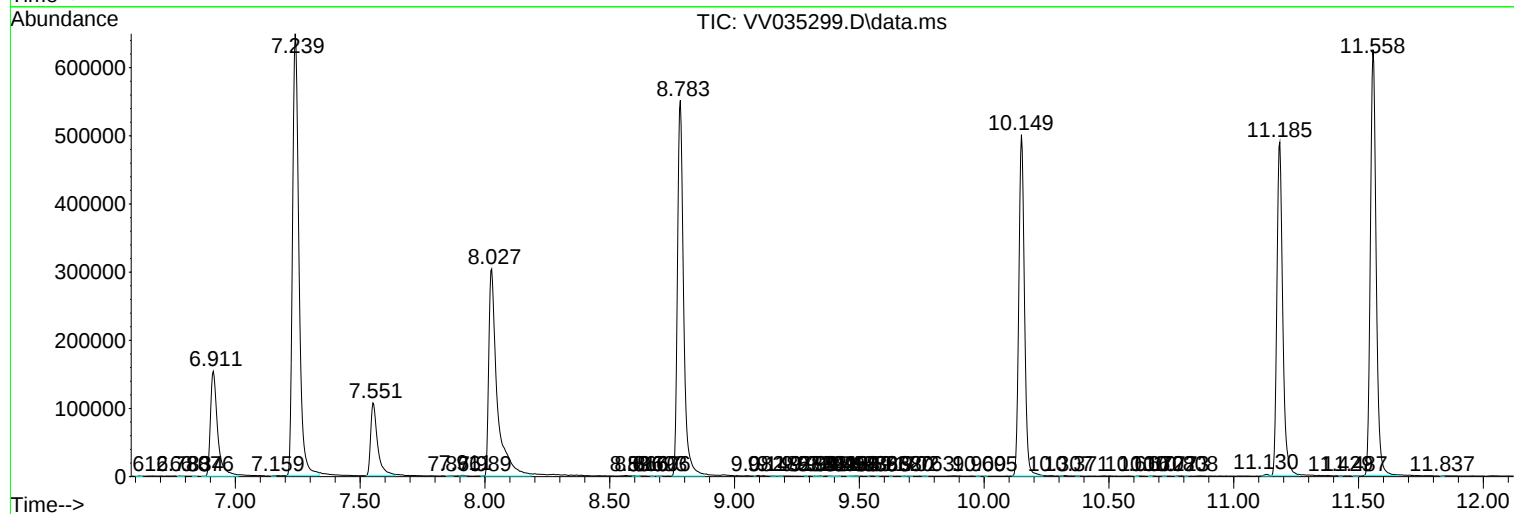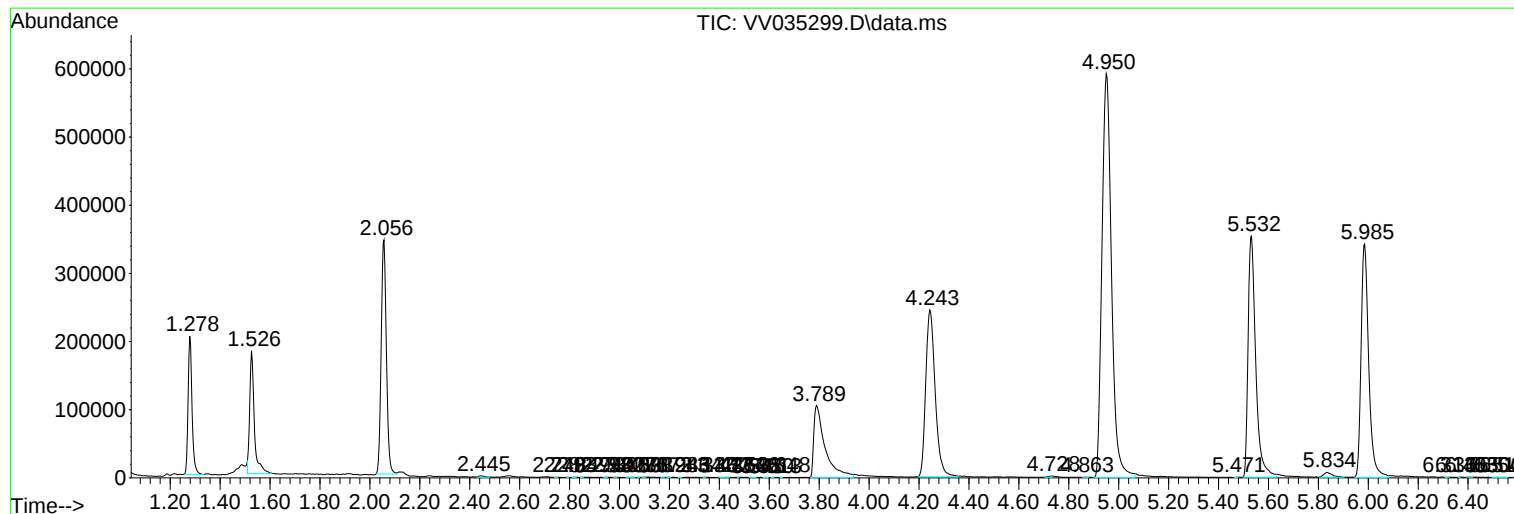

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035299.D
Acq On : 19 Apr 2024 11:49
Operator : SY/MD
Sample : P2158-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035299.D
Acq On : 19 Apr 2024 11:49
Operator : SY/MD
Sample : P2158-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
