

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035303.D
 Acq On : 19 Apr 2024 13:23
 Operator : SY/MD
 Sample : P2157-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rBV	181727	192866	13.04%	1.714%
2	1.532	146	153	167	rVB	163454	192713	13.02%	1.713%
3	2.060	307	317	331	rBV	305219	445115	30.08%	3.956%
4	2.777	538	540	544	rVB2	397	255	0.02%	0.002%
5	2.809	547	550	553	rBV2	253	149	0.01%	0.001%
6	2.828	554	556	557	rBV	187	64	0.00%	0.001%
7	2.899	574	578	581	rBV3	419	335	0.02%	0.003%
8	3.098	638	640	645	rVB2	371	228	0.02%	0.002%
9	3.127	645	649	650	rBV	403	266	0.02%	0.002%
10	3.172	659	663	666	rBV2	254	213	0.01%	0.002%
11	3.240	681	684	685	rBV2	225	130	0.01%	0.001%
12	3.268	691	693	696	rVB	250	127	0.01%	0.001%
13	3.281	696	697	699	rVB	121	46	0.00%	0.000%
14	3.301	699	703	707	rBV3	243	197	0.01%	0.002%
15	3.323	707	710	712	rBV	224	127	0.01%	0.001%
16	3.352	716	719	721	rBV2	201	132	0.01%	0.001%
17	3.436	740	745	748	rBV	292	303	0.02%	0.003%
18	3.471	755	756	759	rBV2	225	71	0.00%	0.001%
19	3.484	759	760	761	rBV2	134	44	0.00%	0.000%
20	3.513	766	769	771	rBV	142	102	0.01%	0.001%
21	3.577	786	789	790	rBV	83	49	0.00%	0.000%
22	3.587	790	792	795	rBV2	153	119	0.01%	0.001%
23	3.625	801	804	806	rBV	130	88	0.01%	0.001%
24	3.635	806	807	808	rBV	216	76	0.01%	0.001%
25	3.683	817	822	823	rBV	137	86	0.01%	0.001%
26	3.703	825	828	829	rBV	155	87	0.01%	0.001%
27	3.722	833	834	837	rBV	203	104	0.01%	0.001%
28	3.786	846	854	895	rBV	110982	331647	22.41%	2.948%
29	4.246	982	997	1034	rBV	231478	604851	40.88%	5.376%
30	4.567	1095	1097	1102	rBV4	450	415	0.03%	0.004%
31	4.776	1160	1162	1165	rVB	318	154	0.01%	0.001%
32	4.799	1165	1169	1171	rBV2	357	288	0.02%	0.003%
33	4.953	1202	1217	1263	rBV2	553490	1479596	100.00%	13.152%
34	5.416	1359	1361	1364	rBV3	306	179	0.01%	0.002%
35	5.493	1382	1385	1386	rBV	411	207	0.01%	0.002%
36	5.532	1386	1397	1442	rVV	456987	959835	64.87%	8.532%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035303.D
 Acq On : 19 Apr 2024 13:23
 Operator : SY/MD
 Sample : P2157-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.838	1482	1492	1510	rBV5	5955	13489	0.91%	0.120%
38	5.985	1526	1538	1564	rBV	320687	679583	45.93%	6.041%
39	6.333	1644	1646	1649	rBV4	315	116	0.01%	0.001%
40	6.400	1665	1667	1669	rBV3	387	216	0.01%	0.002%
41	6.465	1685	1687	1690	rBV	208	99	0.01%	0.001%
42	6.490	1692	1695	1698	rVV2	203	179	0.01%	0.002%
43	6.558	1713	1716	1720	rBV3	171	113	0.01%	0.001%
44	6.603	1727	1730	1733	rBV2	332	248	0.02%	0.002%
45	6.638	1738	1741	1743	rBV2	653	449	0.03%	0.004%
46	6.670	1747	1751	1756	rBV4	607	745	0.05%	0.007%
47	6.728	1765	1769	1771	rBV	226	156	0.01%	0.001%
48	6.744	1771	1774	1776	rVB3	197	113	0.01%	0.001%
49	6.789	1783	1788	1791	rVB2	362	345	0.02%	0.003%
50	6.805	1791	1793	1794	rBV	229	112	0.01%	0.001%
51	6.860	1807	1810	1812	rBV2	215	85	0.01%	0.001%
52	6.915	1812	1827	1857	rBV	138249	279599	18.90%	2.485%
53	7.243	1918	1929	1952	rBV	601059	1069682	72.30%	9.508%
54	7.554	2017	2026	2051	rBV2	96089	185270	12.52%	1.647%
55	7.783	2095	2097	2100	rBV	372	254	0.02%	0.002%
56	7.841	2111	2115	2118	rBV3	505	380	0.03%	0.003%
57	7.921	2138	2140	2143	rBV4	312	207	0.01%	0.002%
58	8.024	2163	2172	2217	rBV2	308596	702432	47.47%	6.244%
59	8.548	2334	2335	2339	rBV	435	249	0.02%	0.002%
60	8.603	2350	2352	2357	rVB2	571	282	0.02%	0.003%
61	8.628	2357	2360	2368	rBV3	434	557	0.04%	0.005%
62	8.664	2368	2371	2373	rBV2	229	98	0.01%	0.001%
63	8.683	2373	2377	2381	rBV3	489	387	0.03%	0.003%
64	8.702	2381	2383	2384	rBV	200	74	0.01%	0.001%
65	8.783	2397	2408	2438	rBV	725165	1213933	82.04%	10.790%
66	9.188	2532	2534	2537	rVB2	468	184	0.01%	0.002%
67	9.259	2552	2556	2557	rBV	489	303	0.02%	0.003%
68	9.291	2564	2566	2570	rBV2	240	183	0.01%	0.002%
69	9.362	2586	2588	2592	rBV2	241	190	0.01%	0.002%
70	9.400	2598	2600	2601	rBV	152	50	0.00%	0.000%
71	9.497	2628	2630	2631	rBV	297	145	0.01%	0.001%
72	9.542	2642	2644	2646	rBV	232	126	0.01%	0.001%
73	9.638	2671	2674	2677	rBV2	196	133	0.01%	0.001%
74	9.683	2685	2688	2690	rBV2	218	126	0.01%	0.001%
75	9.715	2695	2698	2700	rBV	253	180	0.01%	0.002%
76	9.789	2718	2721	2725	rBV2	323	227	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035303.D
 Acq On : 19 Apr 2024 13:23
 Operator : SY/MD
 Sample : P2157-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.024	2791	2794	2796	rBV	259	182	0.01%	0.002%
78	10.149	2822	2833	2868	rBV	496335	782156	52.86%	6.952%
79	10.381	2902	2905	2908	rBV2	277	269	0.02%	0.002%
80	10.490	2936	2939	2944	rBV2	340	252	0.02%	0.002%
81	10.625	2976	2981	2983	rBV	164	193	0.01%	0.002%
82	10.741	3014	3017	3020	rBV2	330	231	0.02%	0.002%
83	10.895	3062	3065	3068	rVB2	343	196	0.01%	0.002%
84	11.021	3101	3104	3105	rBV2	216	134	0.01%	0.001%
85	11.046	3109	3112	3115	rBV2	244	192	0.01%	0.002%
86	11.130	3134	3138	3144	rBV5	810	1049	0.07%	0.009%
87	11.185	3144	3155	3184	rVV	658747	1059941	71.64%	9.421%
88	11.509	3249	3256	3258	rBV5	2986	3549	0.24%	0.032%
89	11.558	3261	3271	3305	rVB	633513	1036789	70.07%	9.216%
90	11.947	3388	3392	3393	rBV2	356	262	0.02%	0.002%
91	12.085	3433	3435	3438	rBV2	408	263	0.02%	0.002%
92	12.136	3449	3451	3455	rVB2	324	191	0.01%	0.002%
93	12.194	3465	3469	3473	rBV3	538	502	0.03%	0.004%
94	12.336	3509	3513	3516	rBV3	475	429	0.03%	0.004%
95	12.586	3588	3591	3599	rBV3	602	695	0.05%	0.006%
96	13.024	3723	3727	3729	rBV	396	250	0.02%	0.002%




Sum of corrected areas: 11250288

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035303.D
Acq On : 19 Apr 2024 13:23
Operator : SY/MD
Sample : P2157-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

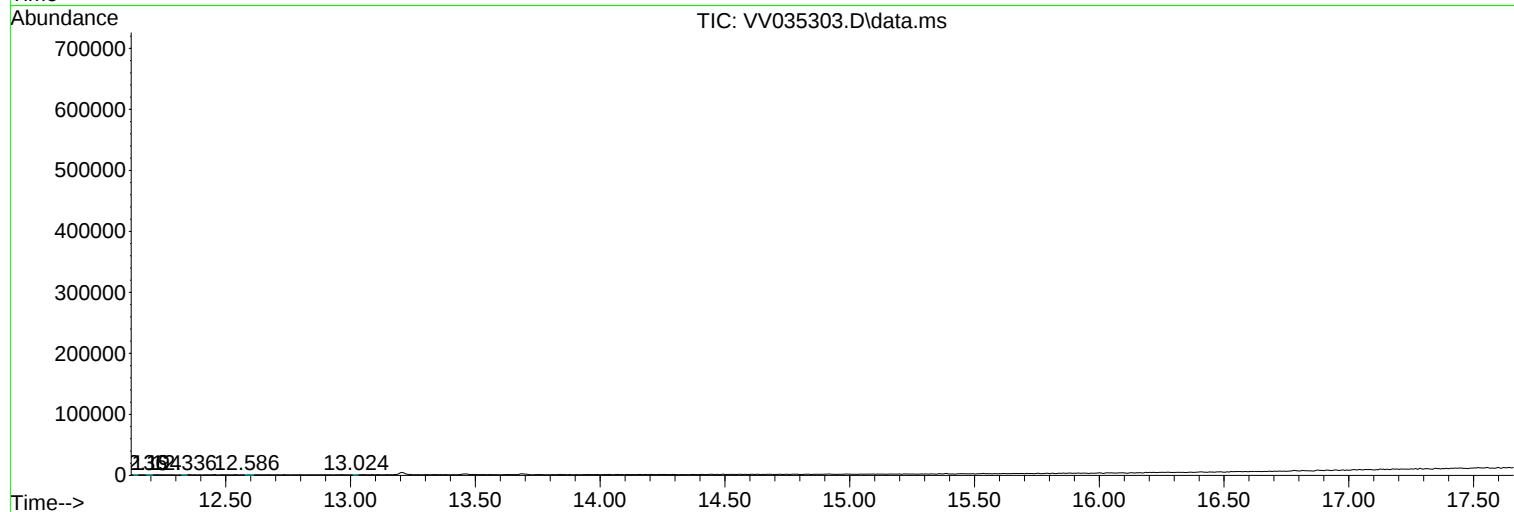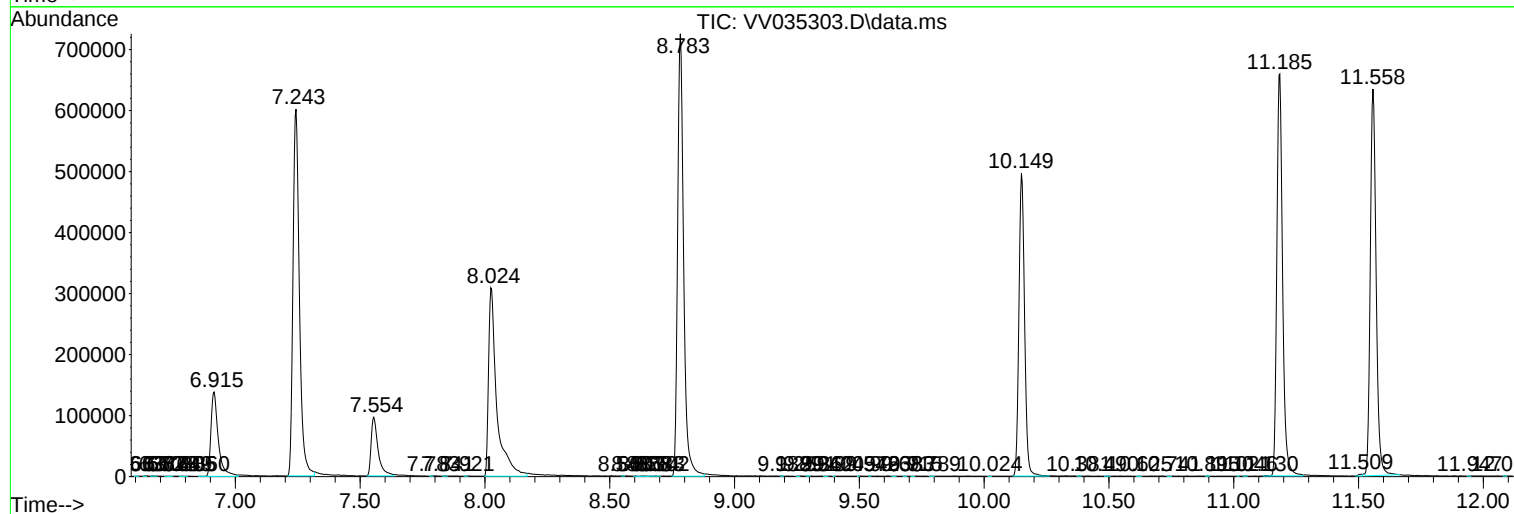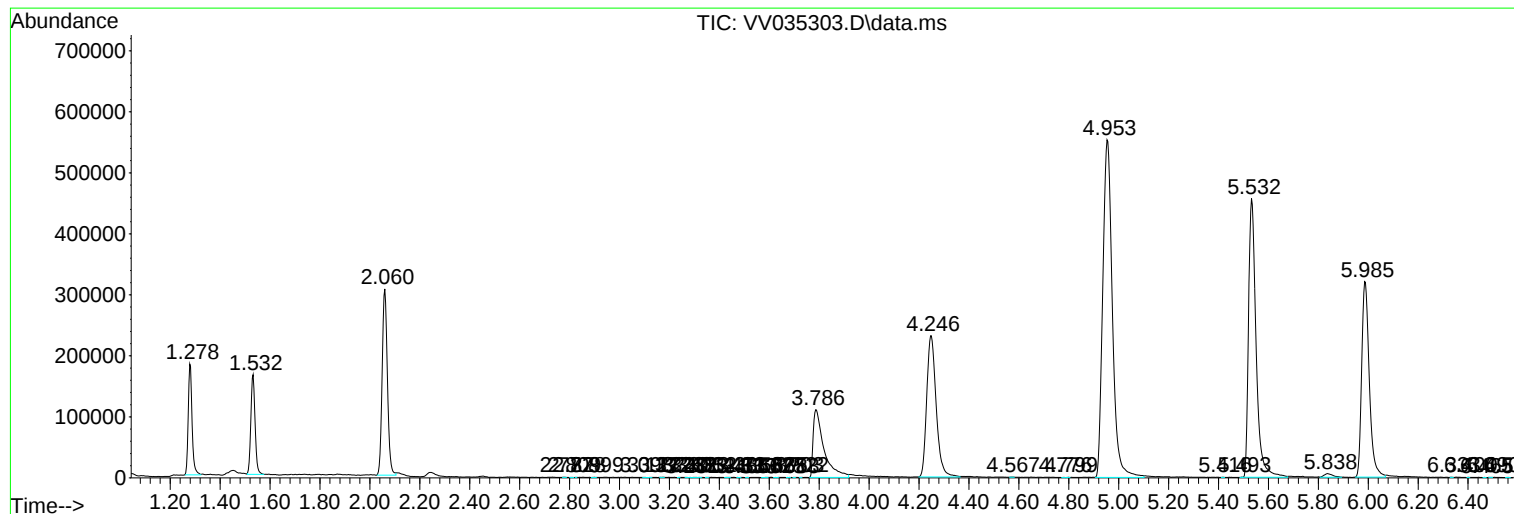

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035303.D
Acq On : 19 Apr 2024 13:23
Operator : SY/MD
Sample : P2157-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035303.D
Acq On : 19 Apr 2024 13:23
Operator : SY/MD
Sample : P2157-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc