

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035305.D
 Acq On : 19 Apr 2024 14:08
 Operator : SY/MD
 Sample : P2157-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	176869	189177	12.79%	1.730%
2	1.532	146	153	171	rVB	168468	200466	13.56%	1.833%
3	2.060	308	317	331	rBV	296596	423478	28.64%	3.872%
4	2.548	467	469	471	rBV3	289	152	0.01%	0.001%
5	2.577	474	478	480	rBV2	433	351	0.02%	0.003%
6	2.632	492	495	498	rBV	323	214	0.01%	0.002%
7	2.719	520	522	523	rBV2	369	159	0.01%	0.001%
8	2.822	549	554	555	rBV2	222	189	0.01%	0.002%
9	2.838	557	559	562	rVB2	355	187	0.01%	0.002%
10	2.873	567	570	572	rVV	193	117	0.01%	0.001%
11	2.995	605	608	610	rBV2	200	154	0.01%	0.001%
12	3.072	629	632	636	rVB2	397	257	0.02%	0.002%
13	3.101	638	641	643	rBV2	211	118	0.01%	0.001%
14	3.349	715	718	722	rVV	240	197	0.01%	0.002%
15	3.423	738	741	743	rBV2	173	118	0.01%	0.001%
16	3.523	769	772	775	rVV	281	156	0.01%	0.001%
17	3.558	781	783	786	rVB2	291	144	0.01%	0.001%
18	3.587	786	792	796	rBB3	270	232	0.02%	0.002%
19	3.609	796	799	801	rBV	293	199	0.01%	0.002%
20	3.661	811	815	817	rBV2	262	180	0.01%	0.002%
21	3.741	837	840	843	rVB3	322	234	0.02%	0.002%
22	3.789	846	855	901	rBV	113330	340387	23.02%	3.112%
23	4.249	983	998	1030	rBV	231881	603022	40.78%	5.513%
24	4.818	1171	1175	1180	rBV2	352	357	0.02%	0.003%
25	4.889	1192	1197	1199	rBV2	419	342	0.02%	0.003%
26	4.957	1202	1218	1258	rBV2	552346	1478862	100.00%	13.521%
27	5.320	1329	1331	1333	rBV3	346	122	0.01%	0.001%
28	5.474	1376	1379	1381	rVB2	330	171	0.01%	0.002%
29	5.532	1386	1397	1438	rBV	424647	900716	60.91%	8.235%
30	5.989	1526	1539	1573	rVV	329885	701924	47.46%	6.417%
31	6.346	1647	1650	1651	rBV3	367	229	0.02%	0.002%
32	6.410	1666	1670	1673	rVB3	419	382	0.03%	0.003%
33	6.432	1673	1677	1678	rBV	442	232	0.02%	0.002%
34	6.461	1684	1686	1694	rVB3	357	416	0.03%	0.004%
35	6.500	1697	1698	1700	rVV2	312	124	0.01%	0.001%
36	6.519	1702	1704	1708	rVV2	431	211	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041924\
 Data File : VW035305.D
 Acq On : 19 Apr 2024 14:08
 Operator : SY/MD
 Sample : P2157-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.551	1712	1714	1719	rVB2	361	179	0.01%	0.002%
38	6.580	1719	1723	1728	rVB2	559	444	0.03%	0.004%
39	6.629	1731	1738	1741	rBV4	437	575	0.04%	0.005%
40	6.683	1753	1755	1758	rVB	270	146	0.01%	0.001%
41	6.699	1758	1760	1763	rBV3	480	205	0.01%	0.002%
42	6.725	1765	1768	1771	rBV2	193	118	0.01%	0.001%
43	6.821	1794	1798	1799	rBV2	208	162	0.01%	0.001%
44	6.866	1809	1812	1816	rBV2	328	289	0.02%	0.003%
45	6.915	1816	1827	1850	rBV	142264	280129	18.94%	2.561%
46	7.156	1900	1902	1905	rBV2	556	410	0.03%	0.004%
47	7.243	1918	1929	1956	rBV	580652	1032634	69.83%	9.441%
48	7.555	2017	2026	2055	rBV	98893	186496	12.61%	1.705%
49	7.857	2114	2120	2123	rBV3	558	505	0.03%	0.005%
50	7.918	2136	2139	2140	rVB2	313	124	0.01%	0.001%
51	7.940	2144	2146	2149	rBV2	322	150	0.01%	0.001%
52	7.960	2151	2152	2154	rBV	353	139	0.01%	0.001%
53	7.979	2154	2158	2160	rBV	266	221	0.01%	0.002%
54	8.024	2163	2172	2208	rBV2	321568	719552	48.66%	6.579%
55	8.567	2337	2341	2344	rBV	439	361	0.02%	0.003%
56	8.625	2355	2359	2360	rBV3	359	214	0.01%	0.002%
57	8.712	2383	2386	2389	rBV2	324	311	0.02%	0.003%
58	8.744	2394	2396	2397	rBV	457	179	0.01%	0.002%
59	8.783	2397	2408	2435	rBV	657964	1105278	74.74%	10.105%
60	9.114	2508	2511	2513	rBV	376	253	0.02%	0.002%
61	9.127	2513	2515	2517	rBV	396	161	0.01%	0.001%
62	9.272	2558	2560	2562	rBV	295	139	0.01%	0.001%
63	9.300	2564	2569	2570	rBV2	239	153	0.01%	0.001%
64	9.336	2576	2580	2582	rBV3	442	310	0.02%	0.003%
65	9.349	2582	2584	2587	rVB	416	179	0.01%	0.002%
66	9.368	2587	2590	2592	rBV	212	150	0.01%	0.001%
67	9.410	2601	2603	2608	rVB2	342	278	0.02%	0.003%
68	9.445	2608	2614	2615	rBV2	216	163	0.01%	0.001%
69	9.487	2624	2627	2631	rBV3	443	288	0.02%	0.003%
70	9.506	2631	2633	2635	rVV3	205	119	0.01%	0.001%
71	9.532	2639	2641	2646	rVB	259	158	0.01%	0.001%
72	9.564	2646	2651	2652	rBV	362	241	0.02%	0.002%
73	9.776	2712	2717	2720	rBV3	312	308	0.02%	0.003%
74	9.837	2733	2736	2740	rVB	423	349	0.02%	0.003%
75	9.879	2745	2749	2755	rBV2	356	316	0.02%	0.003%
76	9.940	2765	2768	2772	rBV2	385	271	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035305.D
 Acq On : 19 Apr 2024 14:08
 Operator : SY/MD
 Sample : P2157-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.005	2785	2788	2791	rBV	233	163	0.01%	0.001%
78	10.046	2798	2801	2805	rVB2	332	201	0.01%	0.002%
79	10.149	2821	2833	2861	rBV	500988	803475	54.33%	7.346%
80	10.323	2884	2887	2888	rBV2	737	370	0.03%	0.003%
81	10.554	2957	2959	2961	rBV	265	145	0.01%	0.001%
82	10.677	2994	2997	2998	rBV2	202	121	0.01%	0.001%
83	10.718	3006	3010	3012	rBV2	296	194	0.01%	0.002%
84	10.847	3047	3050	3052	rVB2	295	149	0.01%	0.001%
85	10.863	3053	3055	3060	rBV2	430	236	0.02%	0.002%
86	11.008	3098	3100	3105	rVB3	279	241	0.02%	0.002%
87	11.130	3131	3138	3140	rBV4	1005	1065	0.07%	0.010%
88	11.185	3144	3155	3180	rBV	603465	951620	64.35%	8.700%
89	11.558	3260	3271	3300	rBV	612574	993365	67.17%	9.082%
90	11.841	3357	3359	3360	rBV	542	253	0.02%	0.002%
91	12.188	3462	3467	3472	rBV3	502	572	0.04%	0.005%
92	12.480	3556	3558	3559	rBV3	394	158	0.01%	0.001%
93	12.654	3610	3612	3614	rBV	364	214	0.01%	0.002%
94	12.972	3709	3711	3715	rVB2	333	218	0.01%	0.002%
95	12.995	3715	3718	3719	rBV	275	148	0.01%	0.001%
96	13.091	3744	3748	3752	rBV3	391	349	0.02%	0.003%
97	13.181	3773	3776	3777	rBV2	350	213	0.01%	0.002%
98	13.207	3777	3784	3799	rVB6	3697	6688	0.45%	0.061%
99	13.599	3903	3906	3909	rVB	517	285	0.02%	0.003%
100	14.262	4108	4112	4116	rBV2	763	586	0.04%	0.005%




Sum of corrected areas: 10937662

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035305.D
Acq On : 19 Apr 2024 14:08
Operator : SY/MD
Sample : P2157-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCOB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

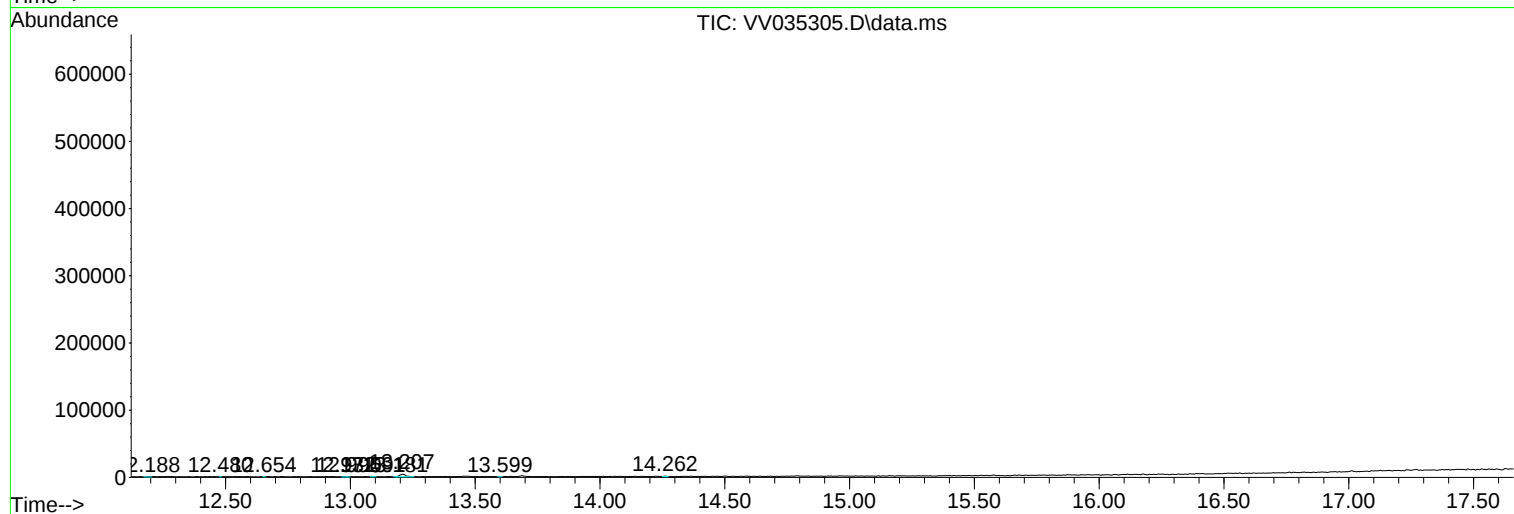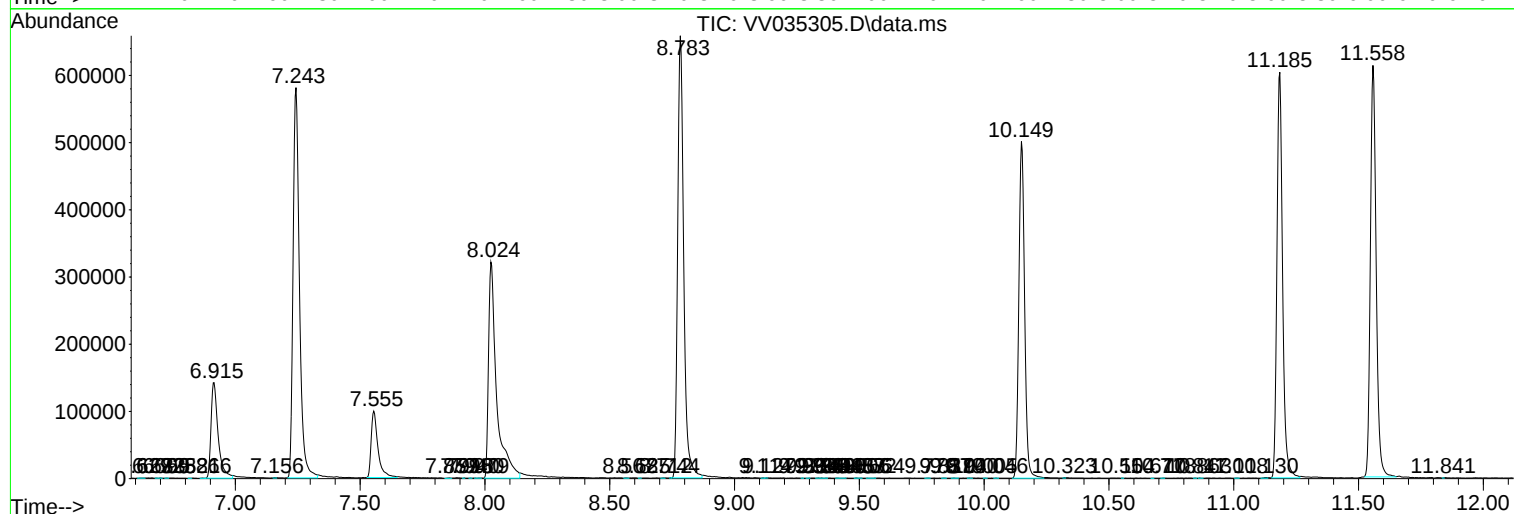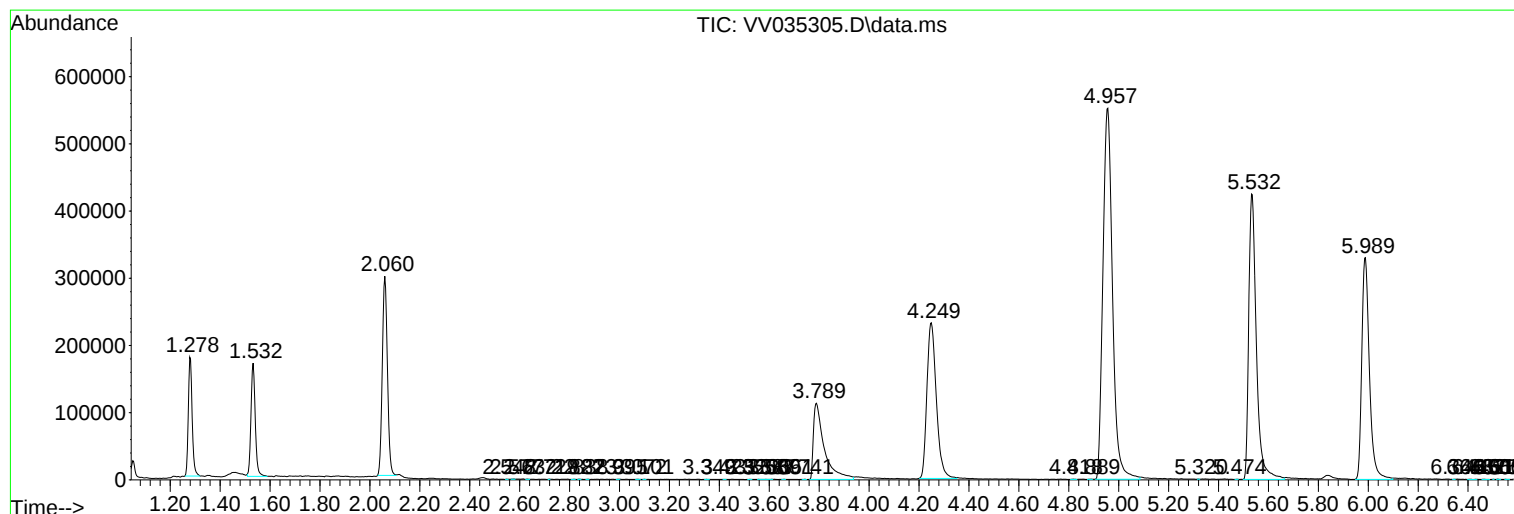

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035305.D
Acq On : 19 Apr 2024 14:08
Operator : SY/MD
Sample : P2157-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035305.D
Acq On : 19 Apr 2024 14:08
Operator : SY/MD
Sample : P2157-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------