

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035307.D
 Acq On : 19 Apr 2024 14:55
 Operator : SY/MD
 Sample : P2157-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	193786	204062	12.92%	1.710%
2	1.529	145	152	169	rVB	172882	205898	13.04%	1.725%
3	2.057	307	316	331	rBV	325823	473672	29.99%	3.969%
4	2.645	497	499	503	rVB2	517	268	0.02%	0.002%
5	2.700	513	516	518	rBV2	515	346	0.02%	0.003%
6	2.841	558	560	563	rVB	299	115	0.01%	0.001%
7	2.883	569	573	574	rBV2	326	173	0.01%	0.001%
8	2.915	582	583	585	rBV2	223	114	0.01%	0.001%
9	2.999	606	609	612	rBV3	286	210	0.01%	0.002%
10	3.011	612	613	617	rVV	321	180	0.01%	0.002%
11	3.066	627	630	635	rBV3	280	300	0.02%	0.003%
12	3.137	649	652	654	rBV	381	259	0.02%	0.002%
13	3.201	669	672	675	rBV	254	196	0.01%	0.002%
14	3.220	675	678	682	rVV2	362	253	0.02%	0.002%
15	3.243	682	685	689	rVV2	327	250	0.02%	0.002%
16	3.265	689	692	697	rBV3	188	174	0.01%	0.001%
17	3.310	704	706	707	rVB2	278	84	0.01%	0.001%
18	3.327	708	711	714	rVB2	260	158	0.01%	0.001%
19	3.397	730	733	734	rBV	212	116	0.01%	0.001%
20	3.471	751	756	757	rBV2	182	141	0.01%	0.001%
21	3.581	786	790	793	rBV2	271	190	0.01%	0.002%
22	3.632	800	806	810	rBV2	270	281	0.02%	0.002%
23	3.667	814	817	819	rVB2	260	158	0.01%	0.001%
24	3.680	819	821	822	rBV2	187	89	0.01%	0.001%
25	3.719	829	833	836	rVB	314	199	0.01%	0.002%
26	3.745	836	841	842	rBV3	250	165	0.01%	0.001%
27	3.786	845	854	900	rBV	121660	363743	23.03%	3.048%
28	4.246	983	997	1035	rVB	249387	638134	40.40%	5.347%
29	4.954	1201	1217	1254	rBV2	589978	1579510	100.00%	13.234%
30	5.429	1361	1365	1369	rVB3	545	483	0.03%	0.004%
31	5.449	1369	1371	1375	rVB2	451	318	0.02%	0.003%
32	5.474	1377	1379	1380	rBV2	305	134	0.01%	0.001%
33	5.532	1386	1397	1435	rBV	460779	970734	61.46%	8.133%
34	5.835	1482	1491	1505	rBV5	5585	12828	0.81%	0.107%
35	5.986	1526	1538	1575	rBV	349063	737328	46.68%	6.178%
36	6.259	1619	1623	1625	rBV3	562	441	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041924\
 Data File : VW035307.D
 Acq On : 19 Apr 2024 14:55
 Operator : SY/MD
 Sample : P2157-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.333	1644	1646	1650	rBV	255	175	0.01%	0.001%
38	6.371	1654	1658	1660	rBV2	366	297	0.02%	0.002%
39	6.439	1677	1679	1682	rBV2	260	144	0.01%	0.001%
40	6.461	1683	1686	1691	rVB2	436	362	0.02%	0.003%
41	6.487	1691	1694	1697	rBV	229	196	0.01%	0.002%
42	6.523	1701	1705	1708	rBV3	282	243	0.02%	0.002%
43	6.564	1717	1718	1723	rBV	323	188	0.01%	0.002%
44	6.587	1723	1725	1729	rVB2	226	123	0.01%	0.001%
45	6.609	1729	1732	1733	rBV	249	124	0.01%	0.001%
46	6.703	1759	1761	1764	rVB2	234	121	0.01%	0.001%
47	6.761	1778	1779	1785	rVB2	597	391	0.02%	0.003%
48	6.793	1785	1789	1794	rVB3	445	352	0.02%	0.003%
49	6.825	1794	1799	1801	rBV2	189	153	0.01%	0.001%
50	6.844	1801	1805	1807	rBV2	306	133	0.01%	0.001%
51	6.876	1812	1815	1816	rBV	168	98	0.01%	0.001%
52	6.912	1816	1826	1863	rBV	151445	303009	19.18%	2.539%
53	7.162	1897	1904	1906	rBV5	756	908	0.06%	0.008%
54	7.243	1917	1929	1963	rBV	661970	1176038	74.46%	9.854%
55	7.555	2017	2026	2050	rBV	105002	199445	12.63%	1.671%
56	7.818	2104	2108	2111	rBV2	469	458	0.03%	0.004%
57	7.850	2115	2118	2120	rVB2	482	294	0.02%	0.002%
58	7.870	2120	2124	2126	rBV3	698	496	0.03%	0.004%
59	7.950	2146	2149	2154	rBV4	486	371	0.02%	0.003%
60	7.979	2156	2158	2162	rVB2	315	124	0.01%	0.001%
61	8.024	2163	2172	2221	rBV2	331225	743849	47.09%	6.232%
62	8.609	2352	2354	2357	rBV3	294	182	0.01%	0.002%
63	8.674	2372	2374	2377	rBV3	249	159	0.01%	0.001%
64	8.783	2397	2408	2451	rBV	724144	1230118	77.88%	10.307%
65	9.140	2516	2519	2520	rBV3	443	247	0.02%	0.002%
66	9.198	2535	2537	2540	rBV2	427	191	0.01%	0.002%
67	9.220	2540	2544	2549	rBV4	238	231	0.01%	0.002%
68	9.249	2549	2553	2556	rBV2	292	312	0.02%	0.003%
69	9.275	2559	2561	2565	rVB2	277	173	0.01%	0.001%
70	9.317	2570	2574	2575	rBV2	275	190	0.01%	0.002%
71	9.352	2580	2585	2587	rBV2	284	251	0.02%	0.002%
72	9.375	2590	2592	2594	rBV	274	140	0.01%	0.001%
73	9.452	2612	2616	2617	rBV2	289	157	0.01%	0.001%
74	9.522	2634	2638	2642	rBV2	360	242	0.02%	0.002%
75	9.603	2660	2663	2664	rBV	300	189	0.01%	0.002%
76	9.638	2671	2674	2676	rBV	192	105	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035307.D
 Acq On : 19 Apr 2024 14:55
 Operator : SY/MD
 Sample : P2157-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.686	2687	2689	2695	rBV2	280	252	0.02%	0.002%
78	9.722	2695	2700	2706	rVB2	369	342	0.02%	0.003%
79	9.780	2714	2718	2720	rBV3	410	261	0.02%	0.002%
80	9.847	2734	2739	2743	rBV2	406	398	0.03%	0.003%
81	9.957	2771	2773	2776	rBV2	362	251	0.02%	0.002%
82	9.985	2780	2782	2784	rBV2	189	88	0.01%	0.001%
83	10.072	2806	2809	2811	rVB	164	93	0.01%	0.001%
84	10.149	2819	2833	2862	rBV	531591	846693	53.60%	7.094%
85	10.439	2920	2923	2926	rVB2	445	315	0.02%	0.003%
86	10.468	2930	2932	2934	rBV2	282	135	0.01%	0.001%
87	10.619	2975	2979	2982	rVB2	322	276	0.02%	0.002%
88	10.638	2982	2985	2987	rBV	263	183	0.01%	0.002%
89	10.854	3051	3052	3055	rVB	463	157	0.01%	0.001%
90	10.870	3055	3057	3060	rBV	397	231	0.01%	0.002%
91	11.001	3096	3098	3102	rVB	231	130	0.01%	0.001%
92	11.027	3102	3106	3107	rBV2	249	187	0.01%	0.002%
93	11.130	3134	3138	3144	rBV5	1169	1408	0.09%	0.012%
94	11.185	3144	3155	3185	rVV	680385	1081170	68.45%	9.059%
95	11.513	3248	3257	3260	rBV6	4416	6474	0.41%	0.054%
96	11.558	3261	3271	3299	rVB	702705	1136201	71.93%	9.520%
97	11.950	3392	3393	3394	rBV	537	166	0.01%	0.001%
98	12.082	3431	3434	3439	rBV2	288	248	0.02%	0.002%
99	13.207	3776	3784	3792	rBV7	4169	6478	0.41%	0.054%
100	13.599	3902	3906	3908	rBV	405	385	0.02%	0.003%




Sum of corrected areas: 11935205

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035307.D
Acq On : 19 Apr 2024 14:55
Operator : SY/MD
Sample : P2157-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

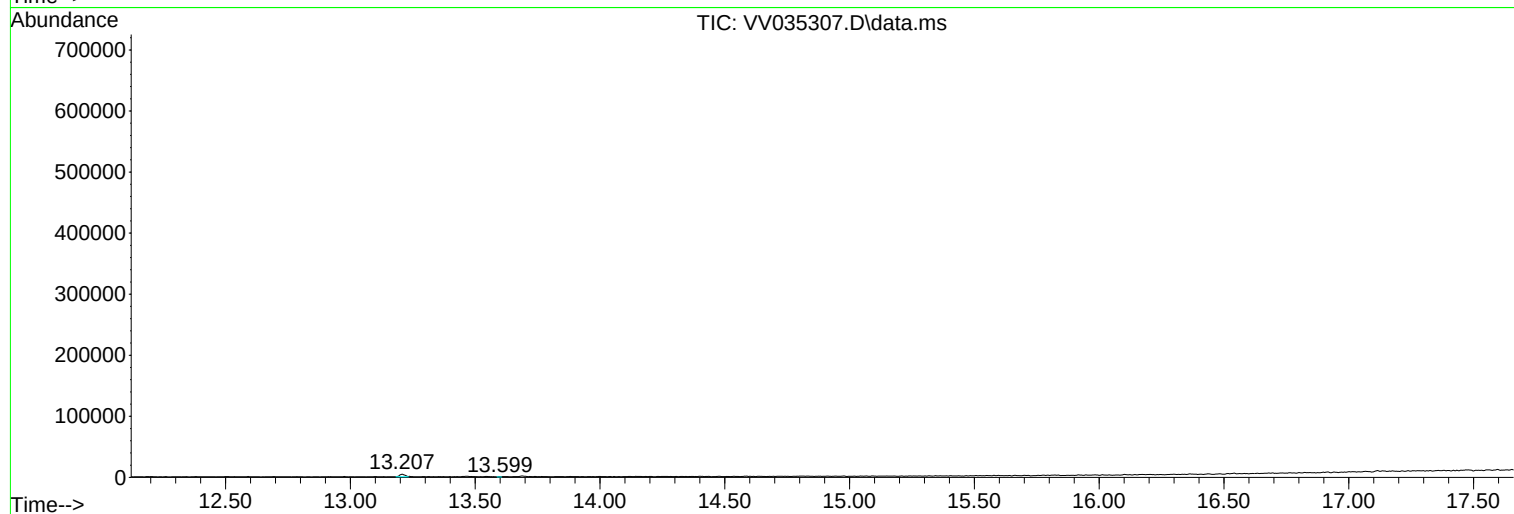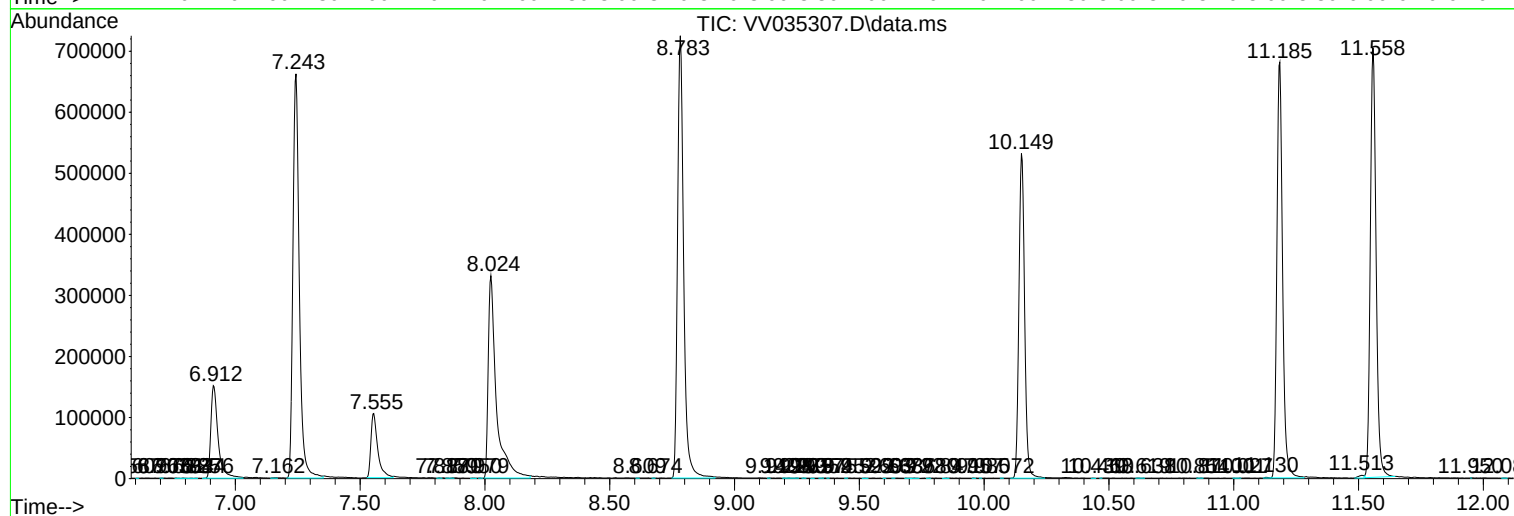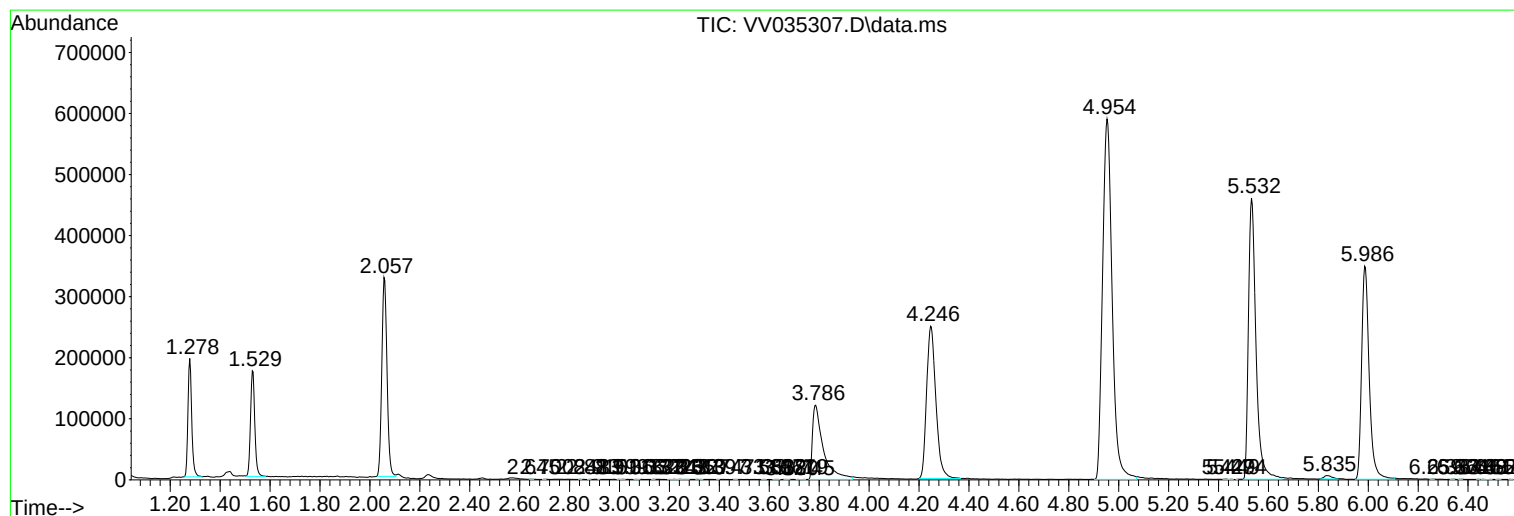

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035307.D
Acq On : 19 Apr 2024 14:55
Operator : SY/MD
Sample : P2157-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035307.D
Acq On : 19 Apr 2024 14:55
Operator : SY/MD
Sample : P2157-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------