

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035308.D
 Acq On : 19 Apr 2024 15:18
 Operator : SY/MD
 Sample : P2157-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	200734	207852	13.01%	1.739%
2	1.529	145	152	172	rVB	172655	207311	12.97%	1.735%
3	2.059	307	317	332	rBV	323066	469770	29.40%	3.931%
4	2.526	460	462	465	rBV2	438	281	0.02%	0.002%
5	2.551	465	470	473	rBV3	521	539	0.03%	0.005%
6	2.783	540	542	543	rBV3	236	96	0.01%	0.001%
7	3.053	622	626	630	rBV3	397	313	0.02%	0.003%
8	3.117	640	646	647	rBV2	147	144	0.01%	0.001%
9	3.191	665	669	673	rVB2	348	327	0.02%	0.003%
10	3.214	673	676	679	rBV2	185	160	0.01%	0.001%
11	3.233	680	682	686	rVB2	288	174	0.01%	0.001%
12	3.323	706	710	712	rBV2	193	182	0.01%	0.002%
13	3.355	717	720	724	rVB	246	187	0.01%	0.002%
14	3.378	724	727	733	rBV2	354	371	0.02%	0.003%
15	3.410	733	737	743	rVB4	354	344	0.02%	0.003%
16	3.442	744	747	749	rBV	152	95	0.01%	0.001%
17	3.535	774	776	782	rVB	275	231	0.01%	0.002%
18	3.593	791	794	797	rBV	295	168	0.01%	0.001%
19	3.622	801	803	806	rVB	133	63	0.00%	0.001%
20	3.648	808	811	815	rVB2	223	157	0.01%	0.001%
21	3.690	822	824	827	rVB	276	136	0.01%	0.001%
22	3.709	827	830	831	rBV	184	112	0.01%	0.001%
23	3.719	831	833	834	rBV	299	120	0.01%	0.001%
24	3.744	839	841	843	rVB2	228	96	0.01%	0.001%
25	3.757	843	845	846	rBV	215	97	0.01%	0.001%
26	3.786	846	854	887	rBV	118390	332335	20.80%	2.781%
27	4.246	982	997	1031	rBV	248570	643272	40.25%	5.383%
28	4.728	1145	1147	1151	rBV2	238	131	0.01%	0.001%
29	4.838	1178	1181	1183	rBV2	327	248	0.02%	0.002%
30	4.953	1201	1217	1270	rBV2	585293	1598010	100.00%	13.372%
31	5.352	1339	1341	1343	rBV2	394	192	0.01%	0.002%
32	5.532	1386	1397	1433	rBV	460009	968315	60.60%	8.103%
33	5.837	1482	1492	1508	rBV5	5423	13328	0.83%	0.112%
34	5.985	1526	1538	1572	rBV	347956	727377	45.52%	6.087%
35	6.275	1626	1628	1631	rVB2	518	232	0.01%	0.002%
36	6.349	1649	1651	1652	rBV2	234	86	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035308.D
 Acq On : 19 Apr 2024 15:18
 Operator : SY/MD
 Sample : P2157-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.400	1666	1667	1670	rVB	248	86	0.01%	0.001%
38	6.432	1675	1677	1680	rBV2	119	75	0.00%	0.001%
39	6.452	1680	1683	1685	rVV3	385	221	0.01%	0.002%
40	6.474	1687	1690	1693	rBV	369	188	0.01%	0.002%
41	6.577	1717	1722	1726	rBV3	345	446	0.03%	0.004%
42	6.677	1751	1753	1756	rVB2	387	157	0.01%	0.001%
43	6.715	1763	1765	1770	rVB3	266	154	0.01%	0.001%
44	6.825	1796	1799	1802	rBV2	210	162	0.01%	0.001%
45	6.911	1813	1826	1853	rBV	148337	297723	18.63%	2.491%
46	7.243	1918	1929	1962	rBV	658430	1162376	72.74%	9.727%
47	7.554	2017	2026	2049	rBV	104756	197037	12.33%	1.649%
48	7.828	2109	2111	2114	rVB2	480	200	0.01%	0.002%
49	7.921	2138	2140	2142	rVB	386	121	0.01%	0.001%
50	7.972	2152	2156	2158	rBV2	239	178	0.01%	0.001%
51	7.989	2158	2161	2163	rBV2	524	303	0.02%	0.003%
52	8.024	2163	2172	2215	rBV2	340102	748961	46.87%	6.267%
53	8.561	2336	2339	2341	rBV2	448	240	0.02%	0.002%
54	8.609	2348	2354	2359	rBV4	517	485	0.03%	0.004%
55	8.632	2359	2361	2363	rBV3	473	288	0.02%	0.002%
56	8.783	2397	2408	2444	rBV	731486	1264178	79.11%	10.579%
57	9.095	2504	2505	2506	rBV	258	81	0.01%	0.001%
58	9.239	2546	2550	2552	rBV2	195	159	0.01%	0.001%
59	9.284	2560	2564	2568	rBV3	533	558	0.03%	0.005%
60	9.349	2580	2584	2587	rBV	188	176	0.01%	0.001%
61	9.542	2642	2644	2646	rVB	289	77	0.00%	0.001%
62	9.554	2646	2648	2651	rBV	277	200	0.01%	0.002%
63	9.574	2651	2654	2655	rBV	323	159	0.01%	0.001%
64	9.625	2667	2670	2672	rBV	99	71	0.00%	0.001%
65	9.638	2672	2674	2677	rVV	207	117	0.01%	0.001%
66	9.654	2677	2679	2681	rBV2	236	103	0.01%	0.001%
67	9.689	2688	2690	2694	rBV2	228	141	0.01%	0.001%
68	9.824	2730	2732	2734	rBV2	242	136	0.01%	0.001%
69	9.879	2746	2749	2751	rBV	280	196	0.01%	0.002%
70	9.937	2765	2767	2769	rVB	247	85	0.01%	0.001%
71	9.976	2773	2779	2785	rBV4	285	397	0.02%	0.003%
72	10.149	2821	2833	2864	rBV	530666	841671	52.67%	7.043%
73	10.429	2916	2920	2923	rBV3	463	389	0.02%	0.003%
74	10.445	2923	2925	2932	rVB2	335	282	0.02%	0.002%
75	10.480	2932	2936	2938	rBV	276	218	0.01%	0.002%
76	10.583	2965	2968	2970	rBV	249	166	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035308.D
 Acq On : 19 Apr 2024 15:18
 Operator : SY/MD
 Sample : P2157-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.619	2977	2979	2981	rVB	256	106	0.01%	0.001%
78	10.632	2981	2983	2985	rBV	125	69	0.00%	0.001%
79	10.664	2989	2993	2998	rVB2	501	487	0.03%	0.004%
80	10.693	2998	3002	3003	rBV	422	236	0.01%	0.002%
81	10.702	3003	3005	3007	rBV	169	81	0.01%	0.001%
82	10.754	3014	3021	3025	rBV3	326	420	0.03%	0.004%
83	10.802	3033	3036	3040	rVB3	480	286	0.02%	0.002%
84	10.857	3051	3053	3056	rBV3	343	214	0.01%	0.002%
85	11.017	3101	3103	3106	rBV	301	233	0.01%	0.002%
86	11.101	3124	3129	3132	rBV2	376	255	0.02%	0.002%
87	11.130	3132	3138	3144	rBV4	1979	2717	0.17%	0.023%
88	11.185	3144	3155	3187	rVV	689173	1109621	69.44%	9.285%
89	11.477	3244	3246	3249	rBV	434	223	0.01%	0.002%
90	11.558	3261	3271	3300	rVB	708111	1133469	70.93%	9.485%
91	11.869	3366	3368	3375	rBV3	425	296	0.02%	0.002%
92	11.921	3382	3384	3386	rBV	492	239	0.01%	0.002%
93	11.998	3403	3408	3414	rBV4	442	602	0.04%	0.005%
94	12.085	3432	3435	3438	rVB2	324	190	0.01%	0.002%
95	12.448	3544	3548	3551	rBV2	390	364	0.02%	0.003%
96	12.490	3559	3561	3567	rBV	359	294	0.02%	0.002%
97	12.538	3570	3576	3580	rBV3	460	536	0.03%	0.004%
98	12.561	3580	3583	3585	rBV2	338	207	0.01%	0.002%
99	13.207	3777	3784	3793	rBV5	4367	6756	0.42%	0.057%
100	13.802	3966	3969	3972	rBV3	506	382	0.02%	0.003%




Sum of corrected areas: 11950096

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035308.D
Acq On : 19 Apr 2024 15:18
Operator : SY/MD
Sample : P2157-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

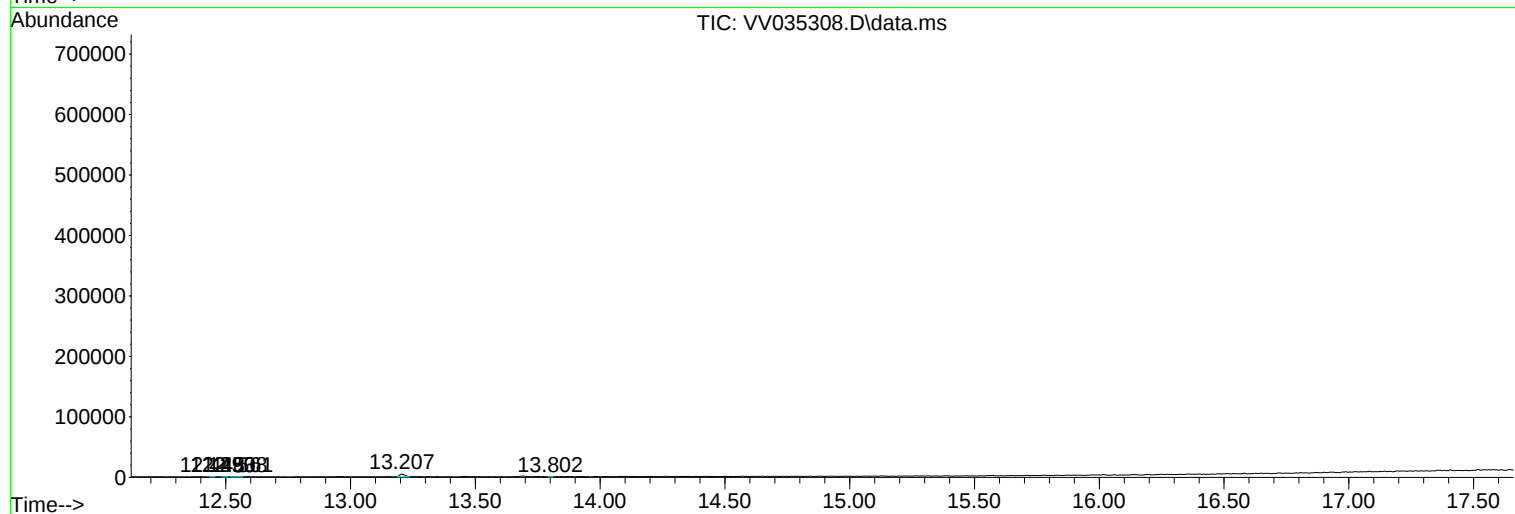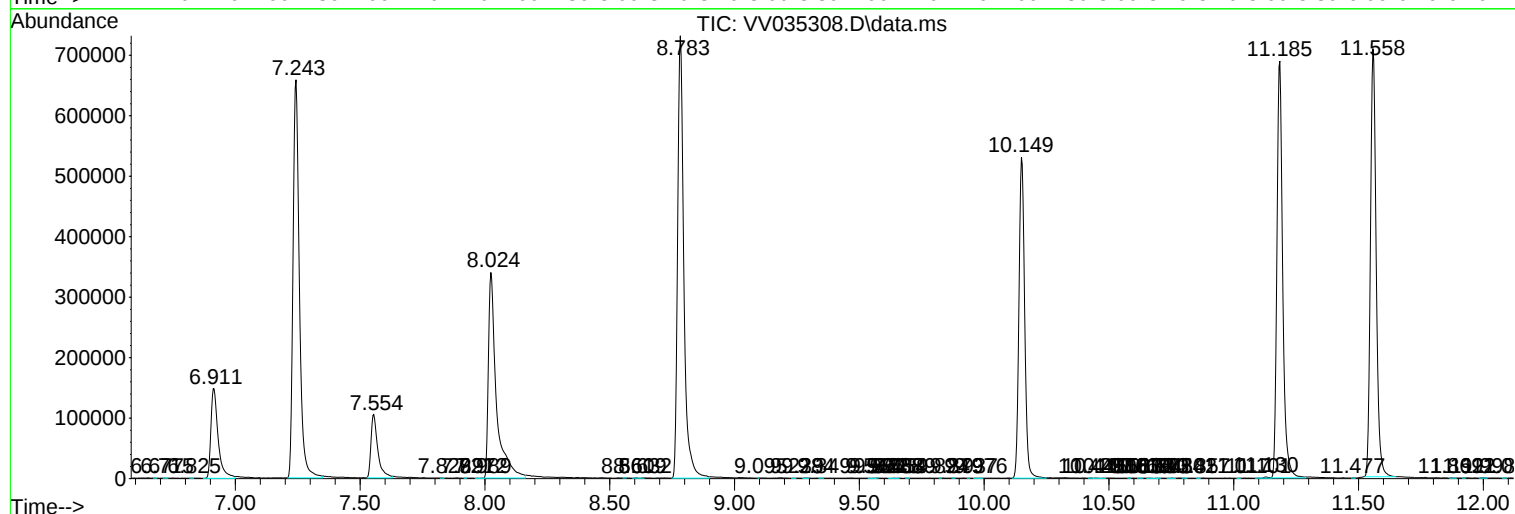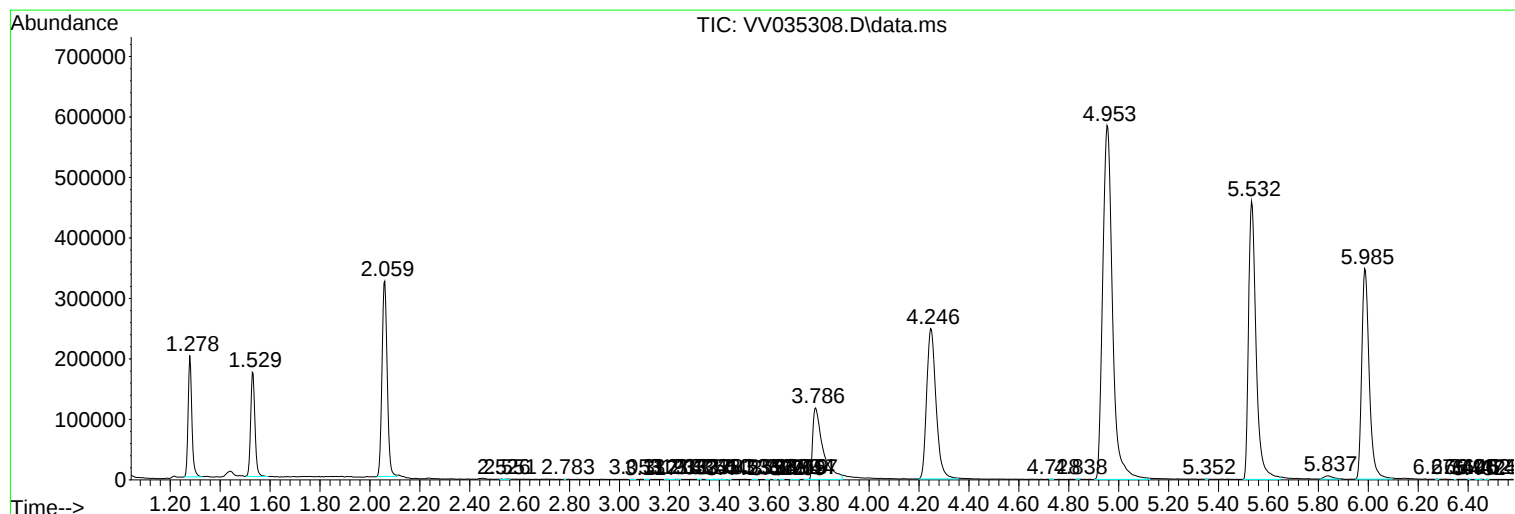

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035308.D
Acq On : 19 Apr 2024 15:18
Operator : SY/MD
Sample : P2157-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035308.D
Acq On : 19 Apr 2024 15:18
Operator : SY/MD
Sample : P2157-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------