

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035310.D
 Acq On : 19 Apr 2024 16:04
 Operator : SY/MD
 Sample : P2157-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	185181	196456	3.26%	0.933%
2	1.529	145	152	171	rVB	165094	199620	3.31%	0.948%
3	2.060	307	317	330	rBV	316334	456583	7.58%	2.168%
4	2.625	491	493	494	rBV	201	86	0.00%	0.000%
5	2.699	514	516	522	rVB3	508	396	0.01%	0.002%
6	2.838	557	559	562	rBV	257	124	0.00%	0.001%
7	2.924	584	586	587	rBV	336	86	0.00%	0.000%
8	3.008	610	612	615	rVB	287	120	0.00%	0.001%
9	3.031	615	619	622	rBV3	192	175	0.00%	0.001%
10	3.063	627	629	633	rVV2	295	172	0.00%	0.001%
11	3.088	633	637	641	rVB2	375	250	0.00%	0.001%
12	3.114	641	645	648	rBV3	226	166	0.00%	0.001%
13	3.304	702	704	707	rVB2	278	143	0.00%	0.001%
14	3.336	711	714	718	rBV2	198	215	0.00%	0.001%
15	3.355	718	720	722	rBV2	221	122	0.00%	0.001%
16	3.404	733	735	738	rBV	245	162	0.00%	0.001%
17	3.436	743	745	750	rBV3	158	152	0.00%	0.001%
18	3.481	755	759	765	rVB3	325	341	0.01%	0.002%
19	3.519	765	771	776	rBV3	331	440	0.01%	0.002%
20	3.555	776	782	784	rBV	257	238	0.00%	0.001%
21	3.606	793	798	799	rBV	172	120	0.00%	0.001%
22	3.670	808	818	819	rBV4	1155	1420	0.02%	0.007%
23	3.748	836	842	845	rBV	164	141	0.00%	0.001%
24	3.786	845	854	898	rBV	117446	353293	5.86%	1.678%
25	4.182	975	977	979	rBV2	478	159	0.00%	0.001%
26	4.246	982	997	1033	rVV	240805	624683	10.37%	2.966%
27	4.793	1165	1167	1170	rVB3	306	149	0.00%	0.001%
28	4.812	1170	1173	1175	rBV2	204	127	0.00%	0.001%
29	4.870	1188	1191	1194	rVB	431	301	0.00%	0.001%
30	4.957	1194	1218	1225	rBV2	587360	1459196	24.22%	6.929%
31	5.532	1386	1397	1432	rBV	456189	955445	15.86%	4.537%
32	5.928	1518	1520	1524	rVB4	449	295	0.00%	0.001%
33	5.985	1525	1538	1575	rBV	335602	709590	11.78%	3.370%
34	6.278	1627	1629	1631	rBV2	279	130	0.00%	0.001%
35	6.362	1653	1655	1657	rVB2	380	124	0.00%	0.001%
36	6.439	1676	1679	1683	rVB2	577	343	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035310.D
 Acq On : 19 Apr 2024 16:04
 Operator : SY/MD
 Sample : P2157-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.465	1683	1687	1692	rBV3	430	369	0.01%	0.002%
38	6.487	1692	1694	1697	rBV	257	137	0.00%	0.001%
39	6.567	1715	1719	1722	rBV3	291	217	0.00%	0.001%
40	6.590	1722	1726	1728	rBV2	200	155	0.00%	0.001%
41	6.670	1749	1751	1756	rVB2	429	280	0.00%	0.001%
42	6.693	1756	1758	1761	rBV2	330	188	0.00%	0.001%
43	6.728	1767	1769	1770	rBV2	303	146	0.00%	0.001%
44	6.760	1777	1779	1783	rVB3	389	264	0.00%	0.001%
45	6.783	1783	1786	1787	rBV2	216	127	0.00%	0.001%
46	6.825	1796	1799	1800	rBV2	153	91	0.00%	0.000%
47	6.873	1811	1814	1816	rBV3	393	264	0.00%	0.001%
48	6.911	1816	1826	1854	rBV	143067	284919	4.73%	1.353%
49	7.243	1917	1929	1969	rBV	631114	1129961	18.76%	5.366%
50	7.554	2017	2026	2050	rBV	102528	190340	3.16%	0.904%
51	7.825	2106	2110	2113	rVB3	514	351	0.01%	0.002%
52	7.860	2116	2121	2123	rBV3	438	418	0.01%	0.002%
53	7.911	2131	2137	2148	rVB7	1969	3084	0.05%	0.015%
54	7.960	2148	2152	2153	rBV2	382	223	0.00%	0.001%
55	7.989	2158	2161	2163	rBV2	266	162	0.00%	0.001%
56	8.024	2163	2172	2211	rBV2	331289	713526	11.84%	3.388%
57	8.577	2342	2344	2345	rBV2	349	104	0.00%	0.000%
58	8.635	2360	2362	2366	rVB2	410	202	0.00%	0.001%
59	8.654	2366	2368	2369	rBV	257	132	0.00%	0.001%
60	8.696	2378	2381	2385	rBV4	638	575	0.01%	0.003%
61	8.808	2396	2416	2457	rBV2	2987464	6024161	100.00%	28.607%
62	9.368	2587	2590	2592	rBV4	335	227	0.00%	0.001%
63	9.387	2594	2596	2598	rBV	557	309	0.01%	0.001%
64	9.452	2614	2616	2619	rBV4	438	239	0.00%	0.001%
65	9.548	2642	2646	2651	rBV4	542	568	0.01%	0.003%
66	9.686	2687	2689	2690	rBV	319	135	0.00%	0.001%
67	9.718	2697	2699	2702	rBV3	233	155	0.00%	0.001%
68	9.860	2739	2743	2747	rBV3	313	313	0.01%	0.001%
69	9.915	2756	2760	2761	rBV2	333	213	0.00%	0.001%
70	9.940	2765	2768	2773	rBV2	496	333	0.01%	0.002%
71	9.969	2773	2777	2779	rBV2	488	370	0.01%	0.002%
72	10.069	2805	2808	2811	rBV3	347	220	0.00%	0.001%
73	10.149	2819	2833	2857	rBV	520283	814303	13.52%	3.867%
74	10.349	2893	2895	2898	rBV	235	128	0.00%	0.001%
75	10.368	2898	2901	2907	rVB5	388	363	0.01%	0.002%
76	10.423	2915	2918	2923	rVB3	317	264	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035310.D
 Acq On : 19 Apr 2024 16:04
 Operator : SY/MD
 Sample : P2157-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.448	2923	2926	2927	rBV	297	163	0.00%	0.001%
78	10.493	2938	2940	2943	rVB2	536	273	0.00%	0.001%
79	10.542	2950	2955	2957	rBV2	400	389	0.01%	0.002%
80	10.632	2981	2983	2985	rBV	268	96	0.00%	0.000%
81	10.677	2992	2997	3000	rBV2	399	370	0.01%	0.002%
82	10.767	3022	3025	3027	rBV	278	174	0.00%	0.001%
83	10.850	3049	3051	3054	rBV2	285	155	0.00%	0.001%
84	10.966	3086	3087	3094	rVB	250	196	0.00%	0.001%
85	10.998	3094	3097	3100	rVB	238	177	0.00%	0.001%
86	11.021	3100	3104	3106	rBV	299	163	0.00%	0.001%
87	11.059	3113	3116	3119	rBV	303	231	0.00%	0.001%
88	11.072	3119	3120	3125	rVB2	315	234	0.00%	0.001%
89	11.120	3125	3135	3145	rBV	80557	130122	2.16%	0.618%
90	11.204	3145	3161	3194	rVB2	1534014	3393960	56.34%	16.117%
91	11.503	3247	3254	3259	rBV6	6559	10351	0.17%	0.049%
92	11.574	3261	3276	3302	rVB2	1479699	3158155	52.42%	14.997%
93	11.892	3371	3375	3377	rBV2	444	382	0.01%	0.002%
94	12.049	3421	3424	3427	rBV2	491	399	0.01%	0.002%
95	12.204	3470	3472	3475	rVB3	666	388	0.01%	0.002%
96	12.336	3510	3513	3514	rBV2	325	185	0.00%	0.001%
97	12.493	3558	3562	3565	rBV2	338	341	0.01%	0.002%
98	12.792	3653	3655	3657	rVB	581	222	0.00%	0.001%
99	13.197	3770	3781	3796	rBV	132764	209437	3.48%	0.995%
100	13.683	3924	3932	3944	rBV3	13064	21414	0.36%	0.102%




Sum of corrected areas: 21058076

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035310.D
Acq On : 19 Apr 2024 16:04
Operator : SY/MD
Sample : P2157-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

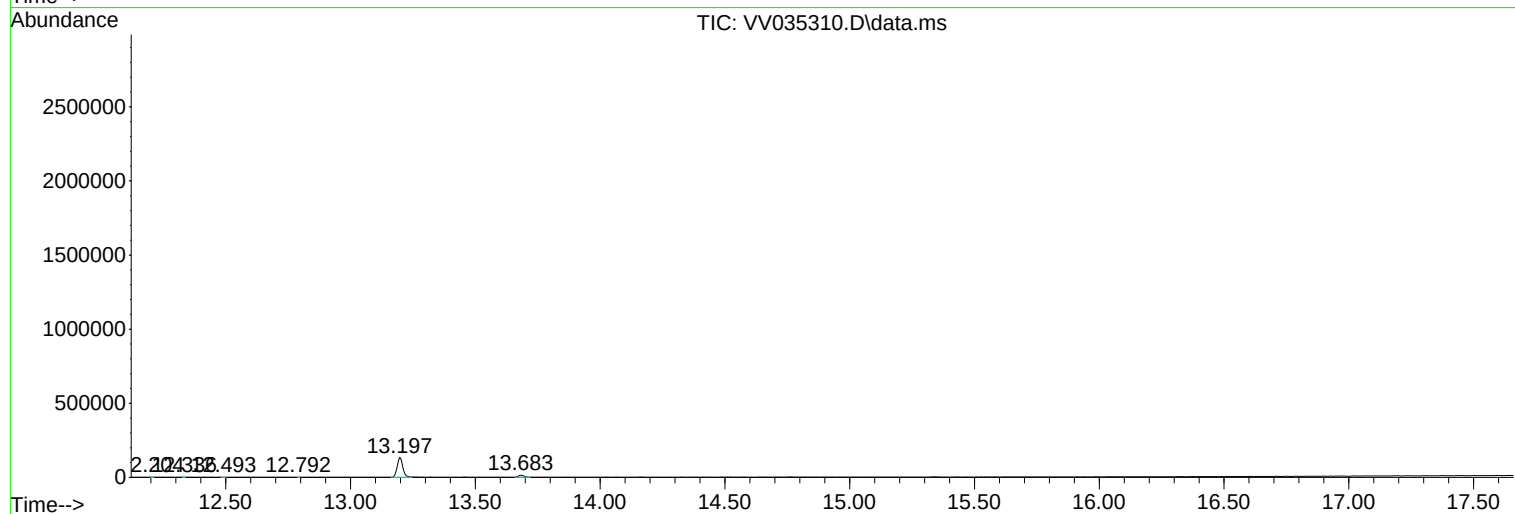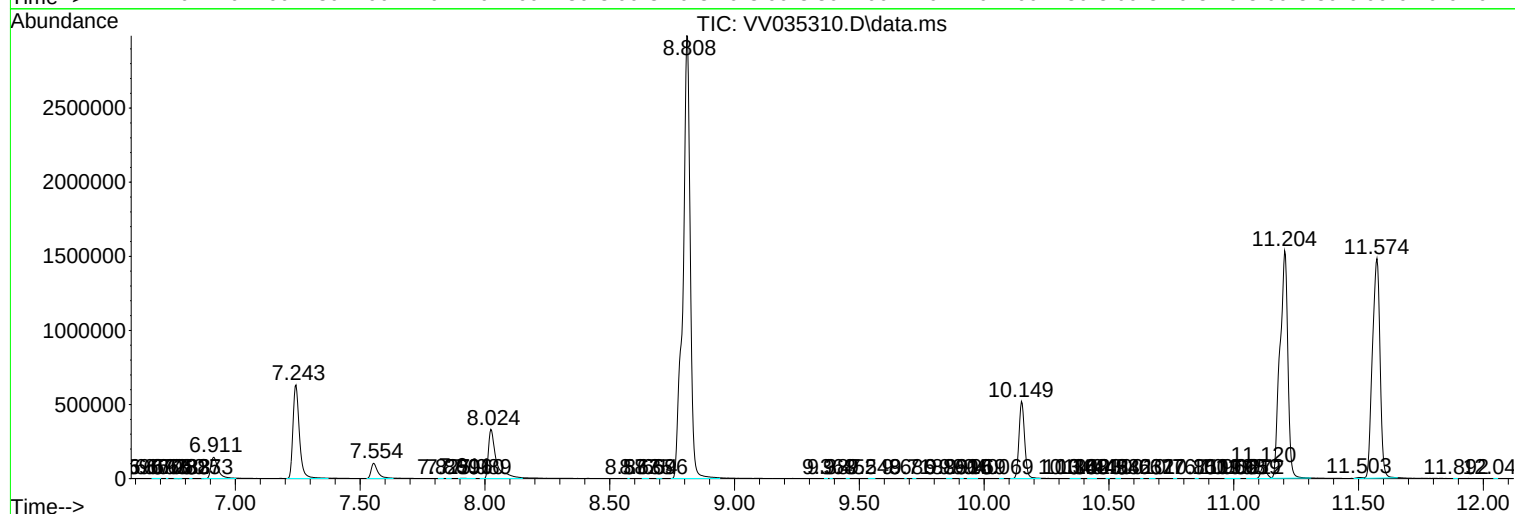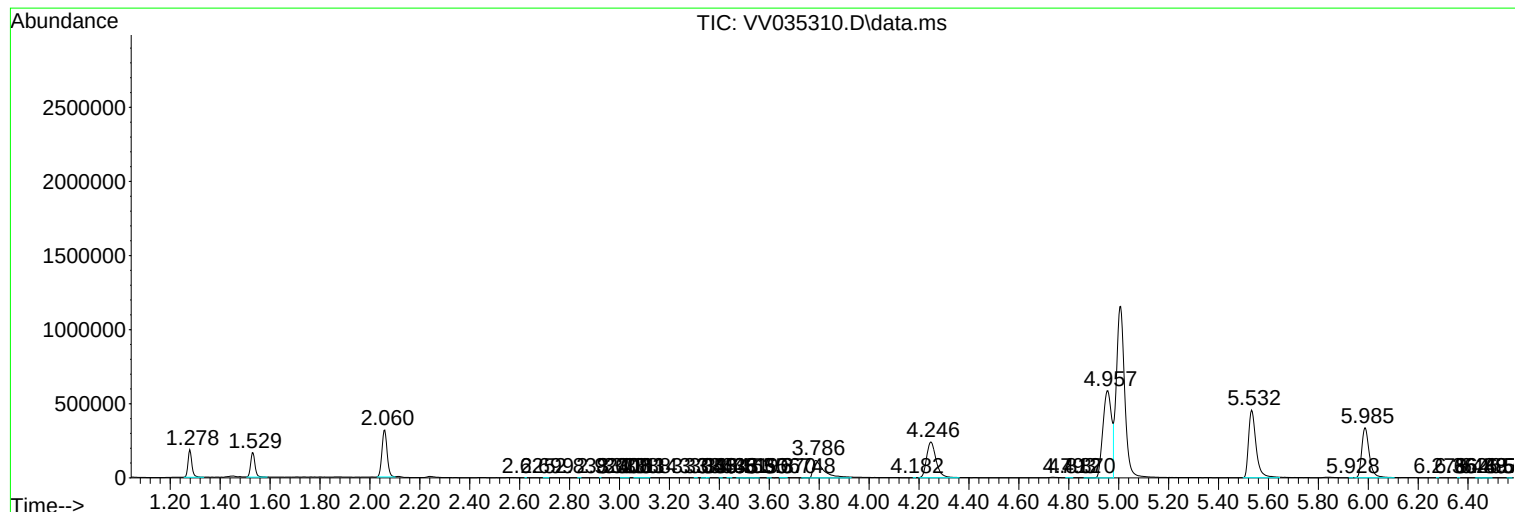

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035310.D
Acq On : 19 Apr 2024 16:04
Operator : SY/MD
Sample : P2157-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035310.D
Acq On : 19 Apr 2024 16:04
Operator : SY/MD
Sample : P2157-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------