

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035311.D
 Acq On : 19 Apr 2024 16:28
 Operator : SY/MD
 Sample : P2157-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	26	rVB	24011	23214	1.22%	0.172%
2	1.191	43	47	51	rBV	7396	6169	0.32%	0.046%
3	1.278	67	74	85	rBV	218968	237037	12.49%	1.757%
4	1.529	147	152	165	rVB	170132	199361	10.50%	1.477%
5	2.060	308	317	333	rVB	319799	463507	24.42%	3.435%
6	2.690	506	513	515	rBV5	2268	2590	0.14%	0.019%
7	2.912	577	582	585	rBV3	559	650	0.03%	0.005%
8	3.249	685	687	689	rVB2	183	71	0.00%	0.001%
9	3.269	691	693	694	rBV2	184	75	0.00%	0.001%
10	3.378	725	727	730	rVB	278	168	0.01%	0.001%
11	3.439	741	746	748	rBV2	369	229	0.01%	0.002%
12	3.449	748	749	752	rVB	222	78	0.00%	0.001%
13	3.474	752	757	761	rBV2	331	321	0.02%	0.002%
14	3.497	761	764	767	rBV2	253	197	0.01%	0.001%
15	3.558	778	783	786	rVB2	171	154	0.01%	0.001%
16	3.577	786	789	791	rBV	354	146	0.01%	0.001%
17	3.590	791	793	795	rVB	238	124	0.01%	0.001%
18	3.613	795	800	801	rBV	216	116	0.01%	0.001%
19	3.670	814	818	820	rBV2	649	347	0.02%	0.003%
20	3.732	835	837	841	rBV	339	239	0.01%	0.002%
21	3.786	845	854	895	rBV	120242	345084	18.18%	2.557%
22	4.246	983	997	1028	rBV	243637	628197	33.09%	4.656%
23	4.760	1156	1157	1160	rBV3	220	90	0.00%	0.001%
24	4.899	1197	1200	1201	rBV2	310	169	0.01%	0.001%
25	4.953	1201	1217	1250	rBV2	581110	1552182	81.77%	11.503%
26	5.381	1348	1350	1353	rBV2	253	157	0.01%	0.001%
27	5.426	1357	1364	1365	rBV4	647	620	0.03%	0.005%
28	5.452	1369	1372	1374	rVB2	331	172	0.01%	0.001%
29	5.532	1386	1397	1427	rBV	453800	953046	50.21%	7.063%
30	5.905	1510	1513	1516	rBV2	386	211	0.01%	0.002%
31	5.989	1526	1539	1566	rBV	345414	721073	37.99%	5.344%
32	6.259	1621	1623	1626	rVB3	761	455	0.02%	0.003%
33	6.285	1626	1631	1635	rBV4	639	704	0.04%	0.005%
34	6.403	1666	1668	1673	rBV4	350	242	0.01%	0.002%
35	6.426	1673	1675	1676	rBV4	253	102	0.01%	0.001%
36	6.567	1716	1719	1721	rBV	354	202	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035311.D
 Acq On : 19 Apr 2024 16:28
 Operator : SY/MD
 Sample : P2157-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.612	1728	1733	1737	rBV3	936	867	0.05%	0.006%
38	6.664	1746	1749	1755	rBV5	480	509	0.03%	0.004%
39	6.703	1759	1761	1762	rBV	272	112	0.01%	0.001%
40	6.731	1765	1770	1773	rVB3	527	502	0.03%	0.004%
41	6.751	1773	1776	1779	rBV2	414	278	0.01%	0.002%
42	6.767	1779	1781	1785	rVB3	220	79	0.00%	0.001%
43	6.783	1785	1786	1788	rBV2	213	91	0.00%	0.001%
44	6.821	1794	1798	1802	rBV2	415	351	0.02%	0.003%
45	6.844	1802	1805	1811	rVB2	297	273	0.01%	0.002%
46	6.876	1811	1815	1816	rBV	367	219	0.01%	0.002%
47	6.912	1816	1826	1855	rBV	147700	291880	15.38%	2.163%
48	7.243	1917	1929	1961	rBV	643619	1147254	60.44%	8.502%
49	7.555	2017	2026	2049	rBV	102339	192848	10.16%	1.429%
50	7.863	2119	2122	2123	rBV	529	329	0.02%	0.002%
51	7.924	2138	2141	2143	rBV	263	183	0.01%	0.001%
52	7.966	2151	2154	2157	rBV2	215	194	0.01%	0.001%
53	8.024	2163	2172	2222	rBV2	345941	753911	39.72%	5.587%
54	8.522	2325	2327	2330	rVB2	556	295	0.02%	0.002%
55	8.564	2338	2340	2342	rBV2	602	255	0.01%	0.002%
56	8.596	2346	2350	2356	rBV3	487	517	0.03%	0.004%
57	8.632	2357	2361	2362	rBV2	362	253	0.01%	0.002%
58	8.783	2397	2408	2438	rBV	736272	1362234	71.76%	10.095%
59	9.014	2477	2480	2484	rVB4	1011	684	0.04%	0.005%
60	9.159	2522	2525	2527	rBV2	267	192	0.01%	0.001%
61	9.188	2531	2534	2535	rBV	348	176	0.01%	0.001%
62	9.233	2543	2548	2550	rBV2	353	316	0.02%	0.002%
63	9.317	2571	2574	2578	rBV2	383	270	0.01%	0.002%
64	9.349	2582	2584	2586	rBV	139	92	0.00%	0.001%
65	9.384	2591	2595	2597	rBV2	397	270	0.01%	0.002%
66	9.403	2599	2601	2603	rVB2	263	85	0.00%	0.001%
67	9.468	2618	2621	2623	rBV2	470	272	0.01%	0.002%
68	9.532	2639	2641	2642	rBV2	384	133	0.01%	0.001%
69	9.603	2660	2663	2664	rBV	122	76	0.00%	0.001%
70	9.677	2681	2686	2692	rBV2	368	439	0.02%	0.003%
71	9.712	2694	2697	2700	rVV3	447	220	0.01%	0.002%
72	9.735	2702	2704	2707	rVB2	502	283	0.01%	0.002%
73	9.786	2718	2720	2724	rVB2	209	105	0.01%	0.001%
74	9.812	2724	2728	2733	rBV2	303	280	0.01%	0.002%
75	9.873	2745	2747	2751	rVB4	384	217	0.01%	0.002%
76	9.892	2751	2753	2757	rBV	244	181	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035311.D
 Acq On : 19 Apr 2024 16:28
 Operator : SY/MD
 Sample : P2157-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.953	2768	2772	2773	rBV	183	132	0.01%	0.001%
78	9.979	2779	2780	2783	rVB	195	88	0.00%	0.001%
79	10.104	2816	2819	2821	rBV	322	162	0.01%	0.001%
80	10.149	2821	2833	2862	rVV	533450	847608	44.65%	6.282%
81	10.471	2930	2933	2934	rBV	310	189	0.01%	0.001%
82	10.493	2938	2940	2951	rVB4	731	805	0.04%	0.006%
83	10.577	2963	2966	2968	rBV3	287	169	0.01%	0.001%
84	10.709	3004	3007	3008	rBV2	349	208	0.01%	0.002%
85	10.783	3028	3030	3035	rBV2	323	256	0.01%	0.002%
86	11.117	3122	3134	3145	rBV	187487	296304	15.61%	2.196%
87	11.185	3145	3155	3191	rVB2	780256	1898297	100.00%	14.068%
88	11.558	3260	3271	3299	rVB	718746	1253666	66.04%	9.291%
89	11.924	3379	3385	3389	rVB5	724	668	0.04%	0.005%
90	11.953	3390	3394	3396	rBV3	626	448	0.02%	0.003%
91	12.033	3417	3419	3422	rBV3	421	248	0.01%	0.002%
92	12.056	3422	3426	3428	rBV3	615	476	0.03%	0.004%
93	12.127	3445	3448	3452	rBV3	414	386	0.02%	0.003%
94	12.413	3532	3537	3539	rBV2	480	412	0.02%	0.003%
95	12.529	3562	3573	3581	rBV7	3908	7423	0.39%	0.055%
96	12.583	3584	3590	3602	rVB4	7275	11722	0.62%	0.087%
97	12.918	3691	3694	3695	rBV	316	173	0.01%	0.001%
98	13.197	3770	3781	3797	rBV2	150636	240688	12.68%	1.784%
99	13.307	3813	3815	3819	rBV3	599	257	0.01%	0.002%
100	13.683	3922	3932	3946	rVB3	22850	37566	1.98%	0.278%




Sum of corrected areas: 13493575

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035311.D
Acq On : 19 Apr 2024 16:28
Operator : SY/MD
Sample : P2157-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

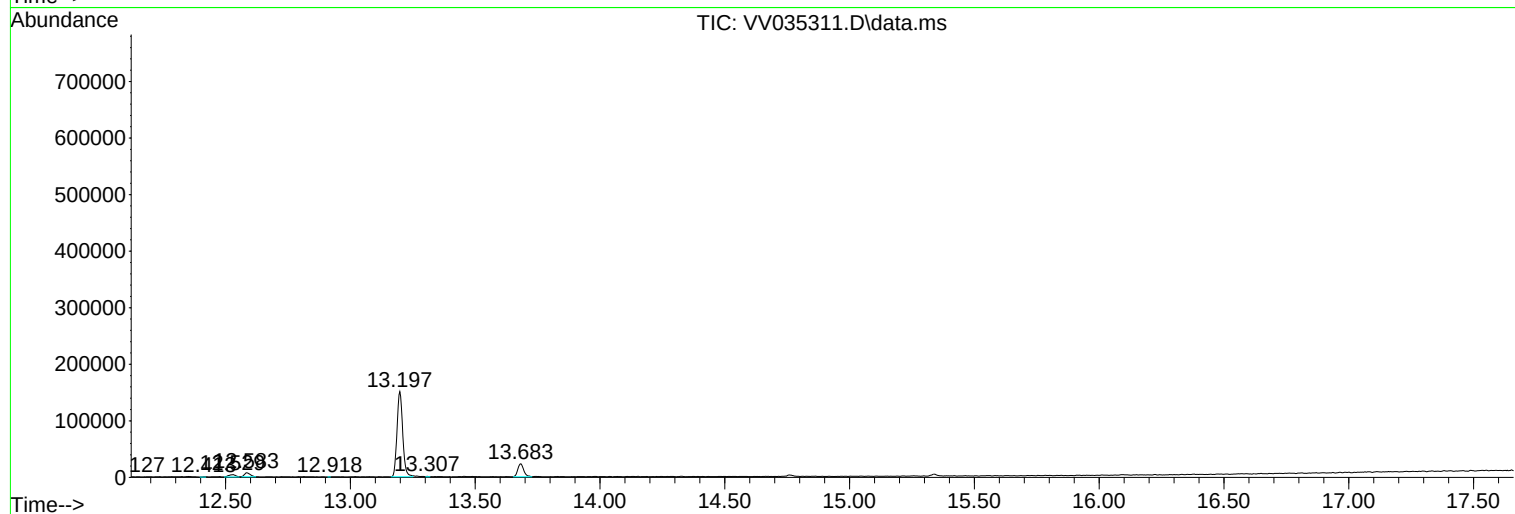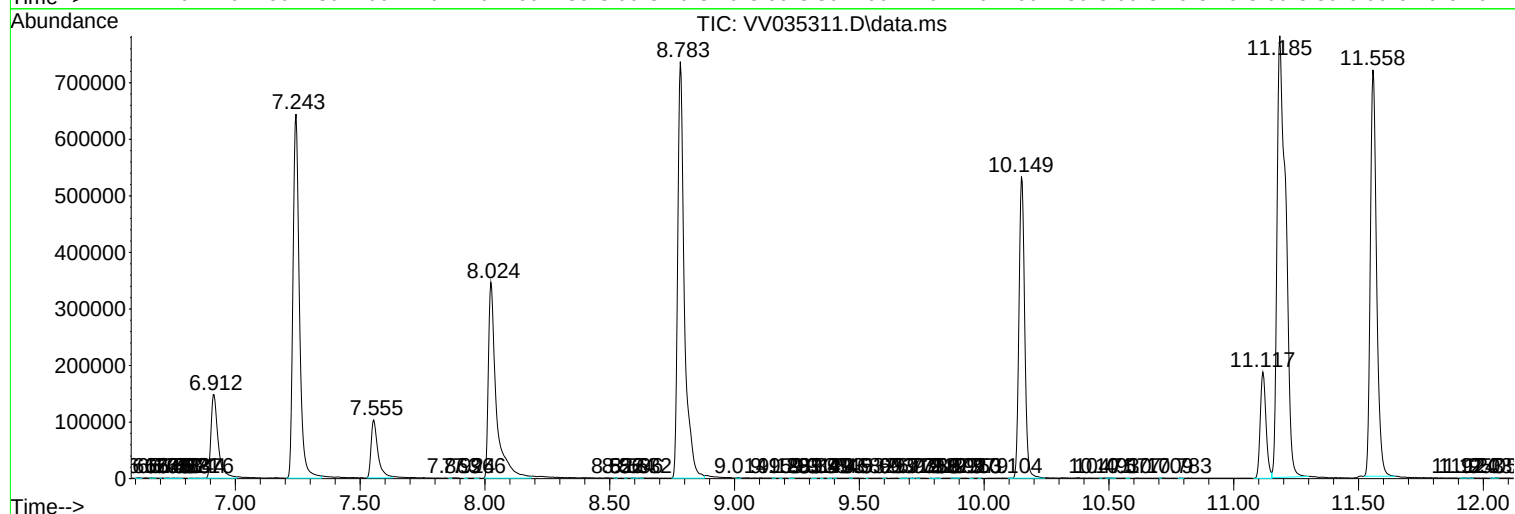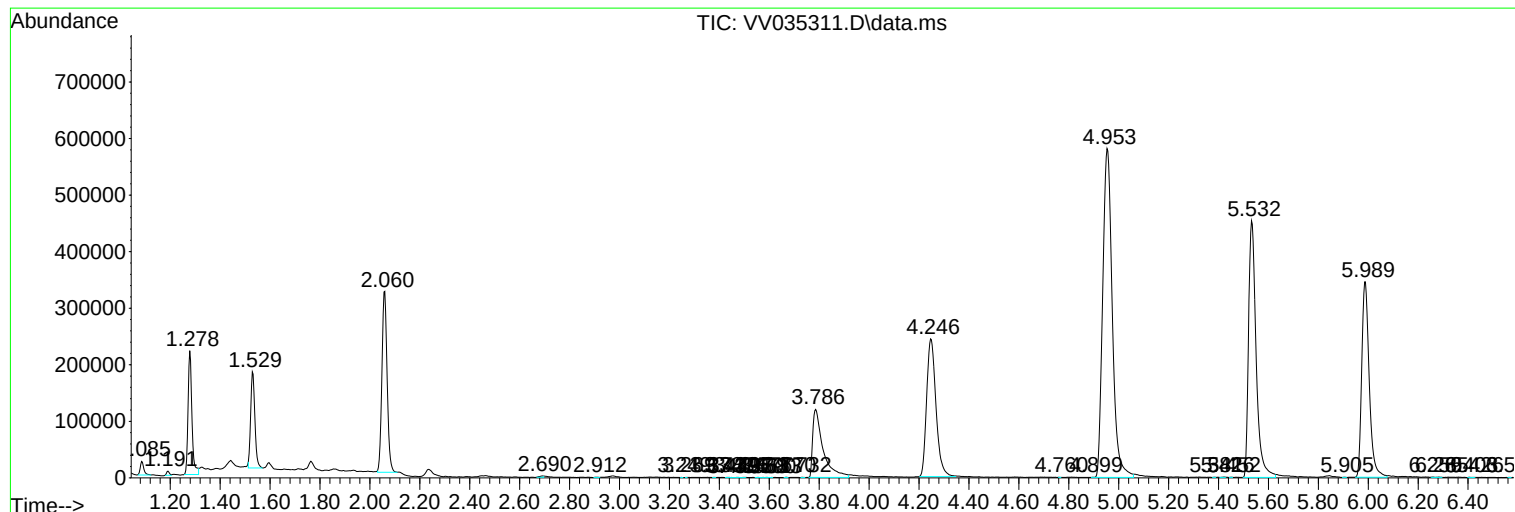

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035311.D
Acq On : 19 Apr 2024 16:28
Operator : SY/MD
Sample : P2157-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035311.D
Acq On : 19 Apr 2024 16:28
Operator : SY/MD
Sample : P2157-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------