

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035314.D
 Acq On : 19 Apr 2024 17:37
 Operator : SY/MD
 Sample : P2157-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	59	rBV4	1917	2259	0.03%	0.009%
2	1.278	67	74	88	rBV	187207	200145	2.94%	0.783%
3	1.532	145	153	172	rVB	178224	211235	3.10%	0.827%
4	2.060	307	317	332	rBV	315821	459458	6.75%	1.799%
5	2.253	368	377	378	rBV4	1958	2408	0.04%	0.009%
6	2.410	424	426	430	rVB3	584	352	0.01%	0.001%
7	2.445	430	437	447	rBV6	2097	3853	0.06%	0.015%
8	2.519	457	460	465	rVB3	635	419	0.01%	0.002%
9	2.552	465	470	474	rBV2	766	760	0.01%	0.003%
10	2.600	482	485	487	rVB2	429	286	0.00%	0.001%
11	2.703	515	517	524	rVB3	454	411	0.01%	0.002%
12	3.117	638	646	653	rBV5	1306	1855	0.03%	0.007%
13	3.214	672	676	680	rBV3	402	382	0.01%	0.001%
14	3.571	783	787	788	rBV	413	241	0.00%	0.001%
15	3.696	824	826	831	rVB3	444	261	0.00%	0.001%
16	3.789	847	855	894	rBV	113992	350119	5.14%	1.371%
17	4.143	962	965	971	rVB3	564	490	0.01%	0.002%
18	4.249	981	998	1029	rBV	241228	633930	9.31%	2.482%
19	4.523	1080	1083	1085	rBV2	475	308	0.00%	0.001%
20	4.568	1093	1097	1100	rVB3	837	477	0.01%	0.002%
21	4.635	1114	1118	1122	rVB2	520	467	0.01%	0.002%
22	4.661	1122	1126	1129	rBV3	293	268	0.00%	0.001%
23	4.738	1139	1150	1162	rVB7	2396	5207	0.08%	0.020%
24	4.789	1162	1166	1167	rBV2	550	350	0.01%	0.001%
25	4.902	1199	1201	1202	rBV	491	271	0.00%	0.001%
26	4.957	1202	1218	1224	rVV2	600100	1407281	20.67%	5.509%
27	5.005	1226	1233	1272	rVB	1374083	3036897	44.61%	11.888%
28	5.433	1363	1366	1371	rVB4	929	770	0.01%	0.003%
29	5.455	1371	1373	1378	rBV3	426	260	0.00%	0.001%
30	5.490	1381	1384	1386	rBV2	584	363	0.01%	0.001%
31	5.532	1386	1397	1435	rBV	459948	965936	14.19%	3.781%
32	5.838	1482	1492	1508	rVB8	4716	11047	0.16%	0.043%
33	5.989	1522	1539	1564	rBV	339115	718136	10.55%	2.811%
34	6.143	1583	1587	1590	rBV4	901	767	0.01%	0.003%
35	6.359	1652	1654	1657	rBV2	487	344	0.01%	0.001%
36	6.381	1659	1661	1665	rVV3	308	306	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041924\
 Data File : VW035314.D
 Acq On : 19 Apr 2024 17:37
 Operator : SY/MD
 Sample : P2157-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.426	1669	1675	1678	rVV3	605	450	0.01%	0.002%
38	6.445	1678	1681	1684	rVV2	286	242	0.00%	0.001%
39	6.613	1729	1733	1735	rBV3	421	369	0.01%	0.001%
40	6.632	1735	1739	1743	rVV3	349	358	0.01%	0.001%
41	6.786	1783	1787	1792	rBV2	387	383	0.01%	0.001%
42	6.915	1814	1827	1859	rBV	145992	293734	4.32%	1.150%
43	7.159	1896	1903	1906	rBV6	785	951	0.01%	0.004%
44	7.175	1906	1908	1912	rVB3	630	363	0.01%	0.001%
45	7.243	1917	1929	1955	rBV	637227	1141617	16.77%	4.469%
46	7.555	2014	2026	2052	rBV	102994	197696	2.90%	0.774%
47	7.757	2087	2089	2092	rBV3	555	245	0.00%	0.001%
48	7.786	2095	2098	2107	rVB5	893	1045	0.02%	0.004%
49	7.838	2107	2114	2117	rBV2	385	372	0.01%	0.001%
50	7.886	2127	2129	2132	rVB2	539	296	0.00%	0.001%
51	7.908	2132	2136	2139	rBV2	1007	840	0.01%	0.003%
52	8.024	2163	2172	2216	rBV2	340133	744972	10.94%	2.916%
53	8.391	2282	2286	2291	rVV6	631	599	0.01%	0.002%
54	8.645	2363	2365	2369	rBV3	363	269	0.00%	0.001%
55	8.809	2396	2416	2459	rBV2	3511745	6807077	100.00%	26.647%
56	9.021	2480	2482	2485	rBV4	671	388	0.01%	0.002%
57	9.127	2513	2515	2518	rVB	584	333	0.00%	0.001%
58	9.429	2603	2609	2611	rVB4	593	491	0.01%	0.002%
59	9.445	2611	2614	2618	rVB3	461	386	0.01%	0.002%
60	9.474	2618	2623	2624	rBV	419	323	0.00%	0.001%
61	9.812	2724	2728	2731	rBV3	280	278	0.00%	0.001%
62	9.902	2752	2756	2757	rBV2	440	300	0.00%	0.001%
63	9.973	2774	2778	2783	rBV2	376	382	0.01%	0.001%
64	10.149	2821	2833	2854	rBV	529616	832185	12.23%	3.258%
65	10.365	2897	2900	2903	rVB3	509	336	0.00%	0.001%
66	10.690	2996	3001	3004	rBV2	301	281	0.00%	0.001%
67	10.709	3004	3007	3011	rVB3	480	363	0.01%	0.001%
68	10.953	3079	3083	3086	rBV2	263	252	0.00%	0.001%
69	11.117	3124	3134	3145	rBV	159702	252535	3.71%	0.989%
70	11.204	3145	3161	3189	rVB2	1205290	2890556	42.46%	11.315%
71	11.445	3234	3236	3238	rBV	423	241	0.00%	0.001%
72	11.493	3242	3251	3260	rBV4	17320	36214	0.53%	0.142%
73	11.574	3260	3276	3301	rVB2	1506034	3256825	47.84%	12.749%
74	11.860	3363	3365	3367	rVB3	598	276	0.00%	0.001%
75	11.918	3381	3383	3387	rVB4	517	322	0.00%	0.001%
76	11.947	3389	3392	3396	rBV2	708	437	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035314.D
 Acq On : 19 Apr 2024 17:37
 Operator : SY/MD
 Sample : P2157-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.050	3421	3424	3430	rVB5	887	686	0.01%	0.003%
78	12.336	3505	3513	3514	rBV3	3603	3070	0.05%	0.012%
79	12.525	3568	3572	3577	rVB3	1544	1434	0.02%	0.006%
80	12.590	3585	3592	3601	rBV4	2761	4200	0.06%	0.016%
81	12.689	3615	3623	3633	rBV7	2437	4576	0.07%	0.018%
82	12.821	3661	3664	3668	rBV3	523	439	0.01%	0.002%
83	12.876	3677	3681	3683	rBV2	334	282	0.00%	0.001%
84	12.998	3716	3719	3723	rBV2	233	274	0.00%	0.001%
85	13.088	3745	3747	3751	rBV	381	334	0.00%	0.001%
86	13.194	3769	3780	3813	rBV	501767	783891	11.52%	3.069%
87	13.358	3828	3831	3836	rVB6	487	350	0.01%	0.001%
88	13.445	3853	3858	3860	rBV4	808	715	0.01%	0.003%
89	13.458	3860	3862	3864	rVV2	521	245	0.00%	0.001%
90	13.525	3880	3883	3885	rBV2	610	340	0.00%	0.001%
91	13.561	3892	3894	3898	rVB3	521	252	0.00%	0.001%
92	13.680	3919	3931	3950	rBV	141484	229003	3.36%	0.896%
93	13.969	4019	4021	4025	rBV2	481	289	0.00%	0.001%
94	13.995	4025	4029	4033	rVB4	578	451	0.01%	0.002%
95	14.368	4142	4145	4152	rBV4	499	586	0.01%	0.002%
96	14.461	4172	4174	4178	rBV3	493	475	0.01%	0.002%
97	14.660	4233	4236	4241	rBV3	587	519	0.01%	0.002%
98	14.734	4254	4259	4262	rBV5	2981	3327	0.05%	0.013%
99	14.857	4293	4297	4300	rBV5	575	549	0.01%	0.002%
100	15.332	4436	4445	4457	rBV2	15428	25475	0.37%	0.100%




Sum of corrected areas: 25545663

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035314.D
Acq On : 19 Apr 2024 17:37
Operator : SY/MD
Sample : P2157-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

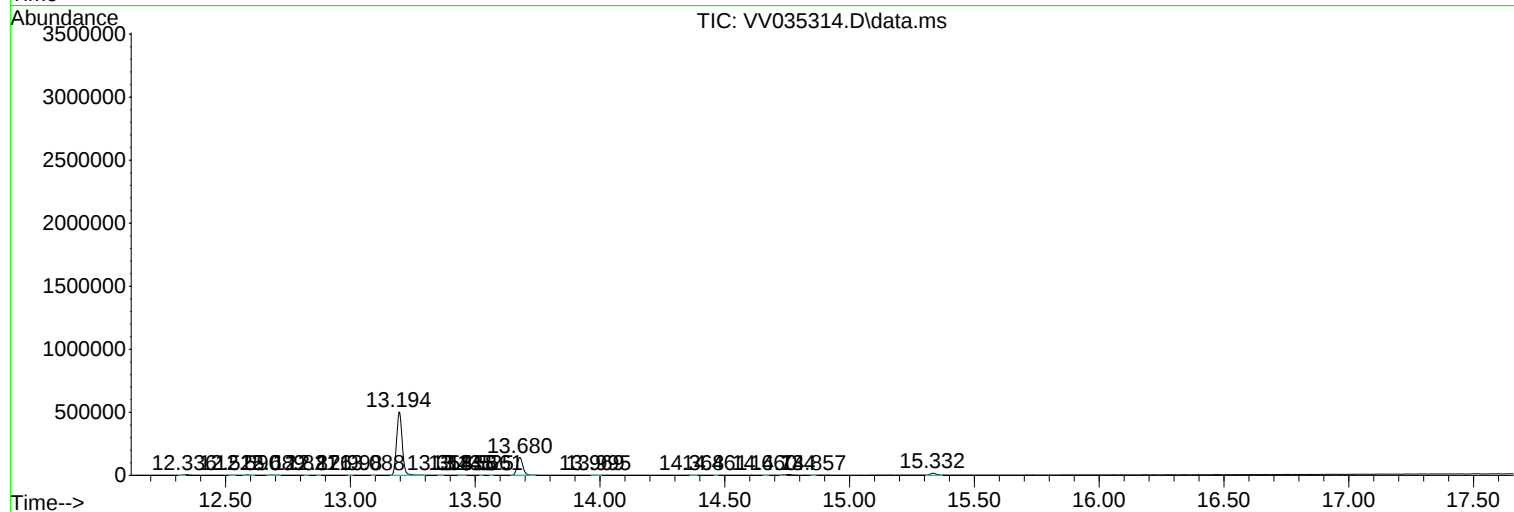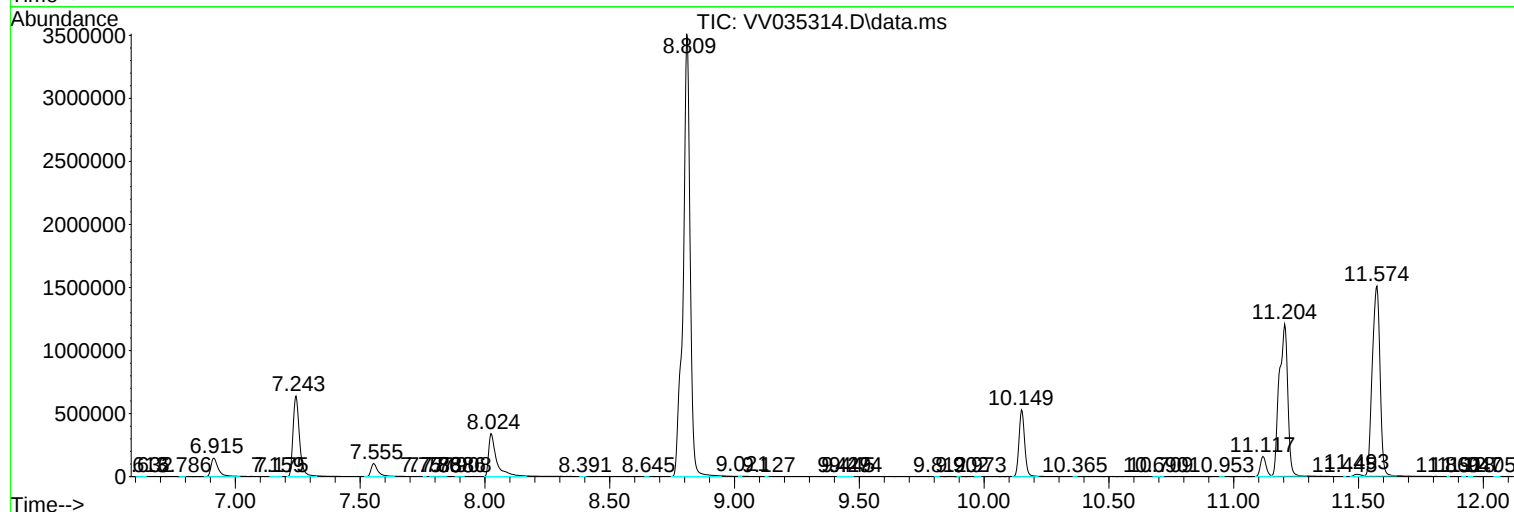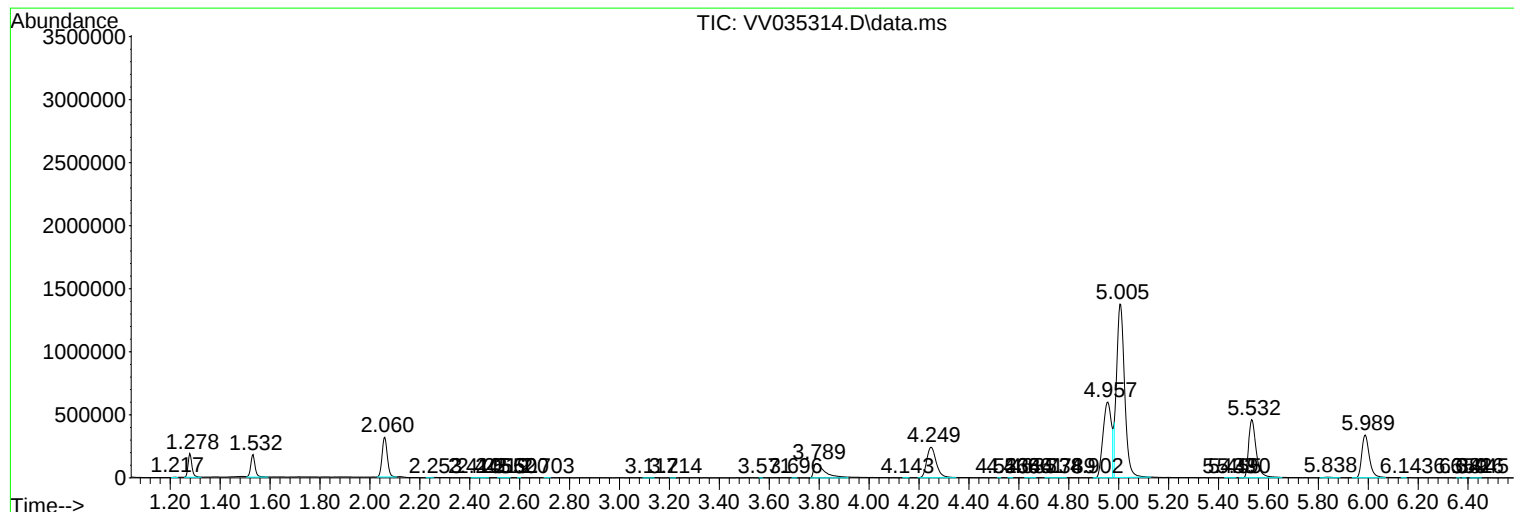

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035314.D
Acq On : 19 Apr 2024 17:37
Operator : SY/MD
Sample : P2157-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035314.D
Acq On : 19 Apr 2024 17:37
Operator : SY/MD
Sample : P2157-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc